

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090119\
 Data File : VV012512.D
 Acq On : 01 Sep 2019 16:13
 Operator : SY/MD
 Sample : K4605-04DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090119WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.319	66	71	86	rVB	160751	161986	13.93%	1.539%
2	1.585	148	154	164	rVB	173446	192564	16.56%	1.829%
3	2.132	315	324	335	rBV	353125	494661	42.53%	4.699%
4	2.457	422	425	428	rBV4	2750	2528	0.22%	0.024%
5	2.675	490	493	496	rBV4	1246	888	0.08%	0.008%
6	2.868	551	553	556	rBV3	1570	722	0.06%	0.007%
7	3.167	644	646	650	rBV5	1236	611	0.05%	0.006%
8	3.309	688	690	698	rVB8	1926	1511	0.13%	0.014%
9	3.367	705	708	709	rBV2	1218	725	0.06%	0.007%
10	3.412	720	722	726	rBV4	1306	663	0.06%	0.006%
11	3.544	759	763	765	rBV4	2328	1796	0.15%	0.017%
12	3.605	779	782	784	rBV3	2069	1583	0.14%	0.015%
13	3.643	791	794	796	rBV4	1291	791	0.07%	0.008%
14	3.666	796	801	803	rBV5	1448	1376	0.12%	0.013%
15	3.708	811	814	818	rBV6	1552	1315	0.11%	0.012%
16	3.772	831	834	838	rBV4	1268	928	0.08%	0.009%
17	3.804	841	844	845	rBV3	2256	1111	0.10%	0.011%
18	3.839	853	855	858	rBV5	1146	607	0.05%	0.006%
19	3.942	875	887	915	rBV3	100219	350475	30.14%	3.329%
20	4.402	1017	1030	1050	rVB	205158	493546	42.44%	4.688%
21	4.971	1204	1207	1209	rBV4	2259	1445	0.12%	0.014%
22	4.987	1209	1212	1215	rVV5	1758	1419	0.12%	0.013%
23	5.029	1222	1225	1226	rBV2	1366	783	0.07%	0.007%
24	5.097	1229	1246	1265	rVV2	458913	1162994	100.00%	11.047%
25	5.662	1410	1422	1450	rBV	403635	805721	69.28%	7.653%
26	5.961	1500	1515	1532	rBV2	293761	597478	51.37%	5.675%
27	6.116	1551	1563	1581	rBV	288762	588007	50.56%	5.585%
28	6.482	1674	1677	1680	rBV5	1781	994	0.09%	0.009%
29	6.563	1700	1702	1704	rBV3	1262	714	0.06%	0.007%
30	6.907	1806	1809	1812	rBV4	2647	1395	0.12%	0.013%
31	6.955	1822	1824	1827	rVB4	2603	1202	0.10%	0.011%
32	7.029	1833	1847	1866	rBV	144476	270143	23.23%	2.566%
33	7.360	1938	1950	1967	rBV	503761	880706	75.73%	8.366%
34	7.611	2024	2028	2033	rBV8	2174	2686	0.23%	0.026%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090119\
 Data File : VV012512.D
 Acq On : 01 Sep 2019 16:13
 Operator : SY/MD
 Sample : K4605-04DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090119WMA.M
 Title : VOC Analysis

35	7.662	2033	2044	2059	rBV	101055	180682	15.54%	1.716%
36	7.903	2116	2119	2121	rBV3	1666	826	0.07%	0.008%
37	7.916	2121	2123	2126	rVB4	1917	970	0.08%	0.009%
38	7.942	2129	2131	2136	rVB5	2556	1967	0.17%	0.019%
39	7.968	2136	2139	2140	rBV3	1662	952	0.08%	0.009%
40	8.019	2144	2155	2169	rVV	173239	295931	25.45%	2.811%
41	8.138	2181	2192	2217	rBV2	278541	606269	52.13%	5.759%
42	8.550	2315	2320	2321	rBV5	3038	2006	0.17%	0.019%
43	8.637	2345	2347	2351	rVB5	1697	685	0.06%	0.007%
44	8.894	2416	2427	2461	rBV	618414	1035063	89.00%	9.832%
45	9.167	2508	2512	2515	rBV5	1620	1524	0.13%	0.014%
46	9.456	2600	2602	2605	rBV3	1323	1099	0.09%	0.010%
47	9.569	2633	2637	2641	rBV5	1811	1644	0.14%	0.016%
48	9.746	2686	2692	2696	rBV8	2184	3204	0.28%	0.030%
49	10.000	2769	2771	2774	rBV4	1328	871	0.07%	0.008%
50	10.260	2840	2852	2866	rBV	375601	609241	52.39%	5.787%
51	10.527	2932	2935	2937	rVB3	1445	723	0.06%	0.007%
52	10.540	2937	2939	2945	rBV8	1978	1490	0.13%	0.014%
53	10.772	3008	3011	3016	rVB6	1215	959	0.08%	0.009%
54	10.794	3016	3018	3020	rVB3	2219	843	0.07%	0.008%
55	10.826	3020	3028	3032	rBV8	2092	3219	0.28%	0.031%
56	10.884	3042	3046	3047	rBV4	1453	988	0.08%	0.009%
57	11.006	3082	3084	3085	rBV2	1427	777	0.07%	0.007%
58	11.058	3098	3100	3104	rBV4	952	844	0.07%	0.008%
59	11.116	3113	3118	3119	rBV4	2225	1493	0.13%	0.014%
60	11.292	3161	3173	3191	rBV	504468	834852	71.78%	7.930%
61	11.588	3262	3265	3270	rVB7	1971	1744	0.15%	0.017%
62	11.669	3278	3290	3311	rBV	510019	853652	73.40%	8.109%
63	12.071	3412	3415	3423	rVB10	2365	2809	0.24%	0.027%
64	12.103	3423	3425	3428	rBV4	1596	1301	0.11%	0.012%
65	12.144	3434	3438	3440	rBV4	1337	1258	0.11%	0.012%
66	12.157	3440	3442	3447	rVB4	3115	2281	0.20%	0.022%
67	12.202	3447	3456	3460	rBV9	2495	3984	0.34%	0.038%
68	12.235	3463	3466	3468	rVB4	1487	852	0.07%	0.008%
69	12.472	3538	3540	3543	rVB4	1701	908	0.08%	0.009%
70	12.656	3593	3597	3600	rBV4	1978	1497	0.13%	0.014%
71	12.694	3601	3609	3616	rVV4	3095	5496	0.47%	0.052%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090119\
 Data File : VV012512.D
 Acq On : 01 Sep 2019 16:13
 Operator : SY/MD
 Sample : K4605-04DL 40X
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA3DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090119WMA.M
 Title : VOC Analysis

72	12.730	3618	3620	3623	rBV4	1498	860	0.07%	0.008%
73	12.807	3641	3644	3646	rBV3	1531	1039	0.09%	0.010%
74	12.897	3669	3672	3676	rBV4	1038	1134	0.10%	0.011%
75	13.000	3700	3704	3707	rVB6	1338	968	0.08%	0.009%
76	13.016	3707	3709	3712	rBV3	1491	754	0.06%	0.007%
77	13.148	3747	3750	3752	rBV4	1804	1068	0.09%	0.010%
78	13.202	3763	3767	3771	rBV5	1531	1474	0.13%	0.014%
79	13.263	3784	3786	3791	rBV5	1937	1760	0.15%	0.017%
80	13.302	3796	3798	3799	rBV2	2461	1144	0.10%	0.011%
81	13.353	3811	3814	3818	rBV5	2289	1654	0.14%	0.016%
82	13.460	3845	3847	3849	rBV3	1937	1053	0.09%	0.010%
83	13.736	3930	3933	3936	rBV5	2528	1586	0.14%	0.015%
84	13.861	3965	3972	3973	rBV5	1735	1792	0.15%	0.017%
85	14.238	4085	4089	4091	rBV4	2062	1274	0.11%	0.012%
86	14.254	4091	4094	4096	rBV4	1261	948	0.08%	0.009%
87	14.431	4143	4149	4155	rVB10	1997	2272	0.20%	0.022%
88	14.524	4176	4178	4181	rVB4	1611	795	0.07%	0.008%
89	14.617	4202	4207	4210	rBV6	2183	1931	0.17%	0.018%
90	14.759	4247	4251	4254	rVB5	1866	1431	0.12%	0.014%
91	14.926	4301	4303	4304	rBV2	1403	629	0.05%	0.006%
92	15.035	4334	4337	4338	rBV3	1941	1267	0.11%	0.012%
93	15.080	4347	4351	4353	rBV4	2157	1497	0.13%	0.014%
94	15.132	4363	4367	4371	rVB6	1783	1365	0.12%	0.013%
95	15.151	4371	4373	4375	rBV2	1367	918	0.08%	0.009%
96	15.209	4389	4391	4393	rBV3	1371	864	0.07%	0.008%
97	15.254	4402	4405	4408	rBV5	1928	1567	0.13%	0.015%
98	15.685	4536	4539	4542	rBV5	1925	1477	0.13%	0.014%
99	15.964	4624	4626	4627	rBV3	1725	780	0.07%	0.007%
100	16.164	4686	4688	4691	rBV4	2211	1377	0.12%	0.013%


Sum of corrected areas: 10527656

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090119\
Data File : VV012512.D
Acq On : 01 Sep 2019 16:13
Operator : SY/MD
Sample : K4605-04DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

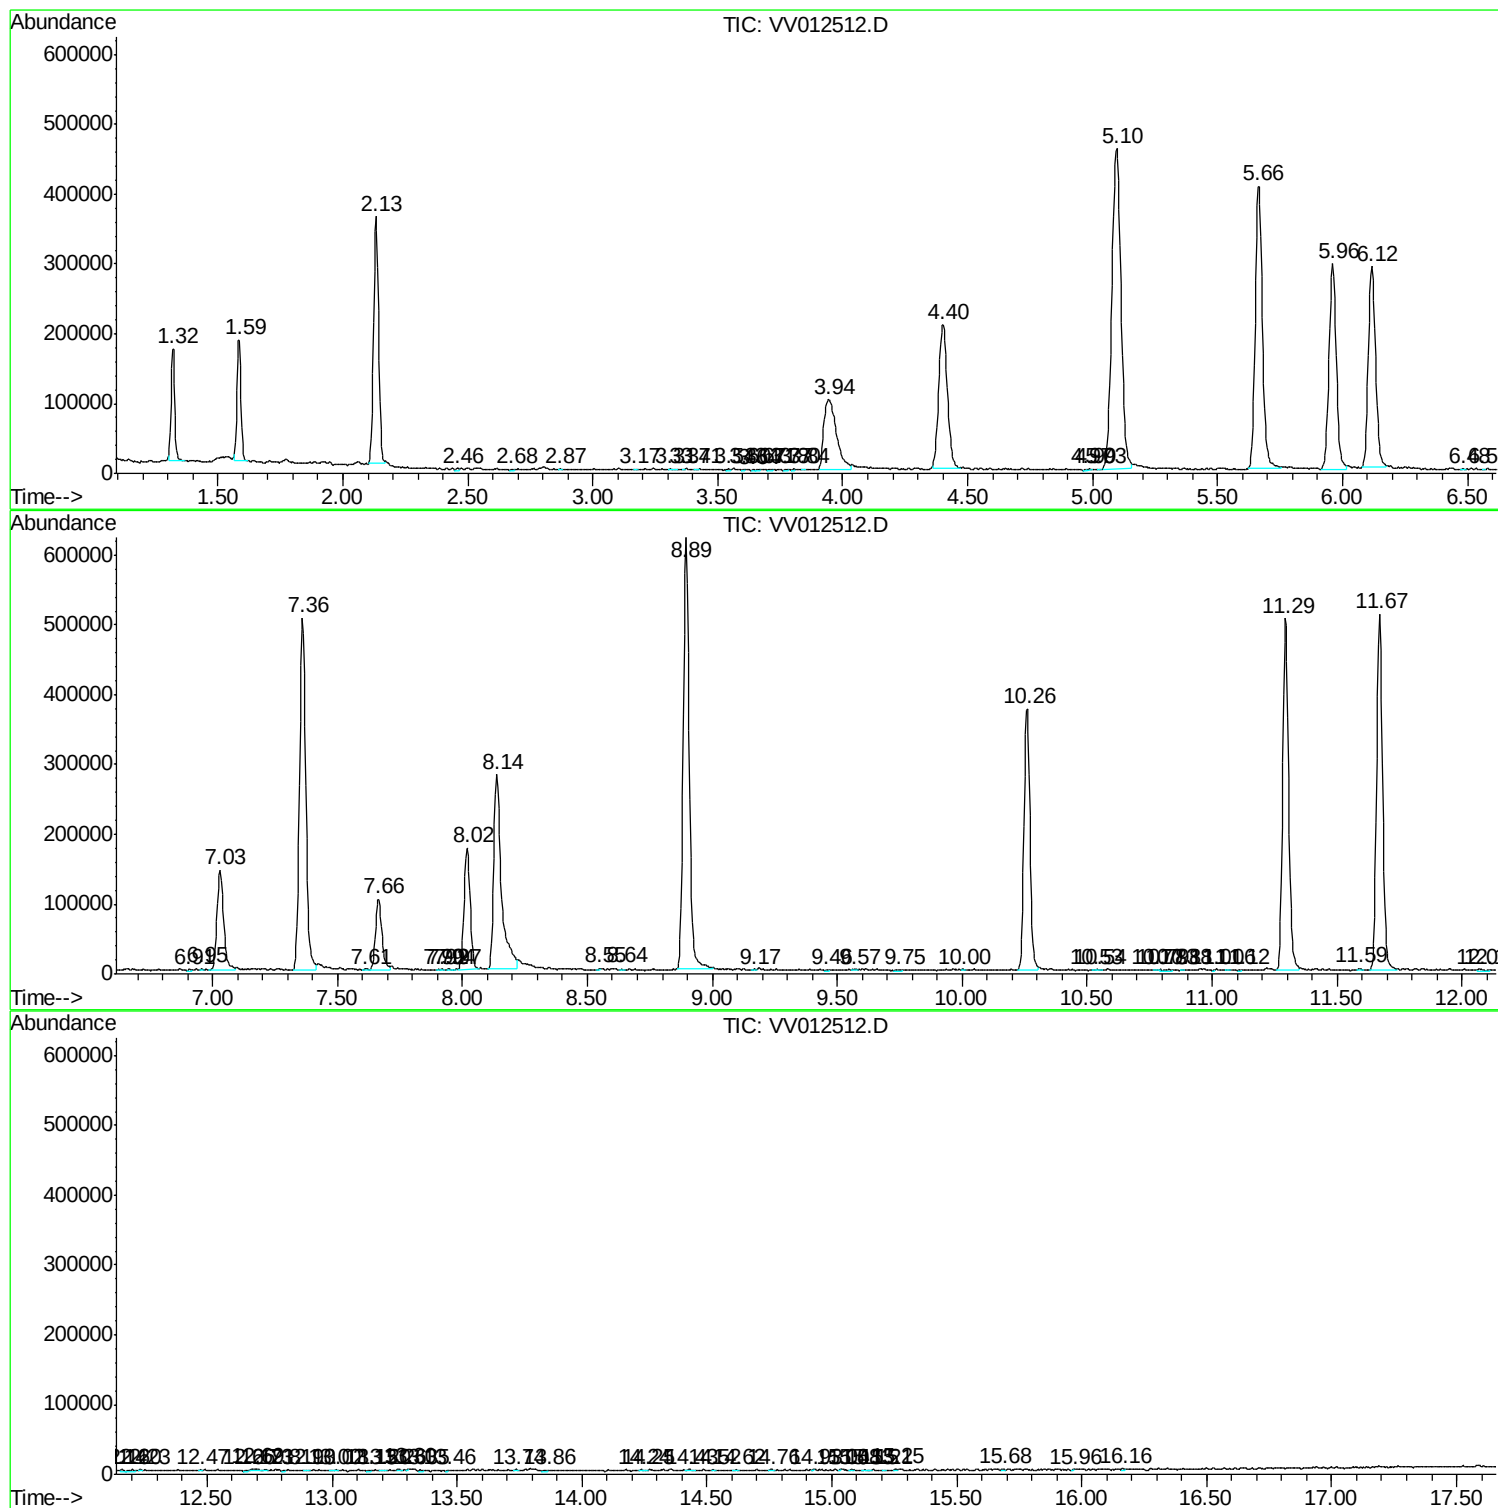

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090119\
Data File : VV012512.D
Acq On : 01 Sep 2019 16:13
Operator : SY/MD
Sample : K4605-04DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090119\
Data File : VV012512.D
Acq On : 01 Sep 2019 16:13
Operator : SY/MD
Sample : K4605-04DL 40X
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA3DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090119WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
