


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090119\
 Data File : VV012501.D
 Acq On : 01 Sep 2019 10:56
 Operator : SY/MD
 Sample : BFB69
 Misc : 5mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB69

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090119WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 04 00:42:16 2019

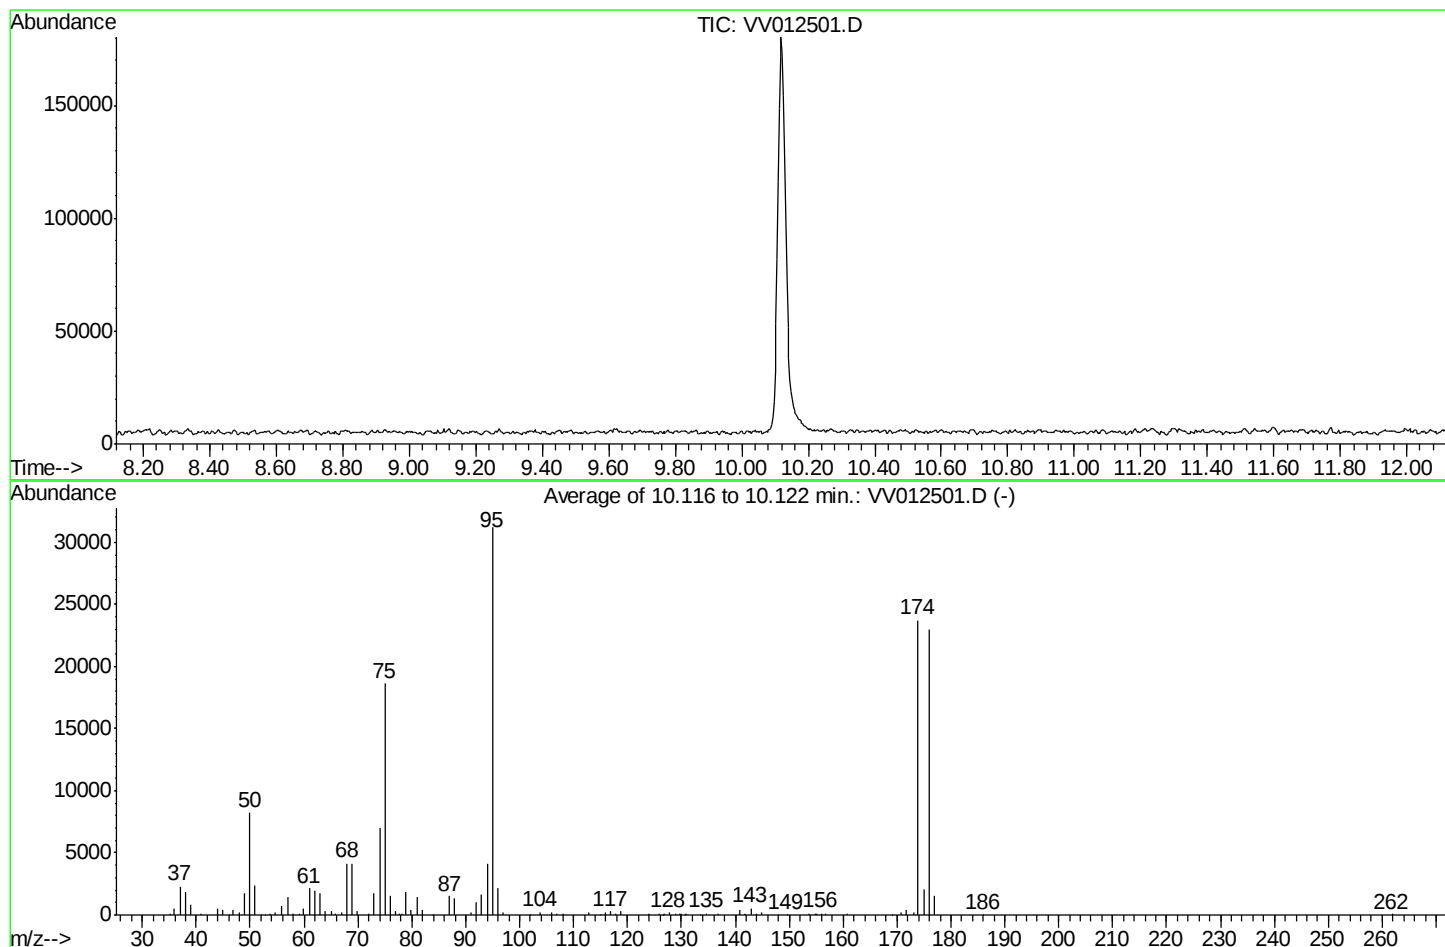

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.3	8211	PASS
75	95	30	80	59.6	18602	PASS
95	95	100	100	100.0	31200	PASS
96	95	5	9	6.9	2152	PASS
173	174	0.00	2	0.8	196	PASS
174	95	50	120	76.1	23730	PASS
175	174	5	9	8.8	2078	PASS
176	174	95	101	97.0	23016	PASS
177	176	5	9	6.6	1517	PASS

m/z	Abundance
35.60	145.0
36.70	215.0
38.10	168.0
40.00	669.0
41.20	110.0
41.70	112.0
42.40	160.0
43.10	131.0
43.80	389.0
45.00	126.0
45.30	119.0
46.20	140.0
47.40	125.0
48.20	113.0
49.50	166.0
50.00	110.0
50.80	107.0
51.30	127.0
52.20	153.0
52.80	119.0
54.10	165.0
57.30	109.0
58.70	132.0
60.50	111.0
62.50	143.0
65.00	105.0
65.60	109.0
66.50	136.0
67.60	132.0
72.10	156.0
74.30	119.0
77.00	106.0
81.10	125.0
83.00	139.0
109.60	107.0
115.10	104.0
117.60	114.0
119.50	112.0
128.40	117.0
189.30	106.0
200.80	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
35.20	168.0
35.90	546.0
37.00	2471.0
38.00	2112.0
39.00	881.0
39.90	599.0
40.70	138.0
41.30	129.0
42.50	135.0
44.00	815.0
45.00	481.0
46.20	209.0
46.90	511.0
48.00	337.0
49.00	1674.0
50.00	8259.0
51.00	2537.0
52.10	168.0
52.90	132.0
53.60	192.0
54.80	205.0
55.90	780.0
57.00	1443.0
58.00	151.0
59.00	127.0
60.00	524.0
61.00	2012.0
62.00	1951.0
63.00	1596.0
64.10	308.0
65.10	423.0
67.10	238.0
68.00	3991.0
69.00	4011.0
69.90	311.0
71.90	256.0
73.00	1976.0
74.00	6979.0
75.00	18616.0
76.00	1575.0
76.90	424.0
77.70	174.0
78.90	1834.0
79.90	381.0
80.90	1562.0
81.90	423.0
83.90	151.0
86.90	1451.0
87.90	1263.0
90.90	261.0
91.90	1126.0
93.00	1746.0
93.90	3895.0
95.00	30376.0
96.00	2214.0
97.00	215.0
103.90	240.0
106.00	179.0
106.90	101.0
112.70	194.0
114.90	128.0
115.90	180.0
116.90	328.0
117.80	225.0
118.80	349.0
125.90	104.0
126.90	114.0
127.70	166.0
128.90	141.0
129.70	130.0
130.60	121.0
131.00	147.0
133.40	108.0
134.80	112.0
140.90	432.0
141.90	144.0
142.90	556.0
144.80	229.0
147.90	134.0
149.60	101.0
154.90	174.0
155.90	138.0
156.80	115.0
169.10	111.0
170.80	150.0
171.70	380.0
173.10	588.0
173.90	22696.0
174.90	2057.0
175.90	21768.0
176.90	1573.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

261.90

130.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
35.20	128.0
35.90	478.0
37.00	2336.0
38.00	2118.0
39.00	843.0
39.90	560.0
40.80	144.0
41.40	161.0
42.40	162.0
43.30	121.0
44.00	898.0
44.90	527.0
46.20	196.0
46.90	461.0
48.10	337.0
49.00	1769.0
50.00	8719.0
51.00	2519.0
52.10	199.0
52.90	151.0
53.70	165.0
54.80	206.0
55.90	759.0
57.00	1519.0
58.10	152.0
59.10	126.0
60.00	559.0
61.00	2219.0
62.00	1975.0
63.00	1747.0
63.90	332.0
65.00	385.0
65.90	119.0
67.10	216.0
68.00	4366.0
69.00	4273.0
69.90	363.0
72.00	295.0
73.00	1827.0
74.00	7278.0
75.00	19120.0
76.00	1518.0
77.00	434.0
78.90	2007.0
79.80	404.0
80.90	1588.0
81.90	473.0
86.90	1518.0
87.90	1375.0
90.90	239.0
91.90	1020.0
92.90	1728.0
94.00	4188.0
95.00	32120.0
96.00	2214.0
97.00	227.0
103.90	207.0
105.90	214.0
106.90	101.0
108.00	109.0
112.70	164.0
115.10	124.0
115.90	190.0
116.90	277.0
117.80	252.0
118.80	303.0
123.90	105.0
126.00	115.0
126.60	124.0
126.80	122.0
127.70	196.0
128.90	164.0
129.70	146.0
130.00	154.0
130.90	146.0
134.70	114.0
136.80	117.0
140.80	418.0
141.70	142.0
142.80	544.0
144.00	117.0
144.80	271.0
153.70	104.0
155.10	180.0
156.00	140.0
156.80	125.0
160.90	133.0
170.80	174.0
171.80	417.0
173.90	24504.0
174.90	2191.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

175.90	23880.0
176.90	1538.0
261.90	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

m/z	Abundance
35.20	109.0
35.90	410.0
37.00	2106.0
38.00	1992.0
39.00	784.0
39.80	569.0
40.80	149.0
41.60	186.0
42.50	170.0
43.30	120.0
44.00	886.0
44.90	567.0
46.10	162.0
46.90	375.0
48.00	344.0
49.00	1682.0
50.00	7987.0
51.00	2409.0
52.10	171.0
53.00	170.0
54.10	154.0
54.70	185.0
55.90	667.0
57.00	1428.0
58.00	130.0
59.10	102.0
59.90	562.0
61.00	2128.0
62.00	1979.0
63.00	1903.0
63.90	379.0
65.00	431.0
65.90	143.0
67.10	165.0
68.00	4141.0
69.00	4073.0
69.90	373.0
72.00	339.0
73.00	1507.0
74.00	6907.0
75.00	18072.0
76.00	1541.0
76.90	339.0
78.10	202.0
78.90	1838.0
79.80	478.0
80.90	1508.0
81.90	452.0
87.00	1527.0
88.00	1487.0
90.90	188.0
91.90	930.0
93.00	1536.0
94.00	4293.0
95.00	31104.0
95.90	2029.0
96.90	215.0
101.90	106.0
103.90	210.0
105.90	226.0
108.10	108.0
112.80	121.0
115.90	196.0
116.90	283.0
117.70	266.0
118.80	211.0
123.80	127.0
126.00	113.0
126.80	126.0
127.80	240.0
128.80	161.0
129.90	185.0
130.80	173.0
134.60	107.0
136.80	161.0
140.80	404.0
141.60	166.0
142.80	563.0
144.00	138.0
144.80	260.0
153.70	122.0
155.10	187.0
156.00	113.0
156.80	103.0
160.80	163.0
170.80	192.0
171.90	512.0
173.90	23992.0
174.90	1986.0
175.90	23400.0
176.90	1440.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69

186.00

142.0

Instrument :
MSVOA_V
ClientSampleId :
BFB69