


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV090120\
 Data File : VV018139.D
 Acq On : 01 Sep 2020 10:00
 Operator : SY/MD
 Sample : BFB85
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB85

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 02 01:43:13 2020

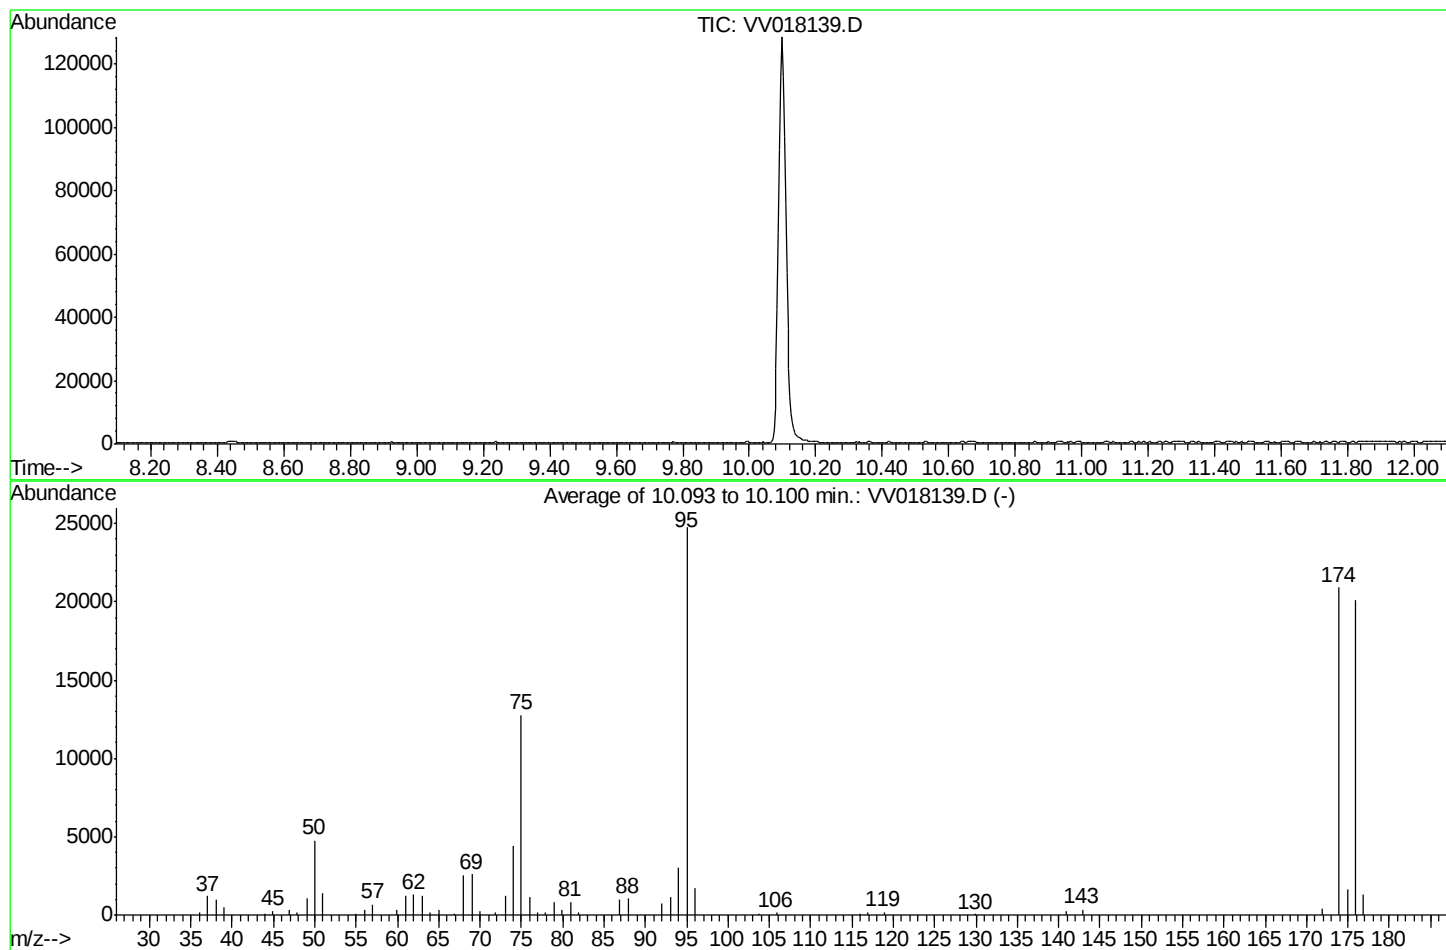

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	4775	PASS
75	95	30	80	51.7	12797	PASS
95	95	100	100	100.0	24762	PASS
96	95	5	9	6.9	1705	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.4	20893	PASS
175	174	5	9	7.9	1647	PASS
176	174	95	101	96.1	20085	PASS
177	176	5	9	6.4	1286	PASS

m/z	Abundance
36.00	199.0
37.00	1111.0
38.00	991.0
39.00	540.0
39.90	181.0
43.90	456.0
45.00	269.0
47.00	342.0
47.90	130.0
49.00	1026.0
50.00	4544.0
51.00	1317.0
56.00	358.0
57.00	658.0
59.90	319.0
61.00	1149.0
62.00	1234.0
63.00	1126.0
64.00	172.0
64.90	289.0
68.00	2448.0
69.00	2540.0
70.00	215.0
71.90	139.0
73.00	1138.0
74.00	4159.0
75.00	11877.0
76.00	1118.0
76.90	155.0
77.80	107.0
78.90	794.0
79.90	291.0
80.90	789.0
81.90	206.0
86.90	941.0
87.90	988.0
92.00	680.0
93.00	1097.0
94.00	2876.0
95.00	23304.0
96.00	1627.0
105.90	133.0
115.90	105.0
117.00	154.0
118.90	165.0
140.80	260.0
142.90	350.0
171.90	358.0
173.90	19048.0
175.00	1473.0
175.90	18520.0
176.90	1200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.00	194.0
37.00	1265.0
38.00	1068.0
39.00	527.0
39.90	168.0
44.00	478.0
45.00	300.0
46.90	337.0
47.90	136.0
49.00	1091.0
50.00	4981.0
51.00	1417.0
54.90	105.0
56.00	383.0
57.00	706.0
60.00	360.0
61.00	1282.0
62.00	1368.0
63.00	1281.0
64.00	171.0
64.90	335.0
66.90	126.0
68.00	2628.0
69.00	2666.0
70.00	228.0
71.90	137.0
73.00	1317.0
74.00	4604.0
75.00	13270.0
76.00	1204.0
76.90	197.0
77.80	130.0
78.90	876.0
79.80	318.0
80.90	840.0
81.90	206.0
86.90	1005.0
87.90	1074.0
92.00	751.0
93.00	1188.0
94.00	3121.0
95.00	25592.0
96.00	1767.0
103.80	121.0
105.90	148.0
115.90	104.0
116.90	175.0
118.90	175.0
130.00	110.0
140.80	293.0
142.90	352.0
171.90	432.0
173.90	21664.0
175.00	1686.0
175.90	20752.0
176.90	1324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

m/z	Abundance
36.00	184.0
37.00	1229.0
38.00	1008.0
39.00	469.0
39.90	176.0
44.00	501.0
44.90	286.0
46.90	304.0
47.80	153.0
49.00	1033.0
50.00	4800.0
51.00	1404.0
54.90	106.0
56.00	353.0
57.00	704.0
60.00	319.0
61.00	1292.0
62.00	1285.0
63.00	1223.0
64.00	158.0
65.00	315.0
66.90	120.0
68.00	2495.0
69.00	2596.0
70.00	224.0
71.90	135.0
73.00	1307.0
74.00	4474.0
75.00	13244.0
76.00	1132.0
76.90	209.0
77.80	156.0
78.90	865.0
79.80	318.0
80.90	832.0
81.90	194.0
86.90	1079.0
87.90	1098.0
92.00	734.0
93.00	1225.0
94.00	3043.0
95.00	25392.0
96.00	1721.0
103.80	137.0
105.90	125.0
116.90	183.0
118.90	180.0
129.90	113.0
140.90	281.0
142.90	353.0
171.90	487.0
173.90	21968.0
174.90	1784.0
175.90	20984.0
176.90	1334.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85

Scan 2790 (10.061 min): VV018139.D
BFB85

m/z	Abundance
40.00	175.0
43.90	432.0

Instrument :
MSVOA_V
ClientSampleId :
BFB85