

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
 Data File : VV022057.D
 Acq On : 01 Sep 2021 10:14
 Operator : SY/MD
 Sample : VV0901MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK247

Quant Time: Sep 02 05:26:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 02 05:24:11 2021
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	358468	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	346481	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	173720	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	134071	54.008	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	108.020%	
7) Chloroethane-d5	1.564	69	105583	54.464	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	108.920%	
11) 1,1-Dichloroethene-d2	2.105	63	175228	42.681	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	85.360%	
21) 2-Butanone-d5	3.873	46	163494	96.032	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	96.030%	
24) Chloroform-d	4.349	84	215345	47.575	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	95.140%	
26) 1,2-Dichloroethane-d4	5.034	65	137543	51.588	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	103.180%	
32) Benzene-d6	5.050	84	478169	50.881	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	101.760%	
36) 1,2-Dichloropropane-d6	6.069	67	148463	50.233	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	100.460%	
41) Toluene-d8	7.317	98	432633	48.768	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	97.540%	
43) trans-1,3-Dichloroprop...	7.622	79	63502	45.143	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	90.280%	
47) 2-Hexanone-d5	8.088	63	99889	88.085	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	88.090%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	176004	46.499	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	93.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	172681	50.563	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	101.120%	
Target Compounds						
25) Chloroform	4.375	83	13899	2.949	ug/L	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
Data File : VV022057.D
Acq On : 01 Sep 2021 10:14
Operator : SY/MD
Sample : VV0901MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Quant Time: Sep 02 05:26:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 02 05:24:11 2021
Response via : Initial Calibration

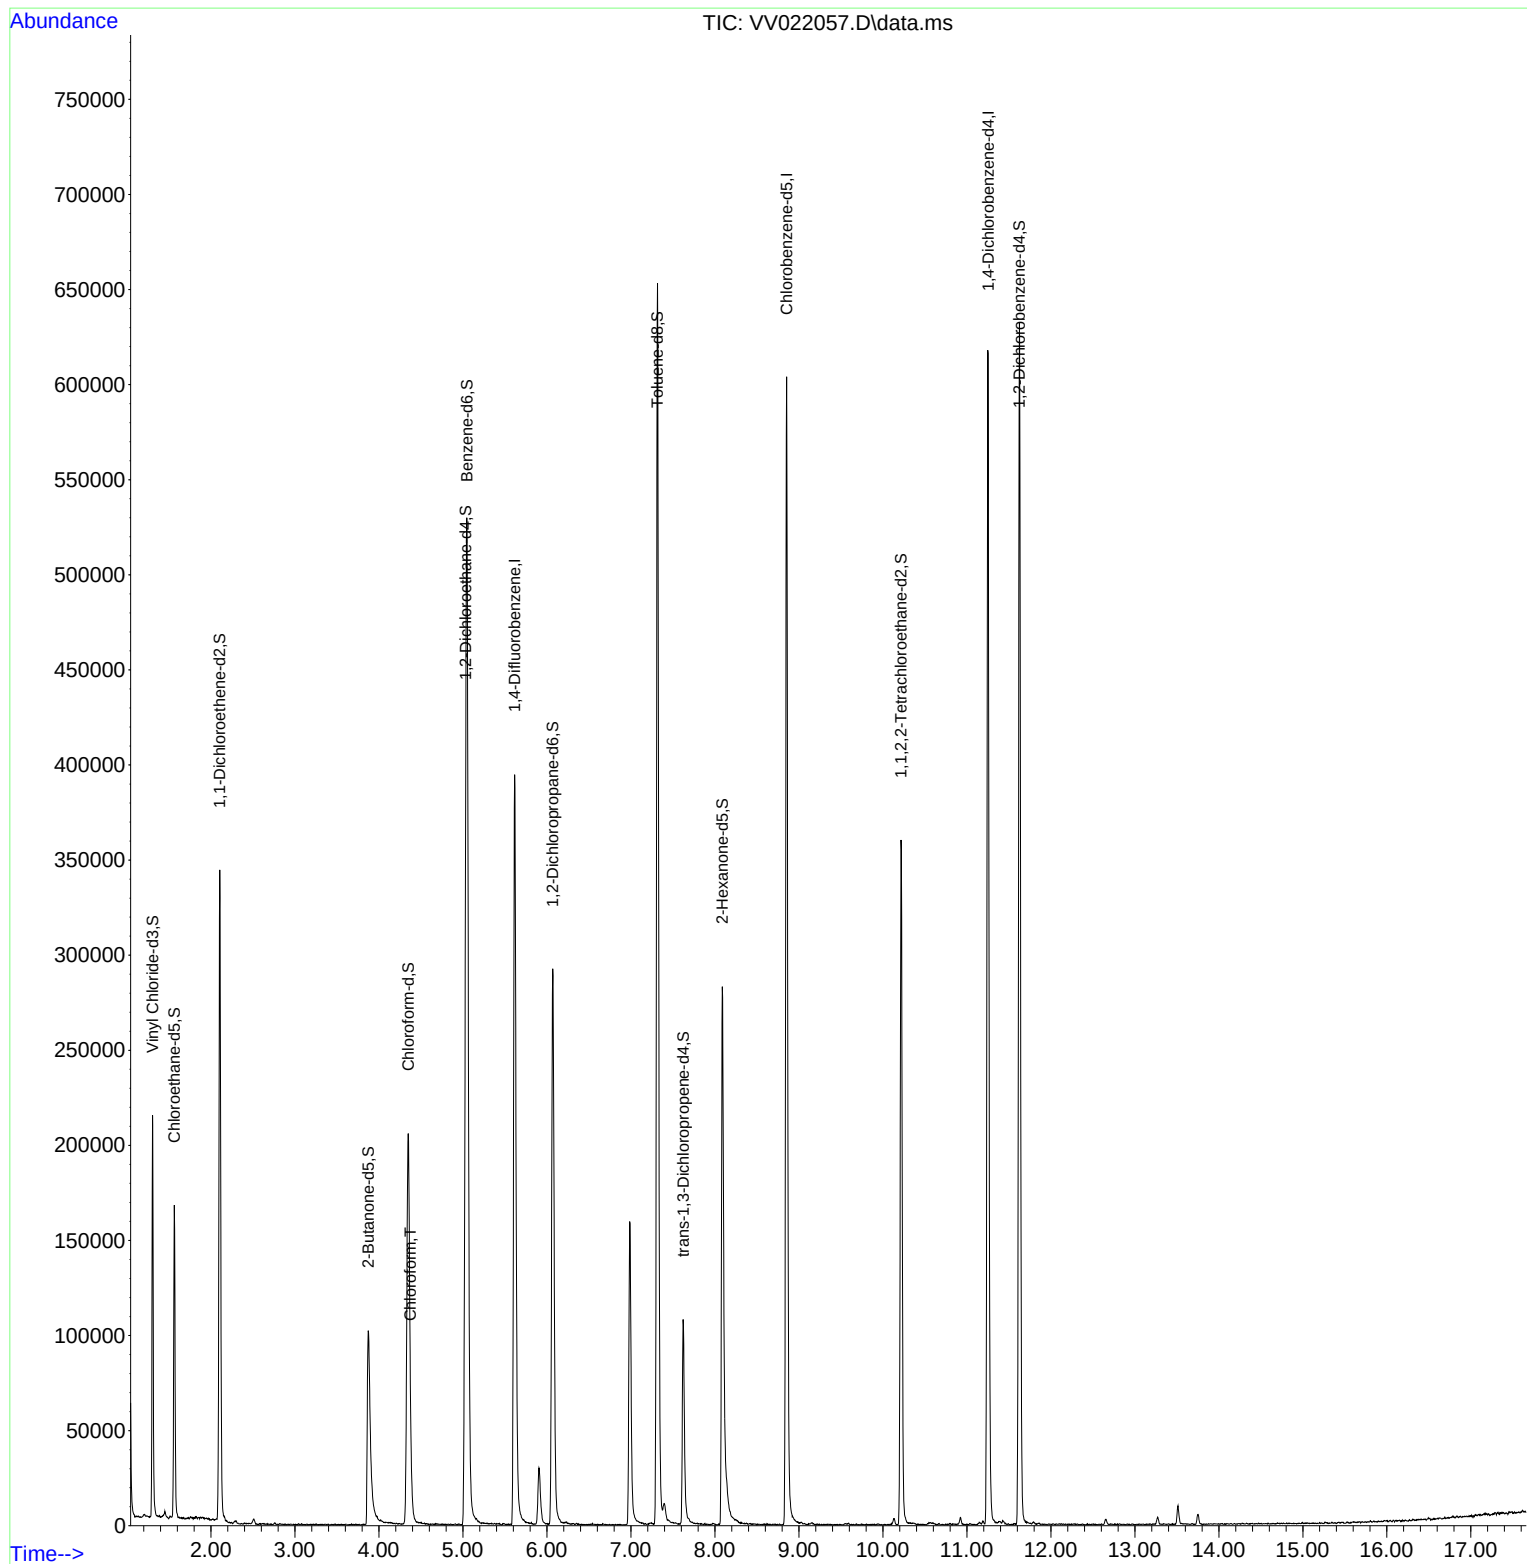

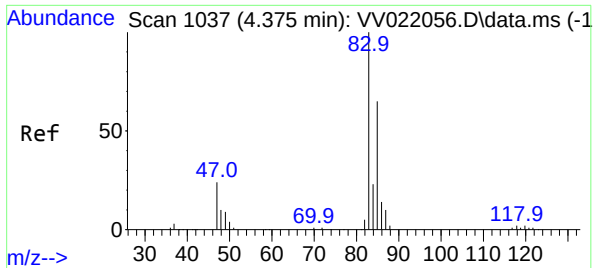

#25
Chloroform
Concen: 2.949 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VV022057.D
Acq: 01 Sep 2021 10:14

Instrument :
MSVOA_V
ClientSampleId :
VBLK247

Tgt Ion: 83 Resp: 13899
Ion Ratio Lower Upper
83 100
85 70.2 46.3 85.9

