

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
 Data File : VV022058.D
 Acq On : 01 Sep 2021 10:39
 Operator : SY/MD
 Sample : VV0901WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK248

Quant Time: Sep 02 05:28:50 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 02 05:24:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	348684	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	337610	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	170590	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	126851	52.533	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	105.060%
7) Chloroethane-d5	1.564	69	102636	54.429	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	108.860%
11) 1,1-Dichloroethene-d2	2.105	63	166710	41.746	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.500%
21) 2-Butanone-d5	3.876	46	166741	100.687	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	100.690%
24) Chloroform-d	4.349	84	207201	47.060	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.120%
26) 1,2-Dichloroethane-d4	5.034	65	137281	52.935	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	105.860%
32) Benzene-d6	5.050	84	465160	50.798	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.600%
36) 1,2-Dichloropropane-d6	6.072	67	146445	50.853	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.700%
41) Toluene-d8	7.317	98	424328	49.089	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	98.180%
43) trans-1,3-Dichloroprop...	7.625	79	62278	45.436	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	90.880%
47) 2-Hexanone-d5	8.088	63	99717	90.244	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	90.240%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	173623	47.075	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	94.160%
66) 1,2-Dichlorobenzene-d4	11.625	152	170509	50.844	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.680%
Target Compounds					Qvalue	
25) Chloroform	4.375	83	15628	3.409	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
Data File : VV022058.D
Acq On : 01 Sep 2021 10:39
Operator : SY/MD
Sample : VV0901WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Quant Time: Sep 02 05:28:50 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 02 05:24:11 2021
Response via : Initial Calibration

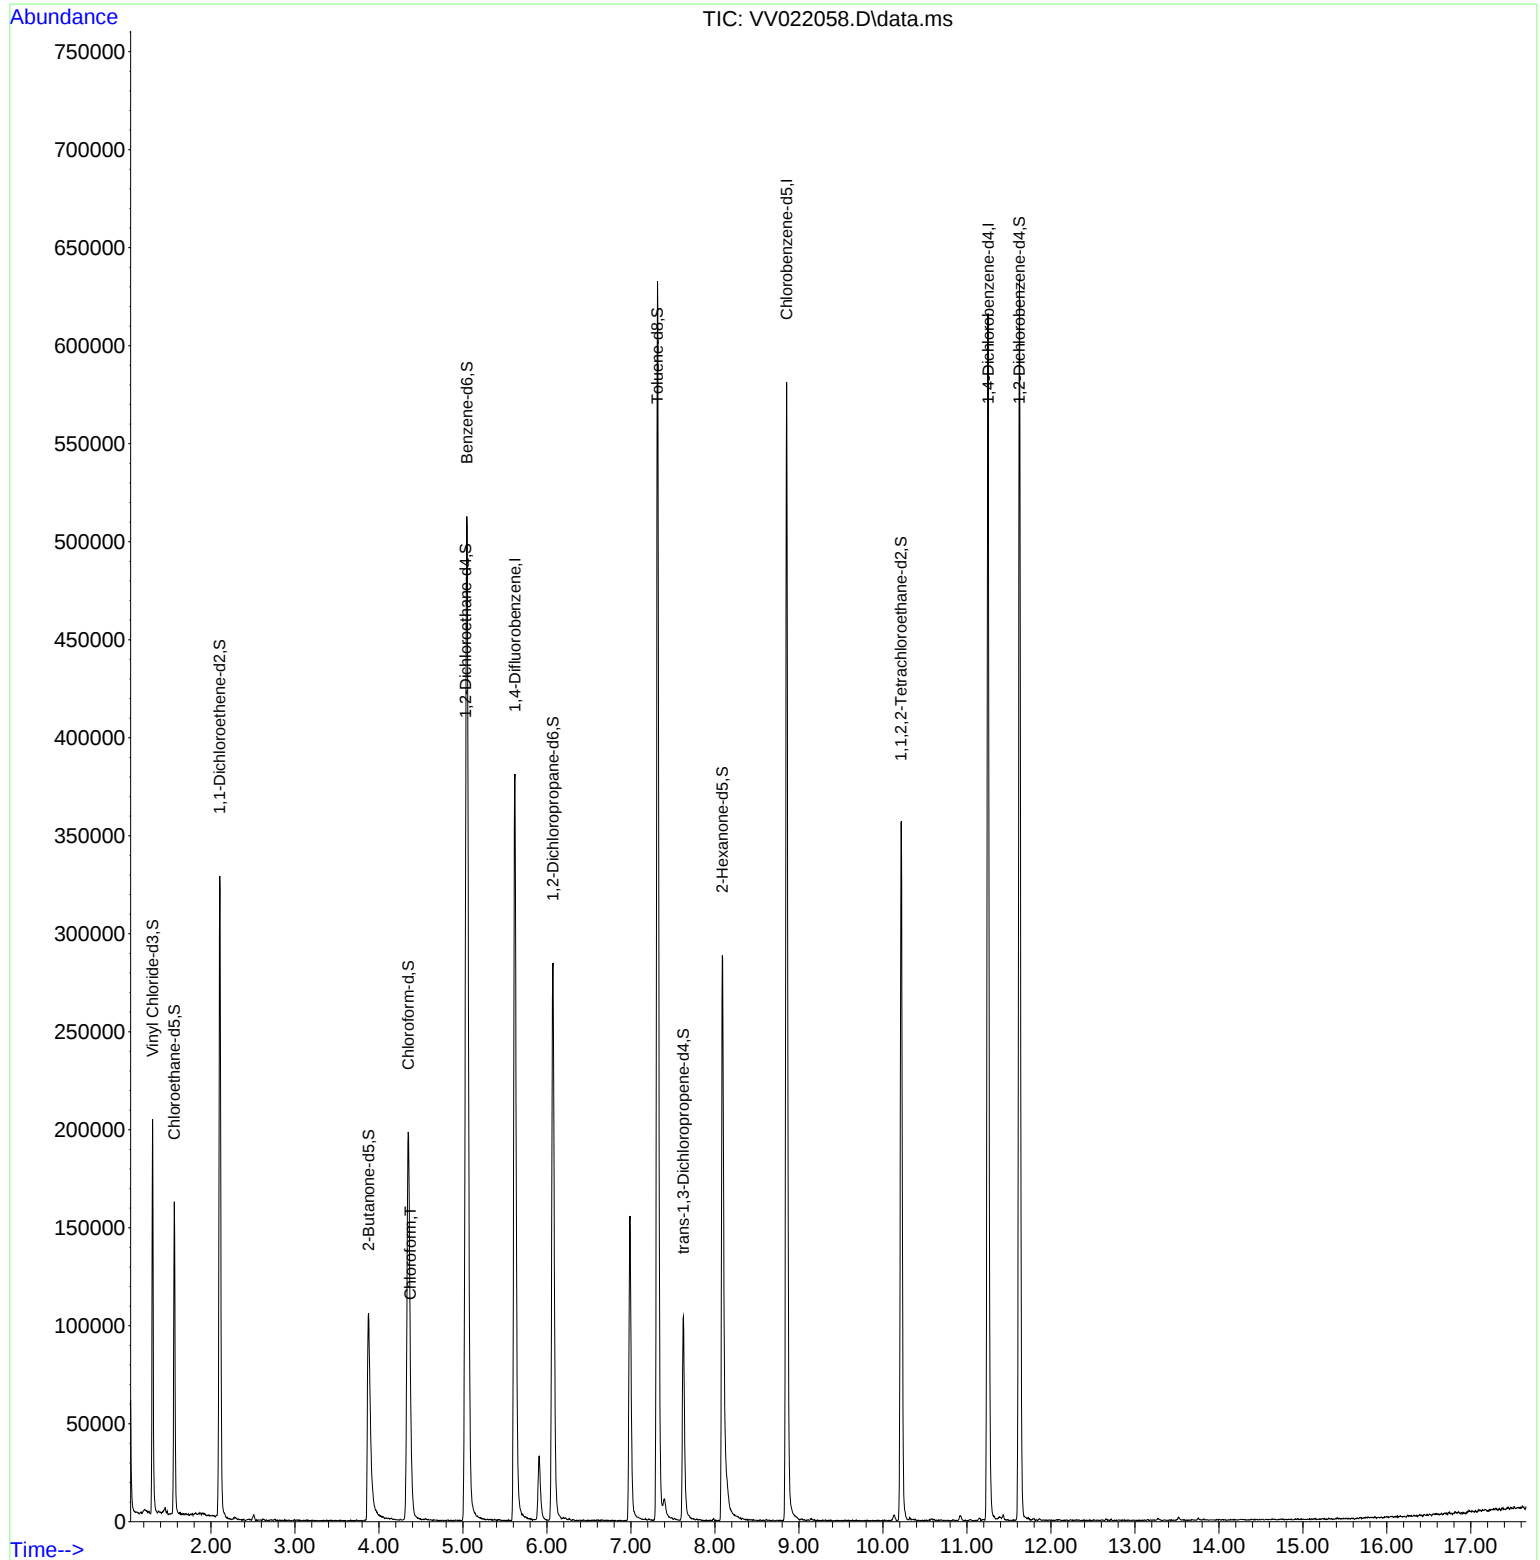

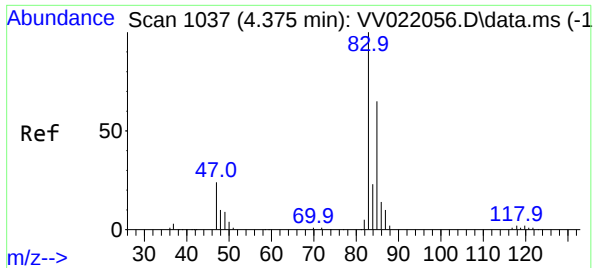

#25
Chloroform
Concen: 3.409 ug/L
RT: 4.375 min Scan# 1037
Delta R.T. -0.000 min
Lab File: VV022058.D
Acq: 01 Sep 2021 10:39

Instrument :
MSVOA_V
ClientSampleId :
VBLK248

Tgt Ion: 83 Resp: 15628
Ion Ratio Lower Upper
83 100
85 65.1 46.3 85.9

