

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
 Data File : VV022063.D
 Acq On : 01 Sep 2021 13:35
 Operator : SY/MD
 Sample : M3608-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKK1

Quant Time: Sep 02 05:43:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 02 05:24:11 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	375303	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	359397	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	185705	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	126569	48.699	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	97.400%	
7) Chloroethane-d5	1.565	69	99990	49.265	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	98.520%	
11) 1,1-Dichloroethene-d2	2.105	63	172025	40.021	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	80.040%	
21) 2-Butanone-d5	3.876	46	174062	97.653	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	97.650%	
24) Chloroform-d	4.352	84	218377	46.080	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.160%	
26) 1,2-Dichloroethane-d4	5.034	65	136363	48.851	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.700%	
32) Benzene-d6	5.050	84	471809	48.400	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.800%	
36) 1,2-Dichloropropane-d6	6.072	67	144599	47.168	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	94.340%	
41) Toluene-d8	7.317	98	431676	46.911	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	93.820%	
43) trans-1,3-Dichloroprop...	7.625	79	60482	41.451	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	82.900%	
47) 2-Hexanone-d5	8.088	63	110599	94.025	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	94.020%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	194365	49.504	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	99.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	178398	48.866	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	97.740%	
Target Compounds						
33) Benzene	5.101	78	13984	1.337	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
Data File : VV022063.D
Acq On : 01 Sep 2021 13:35
Operator : SY/MD
Sample : M3608-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKK1

Quant Time: Sep 02 05:43:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 02 05:24:11 2021
Response via : Initial Calibration

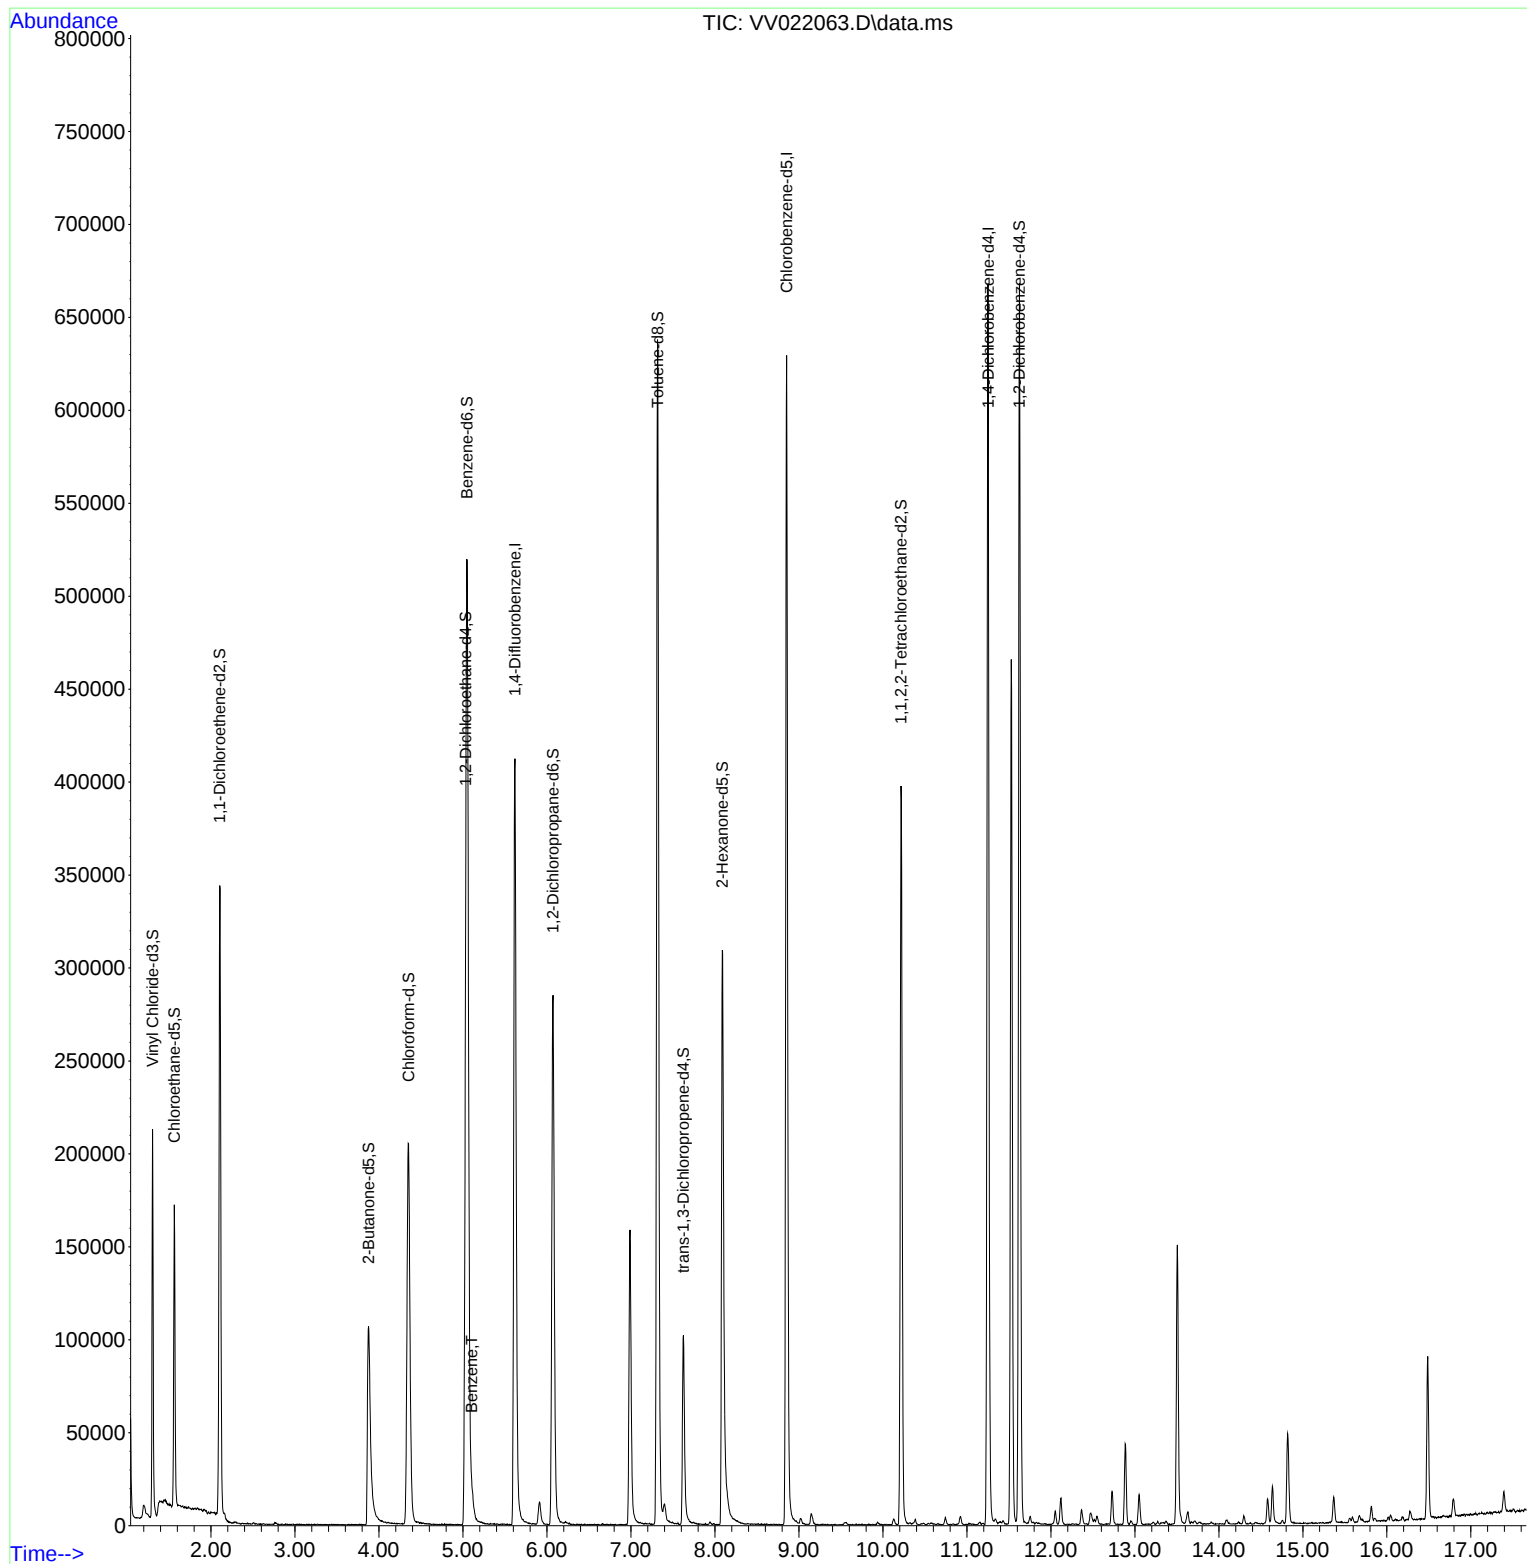

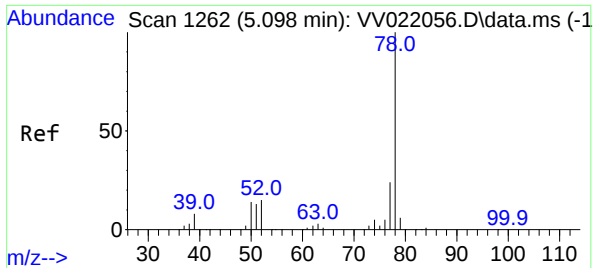

#33

Benzene

Concen: 1.337 ug/L

RT: 5.101 min Scan# 1263

Delta R.T. 0.003 min

Lab File: VV022063.D

Acq: 01 Sep 2021 13:35

Tgt Ion: 78 Resp: 13984

Instrument :
MSVOA_V
ClientSampleId :
DBKK1

