

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
 Data File : VV022066.D
 Acq On : 01 Sep 2021 14:48
 Operator : SY/MD
 Sample : M3579-06ME
 Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6A8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022066.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.298	74	80	112	rBV	132244	196275	6.55%	1.454%
2	2.073	312	321	333	rBV	320030	445877	14.87%	3.304%
3	2.944	589	592	593	rBV	300	163	0.01%	0.001%
4	3.008	609	612	614	rBV2	460	302	0.01%	0.002%
5	3.265	689	692	694	rBV	340	188	0.01%	0.001%
6	3.278	694	696	698	rVV	458	211	0.01%	0.002%
7	3.339	711	715	716	rBV	496	288	0.01%	0.002%
8	3.401	730	734	735	rBV	319	230	0.01%	0.002%
9	3.471	753	756	760	rVB3	367	259	0.01%	0.002%
10	3.494	760	763	766	rBV2	215	152	0.01%	0.001%
11	3.510	766	768	770	rVB	365	172	0.01%	0.001%
12	3.529	770	774	775	rBV	346	218	0.01%	0.002%
13	3.564	782	785	787	rBV	391	180	0.01%	0.001%
14	3.635	805	807	810	rBV2	342	231	0.01%	0.002%
15	3.674	816	819	824	rVB2	269	193	0.01%	0.001%
16	3.716	828	832	833	rBV2	237	181	0.01%	0.001%
17	3.761	843	846	848	rBV2	283	188	0.01%	0.001%
18	3.889	876	886	931	rBV	75710	298539	9.96%	2.212%
19	4.343	1009	1027	1059	rBV	189618	509911	17.01%	3.778%
20	4.571	1096	1098	1101	rVB3	554	184	0.01%	0.001%
21	4.587	1101	1103	1104	rBV	346	157	0.01%	0.001%
22	4.860	1184	1188	1189	rBV2	426	328	0.01%	0.002%
23	4.883	1192	1195	1198	rVB2	420	212	0.01%	0.002%
24	4.928	1207	1209	1213	rBV3	251	208	0.01%	0.002%
25	5.037	1227	1243	1276	rBV2	533488	1330932	44.39%	9.862%
26	5.314	1324	1329	1330	rBV2	422	280	0.01%	0.002%
27	5.481	1379	1381	1382	rBV	356	148	0.00%	0.001%
28	5.542	1397	1400	1405	rBV4	337	384	0.01%	0.003%
29	5.564	1405	1407	1409	rBV	423	210	0.01%	0.002%
30	5.613	1410	1422	1451	rBV	421254	879961	29.35%	6.520%
31	5.908	1502	1514	1535	rBV6	25664	63658	2.12%	0.472%
32	5.992	1535	1540	1542	rBV4	1314	1355	0.05%	0.010%
33	6.066	1551	1563	1598	rVB	270268	584864	19.51%	4.334%
34	6.272	1625	1627	1630	rBV4	446	213	0.01%	0.002%
35	6.310	1637	1639	1643	rBV2	584	361	0.01%	0.003%
36	6.352	1650	1652	1654	rBV	369	149	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
 Data File : VV022066.D
 Acq On : 01 Sep 2021 14:48
 Operator : SY/MD
 Sample : M3579-06ME
 Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6A8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.413	1669	1671	1676	rVB	377	205	0.01%	0.002%
38	6.436	1676	1678	1680	rBV2	355	144	0.00%	0.001%
39	6.468	1686	1688	1691	rVB	363	167	0.01%	0.001%
40	6.545	1708	1712	1715	rBV	308	244	0.01%	0.002%
41	6.635	1737	1740	1741	rBV3	605	343	0.01%	0.003%
42	6.732	1766	1770	1775	rVB6	721	653	0.02%	0.005%
43	6.751	1775	1776	1778	rBV	388	141	0.00%	0.001%
44	6.806	1790	1793	1795	rVB	422	250	0.01%	0.002%
45	6.873	1809	1814	1817	rVB2	505	331	0.01%	0.002%
46	6.892	1817	1820	1821	rBV	242	146	0.00%	0.001%
47	6.921	1826	1829	1834	rBV2	237	185	0.01%	0.001%
48	6.989	1837	1850	1872	rBV	142046	280714	9.36%	2.080%
49	7.275	1937	1939	1940	rBV2	356	141	0.00%	0.001%
50	7.317	1940	1952	1971	rBV	614794	1101235	36.73%	8.160%
51	7.519	2012	2015	2016	rBV2	779	423	0.01%	0.003%
52	7.625	2037	2048	2071	rBV	93236	185708	6.19%	1.376%
53	7.799	2099	2102	2106	rBV4	544	468	0.02%	0.003%
54	7.847	2114	2117	2119	rBV	600	357	0.01%	0.003%
55	7.918	2134	2139	2141	rBV3	376	367	0.01%	0.003%
56	7.976	2143	2157	2177	rBV	1755546	2998197	100.00%	22.216%
57	8.108	2185	2198	2237	rBV	262342	657340	21.92%	4.871%
58	8.548	2332	2335	2341	rBV4	552	539	0.02%	0.004%
59	8.584	2343	2346	2349	rVV2	468	338	0.01%	0.003%
60	8.670	2371	2373	2375	rBV2	366	193	0.01%	0.001%
61	8.767	2400	2403	2404	rBV2	262	157	0.01%	0.001%
62	8.854	2418	2430	2454	rBV	608458	1082171	36.09%	8.019%
63	9.153	2516	2523	2532	rVV5	1406	2338	0.08%	0.017%
64	9.227	2543	2546	2548	rBV	304	183	0.01%	0.001%
65	9.239	2548	2550	2552	rVV3	362	190	0.01%	0.001%
66	9.285	2561	2564	2566	rVB2	439	190	0.01%	0.001%
67	9.439	2608	2612	2614	rVB2	385	166	0.01%	0.001%
68	9.622	2667	2669	2672	rVB2	339	140	0.00%	0.001%
69	9.728	2700	2702	2713	rVB4	465	661	0.02%	0.005%
70	9.780	2713	2718	2721	rBV2	331	274	0.01%	0.002%
71	9.838	2733	2736	2737	rBV2	349	147	0.00%	0.001%
72	9.902	2754	2756	2759	rBV	332	214	0.01%	0.002%
73	10.095	2812	2816	2817	rBV2	435	233	0.01%	0.002%
74	10.130	2818	2827	2839	rVB2	4347	6847	0.23%	0.051%
75	10.223	2843	2856	2877	rBV	396785	657556	21.93%	4.872%
76	10.387	2905	2907	2916	rVB4	957	924	0.03%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
 Data File : VV022066.D
 Acq On : 01 Sep 2021 14:48
 Operator : SY/MD
 Sample : M3579-06ME
 Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB6A8ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

77	10.458	2927	2929	2932	rBV	359	171	0.01%	0.001%
78	10.500	2940	2942	2943	rBV	435	206	0.01%	0.002%
79	10.664	2988	2993	2994	rBV2	439	357	0.01%	0.003%
80	10.767	3021	3025	3027	rBV2	364	319	0.01%	0.002%
81	10.879	3057	3060	3062	rBV2	293	176	0.01%	0.001%
82	11.034	3106	3108	3114	rVB2	1123	926	0.03%	0.007%
83	11.153	3137	3145	3149	rBV6	1734	2682	0.09%	0.020%
84	11.252	3165	3176	3201	rBV	715094	1116531	37.24%	8.273%
85	11.628	3281	3293	3317	rBV	675447	1047897	34.95%	7.765%
86	11.918	3380	3383	3389	rBV4	321	357	0.01%	0.003%
87	11.979	3400	3402	3404	rBV	336	154	0.01%	0.001%
88	12.095	3434	3438	3439	rBV2	854	527	0.02%	0.004%
89	12.178	3460	3464	3470	rVB4	388	317	0.01%	0.002%
90	12.378	3524	3526	3532	rVB2	353	213	0.01%	0.002%
91	12.654	3610	3612	3615	rVB	289	148	0.00%	0.001%
92	12.670	3615	3617	3619	rBV2	398	139	0.00%	0.001%
93	12.741	3636	3639	3642	rBV	328	217	0.01%	0.002%
94	12.853	3671	3674	3675	rBV	337	157	0.01%	0.001%
95	13.281	3804	3807	3810	rBV3	542	333	0.01%	0.002%
96	13.326	3819	3821	3824	rBV	292	159	0.01%	0.001%
97	13.345	3824	3827	3832	rBV2	285	211	0.01%	0.002%
98	13.368	3832	3834	3836	rBV2	435	299	0.01%	0.002%
99	13.513	3870	3879	3889	rBV	14580	24158	0.81%	0.179%
100	13.625	3910	3914	3915	rBV3	681	429	0.01%	0.003%

Sum of corrected areas: 13495665




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
Data File : VV022066.D
Acq On : 01 Sep 2021 14:48
Operator : SY/MD
Sample : M3579-06ME
Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6A8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

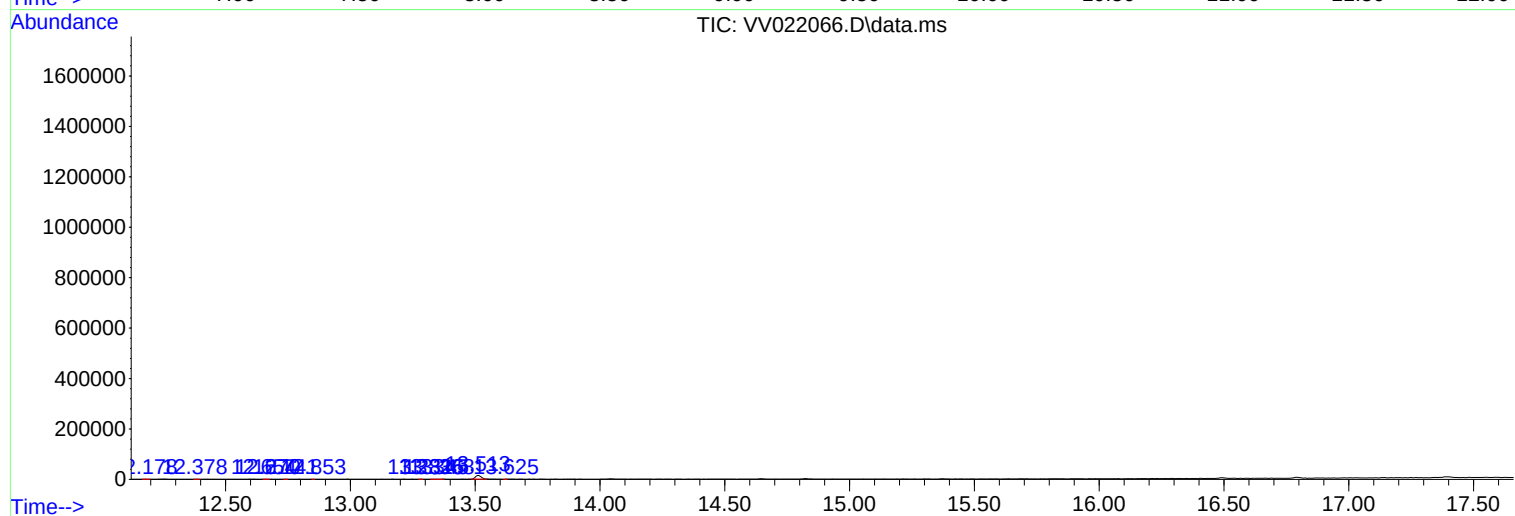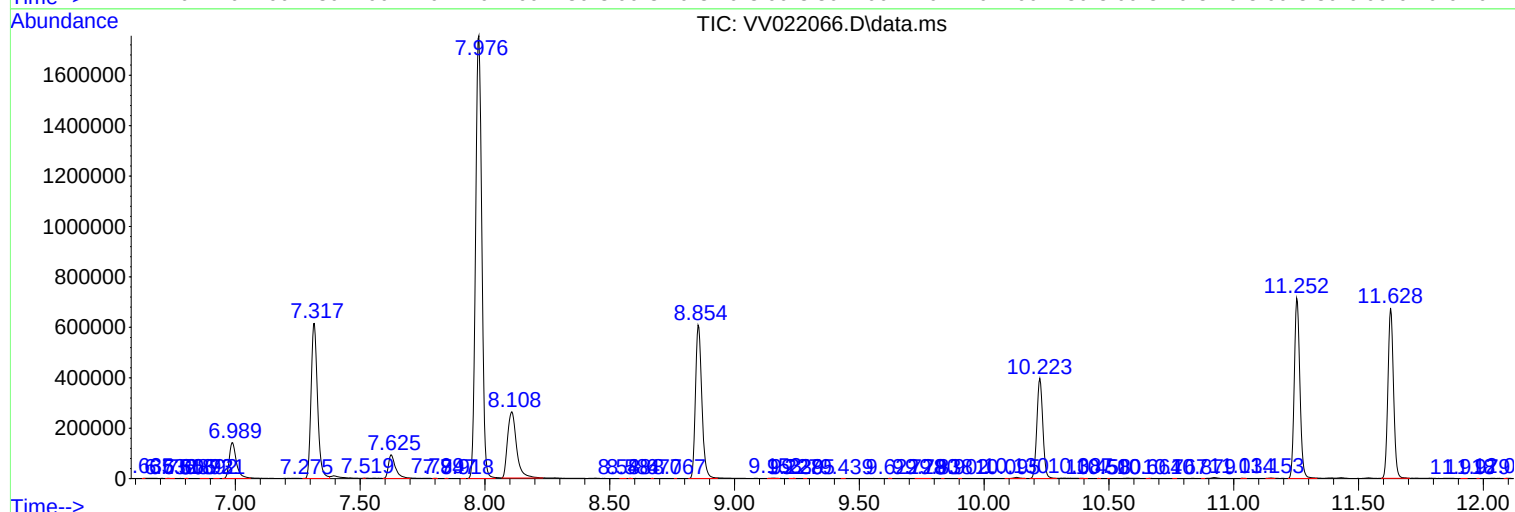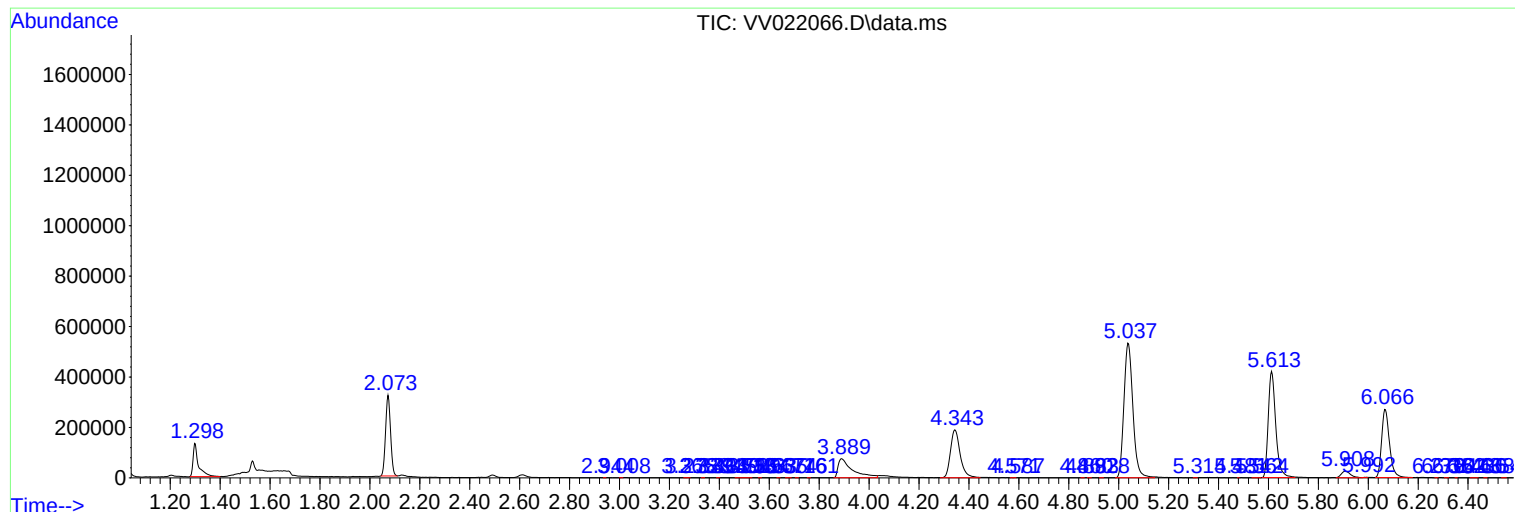

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
Data File : VV022066.D
Acq On : 01 Sep 2021 14:48
Operator : SY/MD
Sample : M3579-06ME
Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6A8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
Data File : VV022066.D
Acq On : 01 Sep 2021 14:48
Operator : SY/MD
Sample : M3579-06ME
Misc : 6.74g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB6A8ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
