


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090121\
 Data File : VV022055.D
 Acq On : 01 Sep 2021 09:19
 Operator : SY/MD
 Sample : BFB226
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB226

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis
 Last Update : Thu Sep 02 05:24:11 2021

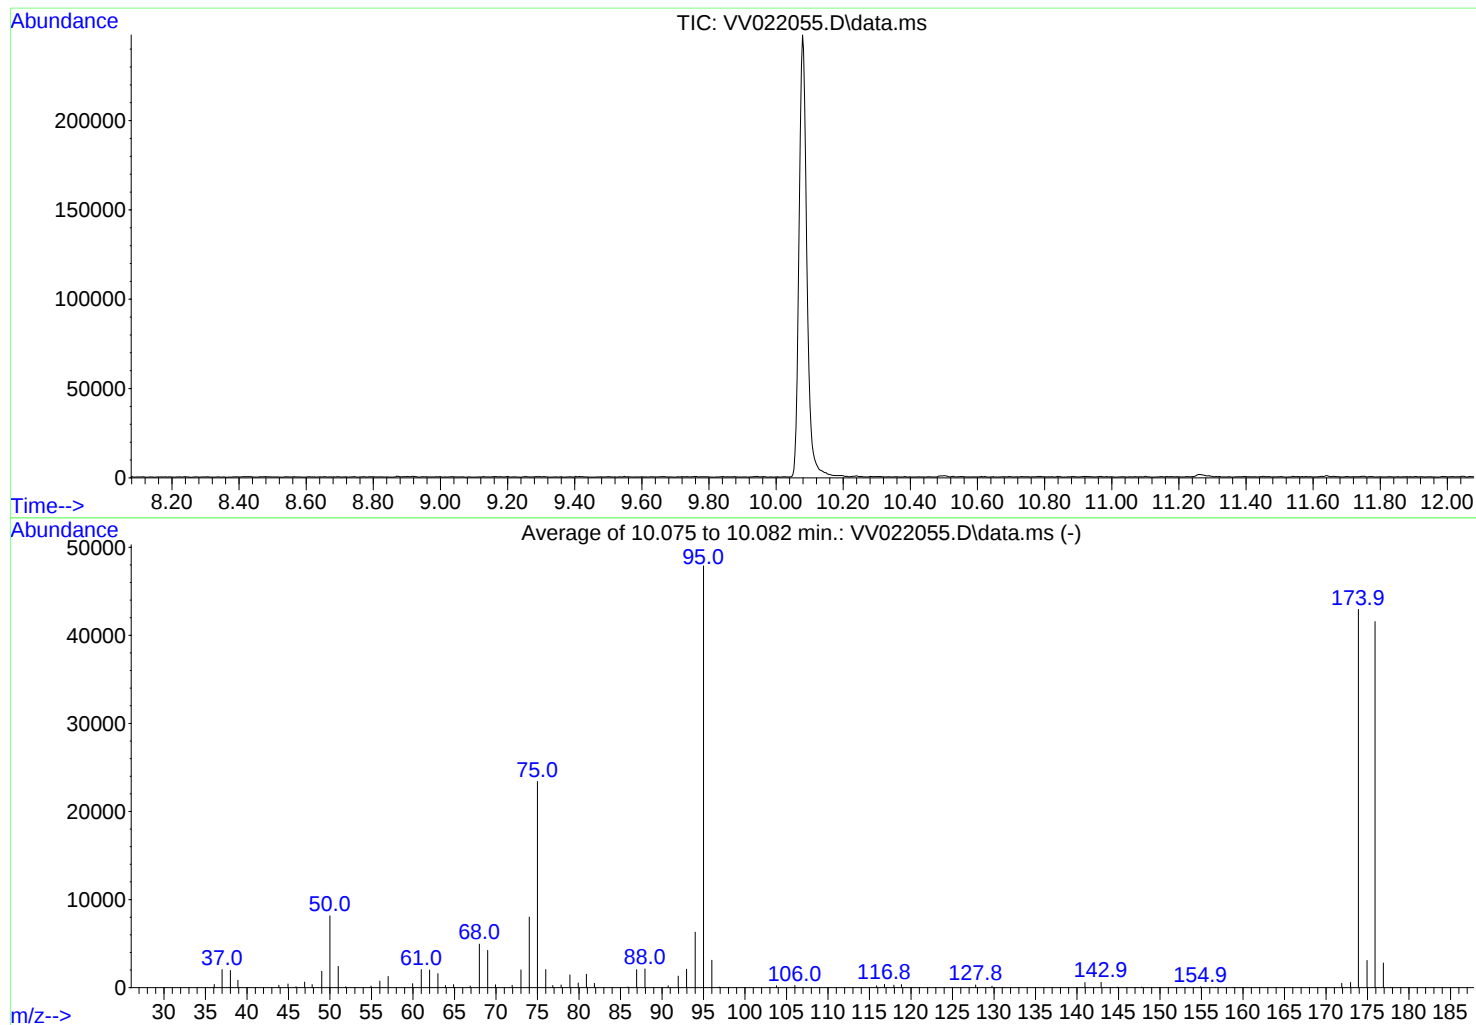

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	8157	PASS
75	95	30	80	48.8	23392	PASS
95	95	100	100	100.0	47888	PASS
96	95	5	9	6.5	3099	PASS
173	174	0.00	2	1.4	591	PASS
174	95	50	120	89.7	42936	PASS
175	174	5	9	7.2	3096	PASS
176	174	95	105	96.8	41571	PASS
177	176	5	10	6.7	2793	PASS

m/z	Abundance
36.00	384.0
37.00	2096.0
38.00	1981.0
38.90	864.0
40.00	213.0
43.90	546.0
45.00	424.0
45.90	131.0
46.90	680.0
47.80	364.0
49.00	1896.0
50.00	8466.0
51.00	2491.0
51.90	119.0
54.90	200.0
56.00	787.0
57.00	1326.0
60.00	448.0
61.00	2104.0
62.00	2011.0
63.00	1653.0
63.90	236.0
64.90	358.0
66.90	205.0
68.00	5132.0
69.00	4386.0
69.90	310.0
71.90	274.0
73.00	2070.0
74.00	8196.0
75.00	24256.0
76.00	2156.0
76.80	220.0
77.80	316.0
78.90	1517.0
79.90	534.0
80.90	1584.0
81.90	509.0
85.90	118.0
86.90	2085.0
87.90	2177.0
90.70	234.0
92.00	1325.0
93.00	2159.0
94.00	6598.0
95.00	49416.0
96.00	3187.0
96.90	103.0
103.80	210.0
106.00	256.0
115.80	230.0
116.80	383.0
118.00	289.0
118.80	369.0
127.80	314.0
129.70	182.0
141.00	596.0
142.90	632.0
144.90	116.0
147.80	112.0
154.90	104.0
156.70	110.0
171.90	501.0
173.00	618.0
173.90	44680.0
175.00	3183.0
175.90	43120.0
176.90	2939.0
177.80	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
36.00	382.0
37.00	2005.0
38.00	1965.0
38.90	813.0
40.10	208.0
43.80	588.0
44.90	369.0
45.90	106.0
47.00	621.0
47.80	391.0
49.00	1868.0
50.00	7829.0
51.00	2322.0
51.90	105.0
55.00	161.0
56.00	740.0
57.00	1202.0
59.80	430.0
61.00	1947.0
62.00	1858.0
63.00	1567.0
63.90	264.0
64.90	342.0
66.90	185.0
68.00	4928.0
69.00	4347.0
69.90	318.0
71.90	271.0
73.00	2025.0
74.00	8088.0
75.00	22960.0
76.00	2070.0
76.80	236.0
77.90	334.0
78.90	1488.0
79.90	516.0
80.90	1497.0
81.80	528.0
87.00	1973.0
87.90	2148.0
90.80	179.0
92.00	1304.0
92.90	2019.0
94.00	6097.0
95.00	48136.0
96.00	3194.0
103.80	234.0
106.00	246.0
115.90	225.0
116.80	341.0
117.90	283.0
118.80	343.0
127.70	331.0
129.80	157.0
131.10	100.0
141.00	547.0
142.90	593.0
144.80	120.0
154.90	103.0
158.80	110.0
171.90	557.0
172.90	618.0
173.90	43696.0
174.90	3019.0
175.90	42640.0
176.90	2728.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

Scan 2799 (10.040 min): VV022055.D\data.ms
BFB226

m/z	Abundance
39.90	276.0
43.90	290.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226

m/z	Abundance
36.10	346.0
37.00	2067.0
38.00	1875.0
38.90	827.0
40.00	181.0
43.90	538.0
45.00	453.0
45.90	120.0
46.90	634.0
47.90	275.0
49.00	1819.0
50.00	8176.0
51.00	2426.0
51.90	126.0
54.90	203.0
56.00	704.0
57.00	1269.0
60.00	502.0
61.00	2107.0
62.00	2117.0
63.00	1606.0
63.90	218.0
64.90	326.0
66.90	180.0
68.00	4752.0
69.00	3975.0
70.00	337.0
72.00	301.0
73.00	1929.0
74.00	7739.0
75.00	22960.0
76.00	1959.0
76.90	232.0
77.80	282.0
78.90	1369.0
79.90	513.0
80.90	1521.0
81.90	446.0
85.90	158.0
86.90	2074.0
88.00	2035.0
90.70	251.0
91.90	1313.0
93.00	2079.0
94.00	6193.0
95.00	46112.0
96.00	2917.0
96.90	107.0
103.80	200.0
106.00	243.0
115.80	213.0
116.80	372.0
118.00	298.0
118.90	318.0
127.90	280.0
129.80	190.0
140.90	602.0
142.90	585.0
147.80	118.0
154.90	106.0
171.90	430.0
173.00	537.0
173.90	40432.0
175.00	3087.0
175.90	38952.0
176.90	2712.0

Instrument :
MSVOA_V
ClientSampleId :
BFB226