


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV090219\
 Data File : VV012515.D
 Acq On : 02 Sep 2019 08:38
 Operator : SY/MD
 Sample : BFB58
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB58

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Sep 04 02:10:17 2019

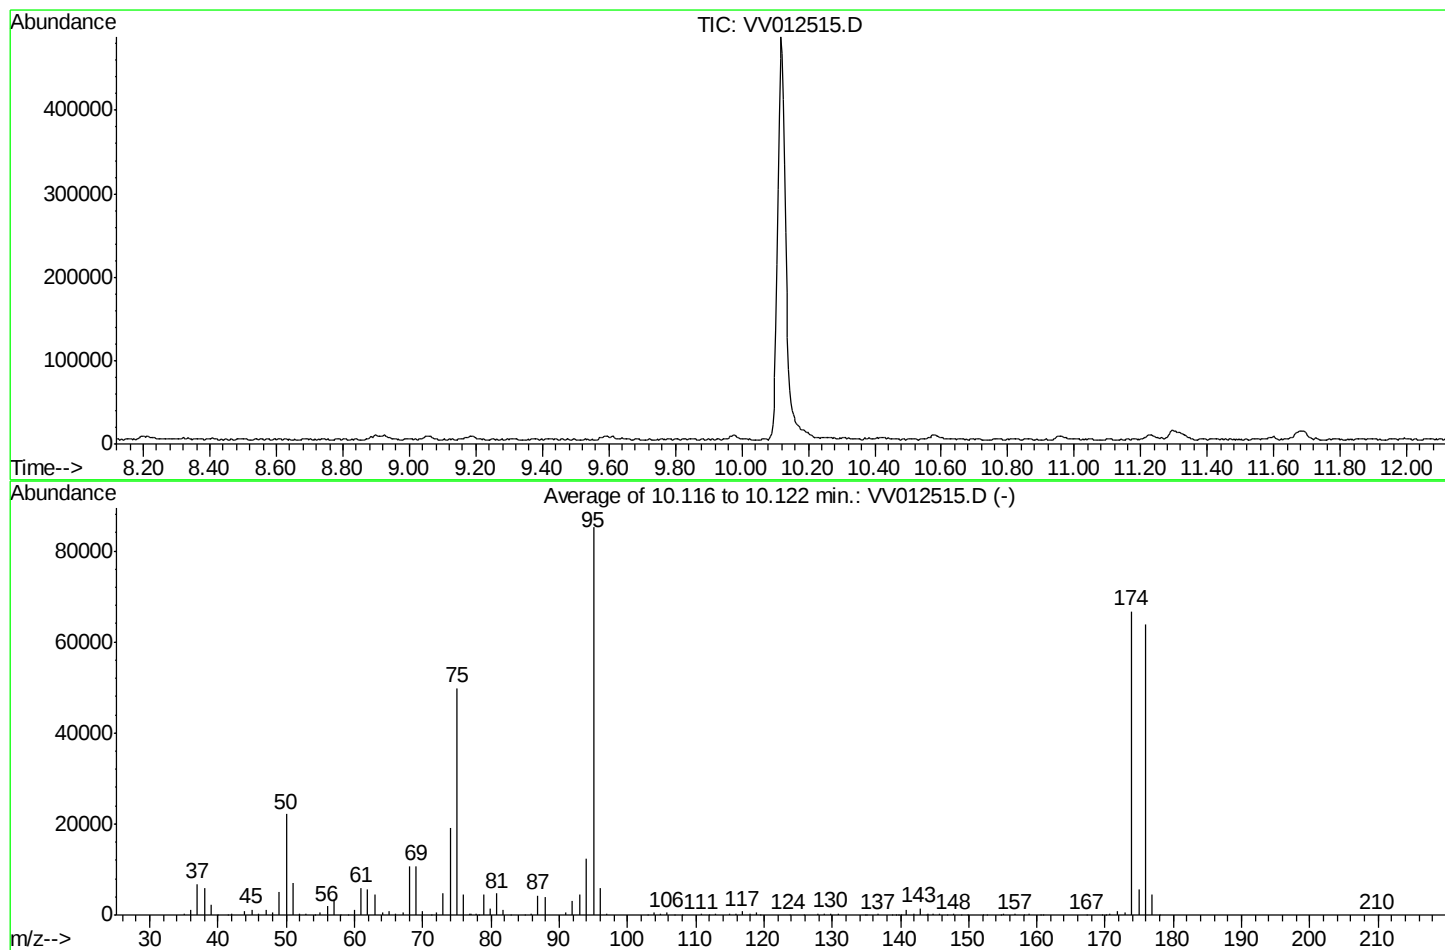

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.0	22161	PASS
75	95	30	80	58.6	49880	PASS
95	95	100	100	100.0	85178	PASS
96	95	5	9	6.9	5877	PASS
173	174	0.00	2	0.7	444	PASS
174	95	50	120	78.4	66789	PASS
175	174	5	9	8.5	5652	PASS
176	174	95	101	95.5	63781	PASS
177	176	5	9	7.2	4586	PASS

m/z	Abundance
35.10	203.0
35.90	1344.0
37.00	6492.0
38.00	5876.0
39.00	2492.0
39.90	729.0
41.40	152.0
41.90	202.0
43.10	141.0
43.90	1419.0
45.00	1217.0
46.00	280.0
47.00	1223.0
47.90	796.0
49.00	5075.0
50.00	22080.0
51.00	7107.0
52.00	353.0
53.00	287.0
54.10	117.0
55.00	660.0
56.00	1764.0
57.00	3325.0
58.00	185.0
58.50	178.0
59.90	1085.0
61.00	5826.0
62.00	5933.0
63.00	4751.0
64.10	615.0
65.00	871.0
66.10	204.0
67.10	407.0
68.00	10467.0
69.00	10575.0
69.90	953.0
71.30	192.0
72.00	598.0
73.00	4826.0
74.00	18448.0
75.00	49616.0
76.00	4312.0
77.10	541.0
77.80	272.0
78.90	4452.0
80.00	1319.0
80.90	4517.0
81.80	1006.0
82.80	144.0
84.90	119.0
85.90	193.0
86.90	4278.0
88.00	3868.0
90.80	695.0
92.00	3162.0
93.00	4251.0
94.00	11851.0
95.00	84272.0
96.00	5738.0
97.00	278.0
103.00	109.0
103.80	510.0
104.70	139.0
105.80	503.0
106.90	137.0
110.90	271.0
112.10	137.0
112.80	167.0
114.90	160.0
115.80	425.0
116.90	722.0
117.90	401.0
118.90	634.0
123.80	153.0
125.80	135.0
127.70	328.0
129.00	244.0
129.80	320.0
130.80	206.0
134.80	163.0
136.70	207.0
139.30	114.0
139.70	102.0
140.90	1041.0
142.00	192.0
142.90	1346.0
143.80	139.0
144.10	158.0
144.90	315.0
145.70	169.0
146.80	100.0
147.80	237.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

152.00	139.0
152.70	119.0
154.80	237.0
156.80	201.0
158.10	108.0
158.80	127.0
160.90	134.0
170.10	103.0
170.60	164.0
171.80	879.0
172.90	1332.0
173.90	64176.0
174.90	5306.0
175.90	60472.0
176.90	4175.0
177.90	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
35.10	164.0
35.90	1425.0
37.00	7100.0
38.00	6266.0
39.00	2622.0
40.00	792.0
41.40	132.0
42.00	190.0
43.00	167.0
43.90	1582.0
45.00	1280.0
46.10	271.0
47.00	1305.0
47.90	745.0
49.00	5269.0
50.00	22976.0
51.00	7466.0
52.00	372.0
53.00	285.0
54.10	105.0
55.00	637.0
56.00	1916.0
57.00	3526.0
57.90	237.0
59.90	1080.0
61.00	6185.0
62.00	6066.0
63.00	4710.0
64.10	570.0
65.00	802.0
66.00	206.0
67.10	500.0
68.00	11140.0
69.00	11095.0
69.90	952.0
71.20	145.0
72.00	621.0
73.00	5025.0
74.00	19696.0
75.00	51320.0
76.00	4547.0
76.80	440.0
77.10	443.0
77.80	332.0
78.10	336.0
78.90	4772.0
79.90	1345.0
80.90	4821.0
81.80	1077.0
82.90	140.0
84.90	118.0
85.90	205.0
86.90	4427.0
88.00	3947.0
90.90	722.0
91.90	3404.0
93.00	4558.0
94.00	12731.0
95.00	87904.0
96.00	5996.0
96.90	287.0
102.90	112.0
103.80	486.0
104.80	181.0
105.80	565.0
106.90	127.0
108.00	105.0
110.90	214.0
111.90	135.0
112.80	165.0
115.00	184.0
115.80	447.0
116.90	803.0
117.90	433.0
118.90	668.0
123.70	122.0
127.80	329.0
128.90	223.0
129.80	357.0
130.80	237.0
134.70	149.0
136.80	223.0
138.70	130.0
139.80	123.0
140.10	137.0
140.90	1126.0
142.10	210.0
142.90	1506.0
144.10	184.0
144.90	294.0
145.80	191.0
147.90	243.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

149.80	121.0
152.10	138.0
155.00	250.0
156.80	232.0
158.80	165.0
160.90	119.0
167.30	107.0
170.10	120.0
170.60	174.0
171.80	1014.0
173.90	69120.0
174.90	5835.0
175.90	65888.0
176.90	4818.0
210.00	101.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
35.10	133.0
36.00	1456.0
37.00	6947.0
38.00	5921.0
39.00	2430.0
40.00	841.0
41.30	112.0
42.00	167.0
43.00	189.0
44.00	1594.0
44.90	1300.0
45.90	291.0
47.00	1220.0
48.00	732.0
49.00	4738.0
50.00	21864.0
51.00	6954.0
52.00	365.0
52.90	203.0
55.00	538.0
56.00	1999.0
57.00	3345.0
57.90	245.0
59.10	162.0
59.90	961.0
61.00	5844.0
62.00	5605.0
63.00	4404.0
64.00	546.0
65.00	714.0
65.90	199.0
67.10	468.0
68.00	10573.0
69.00	10847.0
70.00	829.0
71.00	133.0
72.00	620.0
73.00	4941.0
74.00	18944.0
75.00	48704.0
76.00	4321.0
76.80	438.0
77.80	410.0
78.90	4637.0
79.90	1282.0
80.90	4783.0
81.80	1057.0
82.90	151.0
86.00	206.0
86.90	4157.0
87.90	3778.0
90.90	643.0
91.90	3107.0
93.00	4551.0
94.00	12478.0
95.00	83360.0
96.00	5897.0
97.00	241.0
102.90	138.0
103.80	503.0
104.80	251.0
105.80	547.0
106.90	126.0
107.90	113.0
110.90	180.0
111.90	134.0
112.80	138.0
115.00	190.0
115.80	419.0
116.90	784.0
117.90	436.0
118.90	624.0
119.50	117.0
127.90	345.0
128.80	195.0
129.90	425.0
130.80	201.0
135.00	172.0
136.80	211.0
138.70	125.0
140.10	164.0
140.90	1162.0
142.10	165.0
142.90	1431.0
144.00	187.0
144.80	272.0
145.80	183.0
147.80	214.0
148.90	103.0
149.70	121.0
152.10	101.0
155.00	250.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

156.90	257.0
158.70	214.0
160.60	108.0
160.80	109.0
169.60	130.0
170.60	167.0
171.90	1031.0
173.90	67072.0
174.90	5817.0
175.90	64984.0
176.90	4765.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58

m/z	Abundance
35.90	225.0
36.60	165.0
37.90	198.0
38.60	187.0
39.10	184.0
39.90	709.0
41.00	147.0
42.20	163.0
43.00	208.0
43.90	642.0
44.70	107.0
45.40	140.0
46.60	189.0
47.80	120.0
50.00	145.0
51.00	112.0
51.40	137.0
52.40	157.0
53.40	112.0
55.40	115.0
57.90	106.0
58.70	118.0
60.50	141.0
61.80	124.0
64.60	113.0
67.70	101.0
70.80	100.0
72.40	118.0
84.50	127.0
91.20	115.0
106.10	142.0
116.60	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB58