

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022072.D
 Acq On : 02 Sep 2021 13:49
 Operator : SY/MD
 Sample : VV0902MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Quant Time: Sep 03 01:00:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 03 00:59:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	350600	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	321390	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	156354	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	109489	45.095	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.200%		
7) Chloroethane-d5	1.564	69	89395	47.148	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.300%		
11) 1,1-Dichloroethene-d2	2.105	63	139804	34.817	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.640%		
21) 2-Butanone-d5	3.902	46	173151	103.987	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	103.990%		
24) Chloroform-d	4.349	84	211797	47.841	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.680%		
26) 1,2-Dichloroethane-d4	5.031	65	130810	50.164	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.320%		
32) Benzene-d6	5.050	84	436931	50.123	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.240%		
36) 1,2-Dichloropropane-d6	6.069	67	137957	50.323	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.640%		
41) Toluene-d8	7.317	98	392048	47.643	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	95.280%		
43) trans-1,3-Dichloroprop...	7.622	79	60482	46.353	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	92.700%		
47) 2-Hexanone-d5	8.092	63	107601	102.294	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	102.290%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	176975	50.406	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	100.820%		
66) 1,2-Dichlorobenzene-d4	11.625	152	152062	49.471	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	98.940%		
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	2391	0.882	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022072.D
Acq On : 02 Sep 2021 13:49
Operator : SY/MD
Sample : VV0902MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Time: Sep 03 01:00:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 03 00:59:14 2021
Response via : Initial Calibration

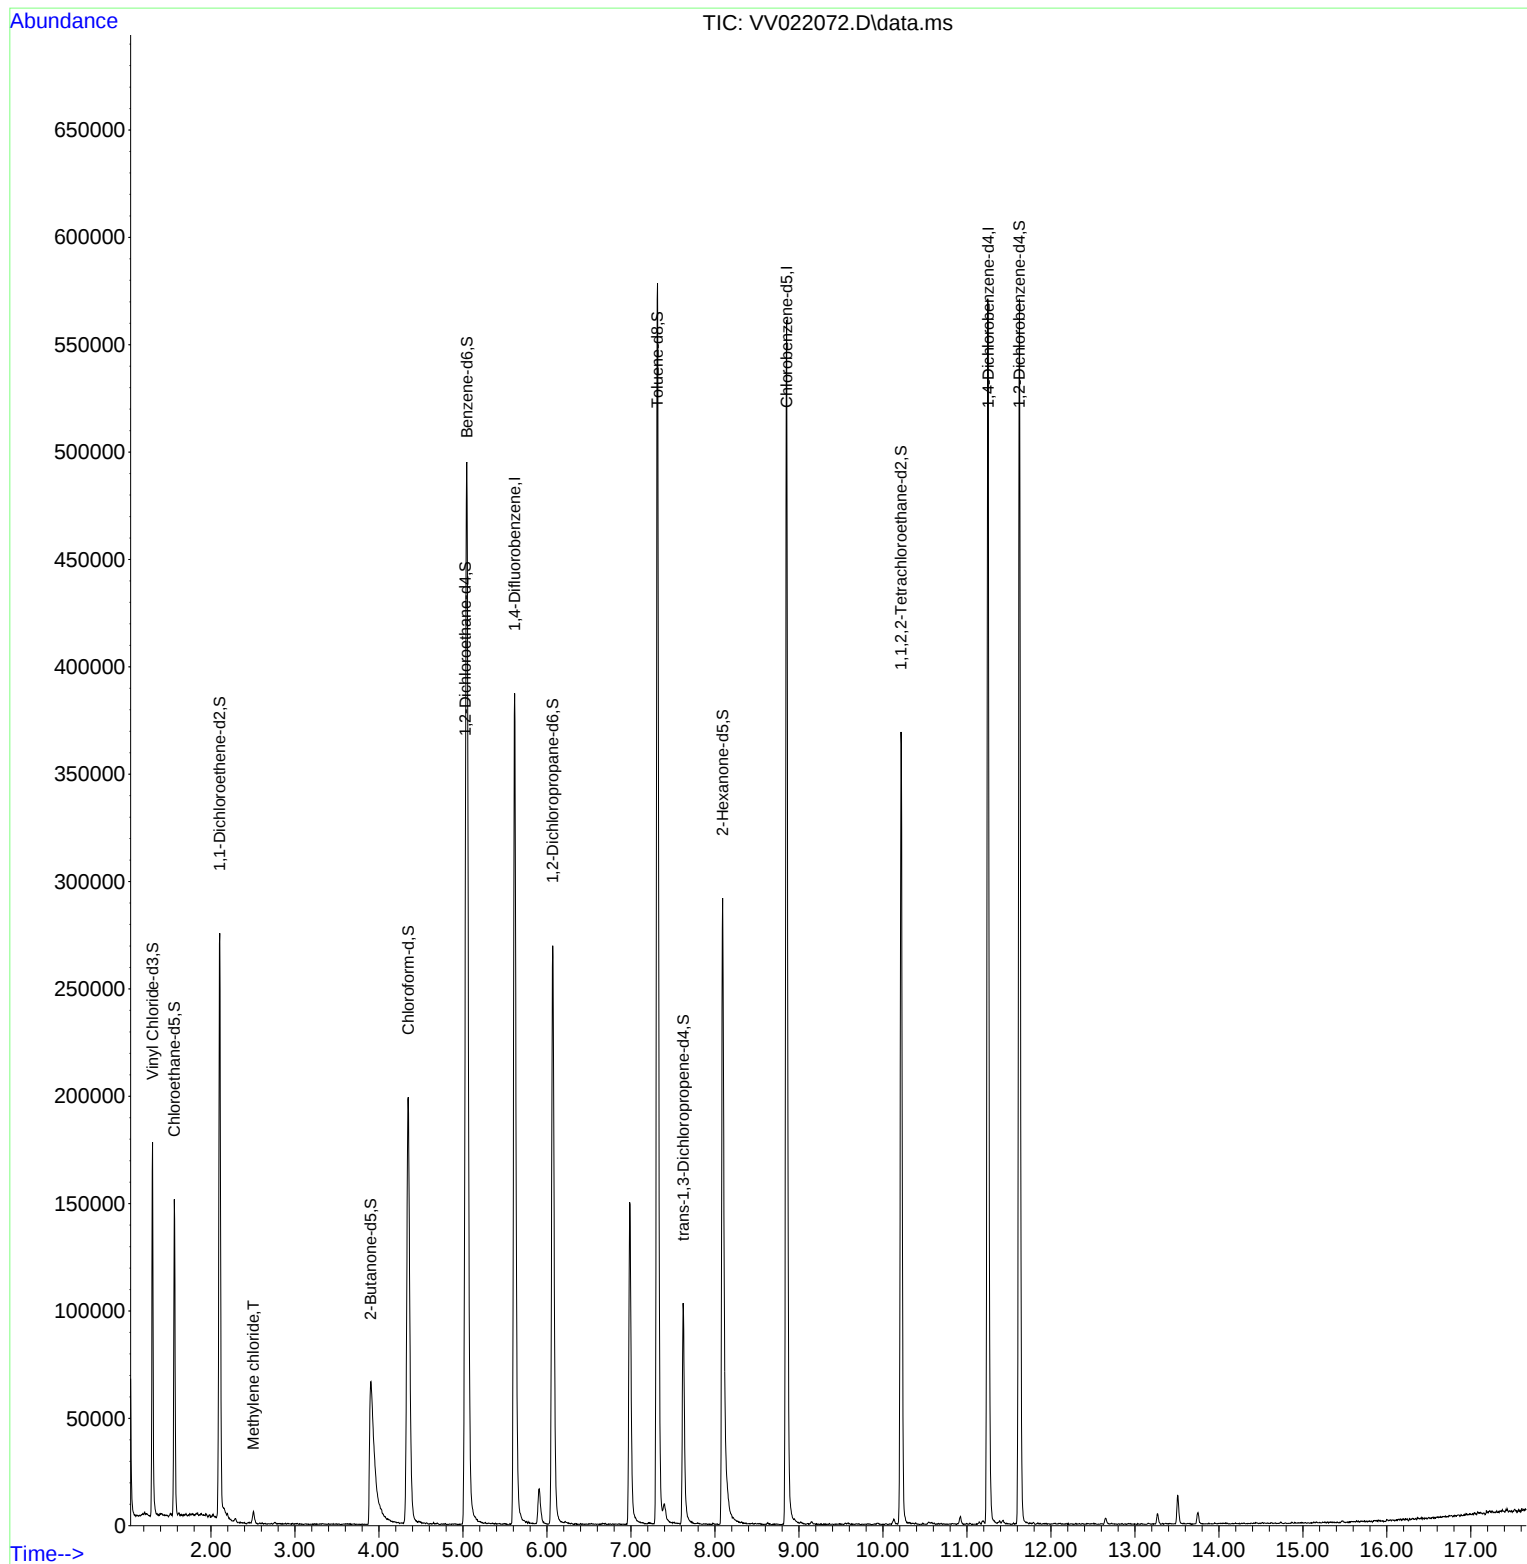

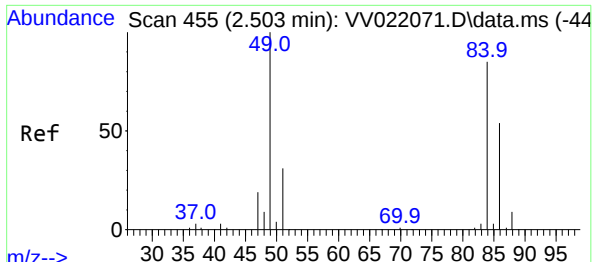

#16
Methylene chloride
Concen: 0.882 ug/L
RT: 2.503 min Scan# 455
Delta R.T. 0.000 min
Lab File: VV022072.D
Acq: 02 Sep 2021 13:49

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Tgt Ion:	84	Resp:	2391
Ion	Ratio	Lower	Upper
84	100		
86	78.0	44.8	83.2
49	109.6	80.2	149.0

