

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022074.D
 Acq On : 02 Sep 2021 14:35
 Operator : SY/MD
 Sample : M3608-18
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL4

Quant Time: Sep 03 01:00:31 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 03 00:59:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	345300	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	318481	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	148031	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	106308	44.457	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.920%		
7) Chloroethane-d5	1.564	69	86992	46.585	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.160%		
11) 1,1-Dichloroethene-d2	2.104	63	146199	36.968	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	73.940%		
21) 2-Butanone-d5	3.899	46	168466	102.726	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	102.730%		
24) Chloroform-d	4.352	84	203156	46.593	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.180%		
26) 1,2-Dichloroethane-d4	5.034	65	126639	49.310	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.620%		
32) Benzene-d6	5.050	84	423491	49.025	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.040%		
36) 1,2-Dichloropropane-d6	6.072	67	131842	48.532	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.060%		
41) Toluene-d8	7.316	98	380249	46.632	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.260%		
43) trans-1,3-Dichloroprop...	7.625	79	59407	45.945	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.880%		
47) 2-Hexanone-d5	8.091	63	106453	102.127	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	102.130%		
56) 1,1,2,2-Tetrachloroeth...	10.220	84	170504	49.006	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.020%		
66) 1,2-Dichlorobenzene-d4	11.628	152	144352	49.603	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.200%		
Target Compounds					Qvalue	
13) Acetone	2.185	43	3351	2.439	ug/L	# 78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022074.D
Acq On : 02 Sep 2021 14:35
Operator : SY/MD
Sample : M3608-18
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL4

Quant Time: Sep 03 01:00:31 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 03 00:59:14 2021
Response via : Initial Calibration

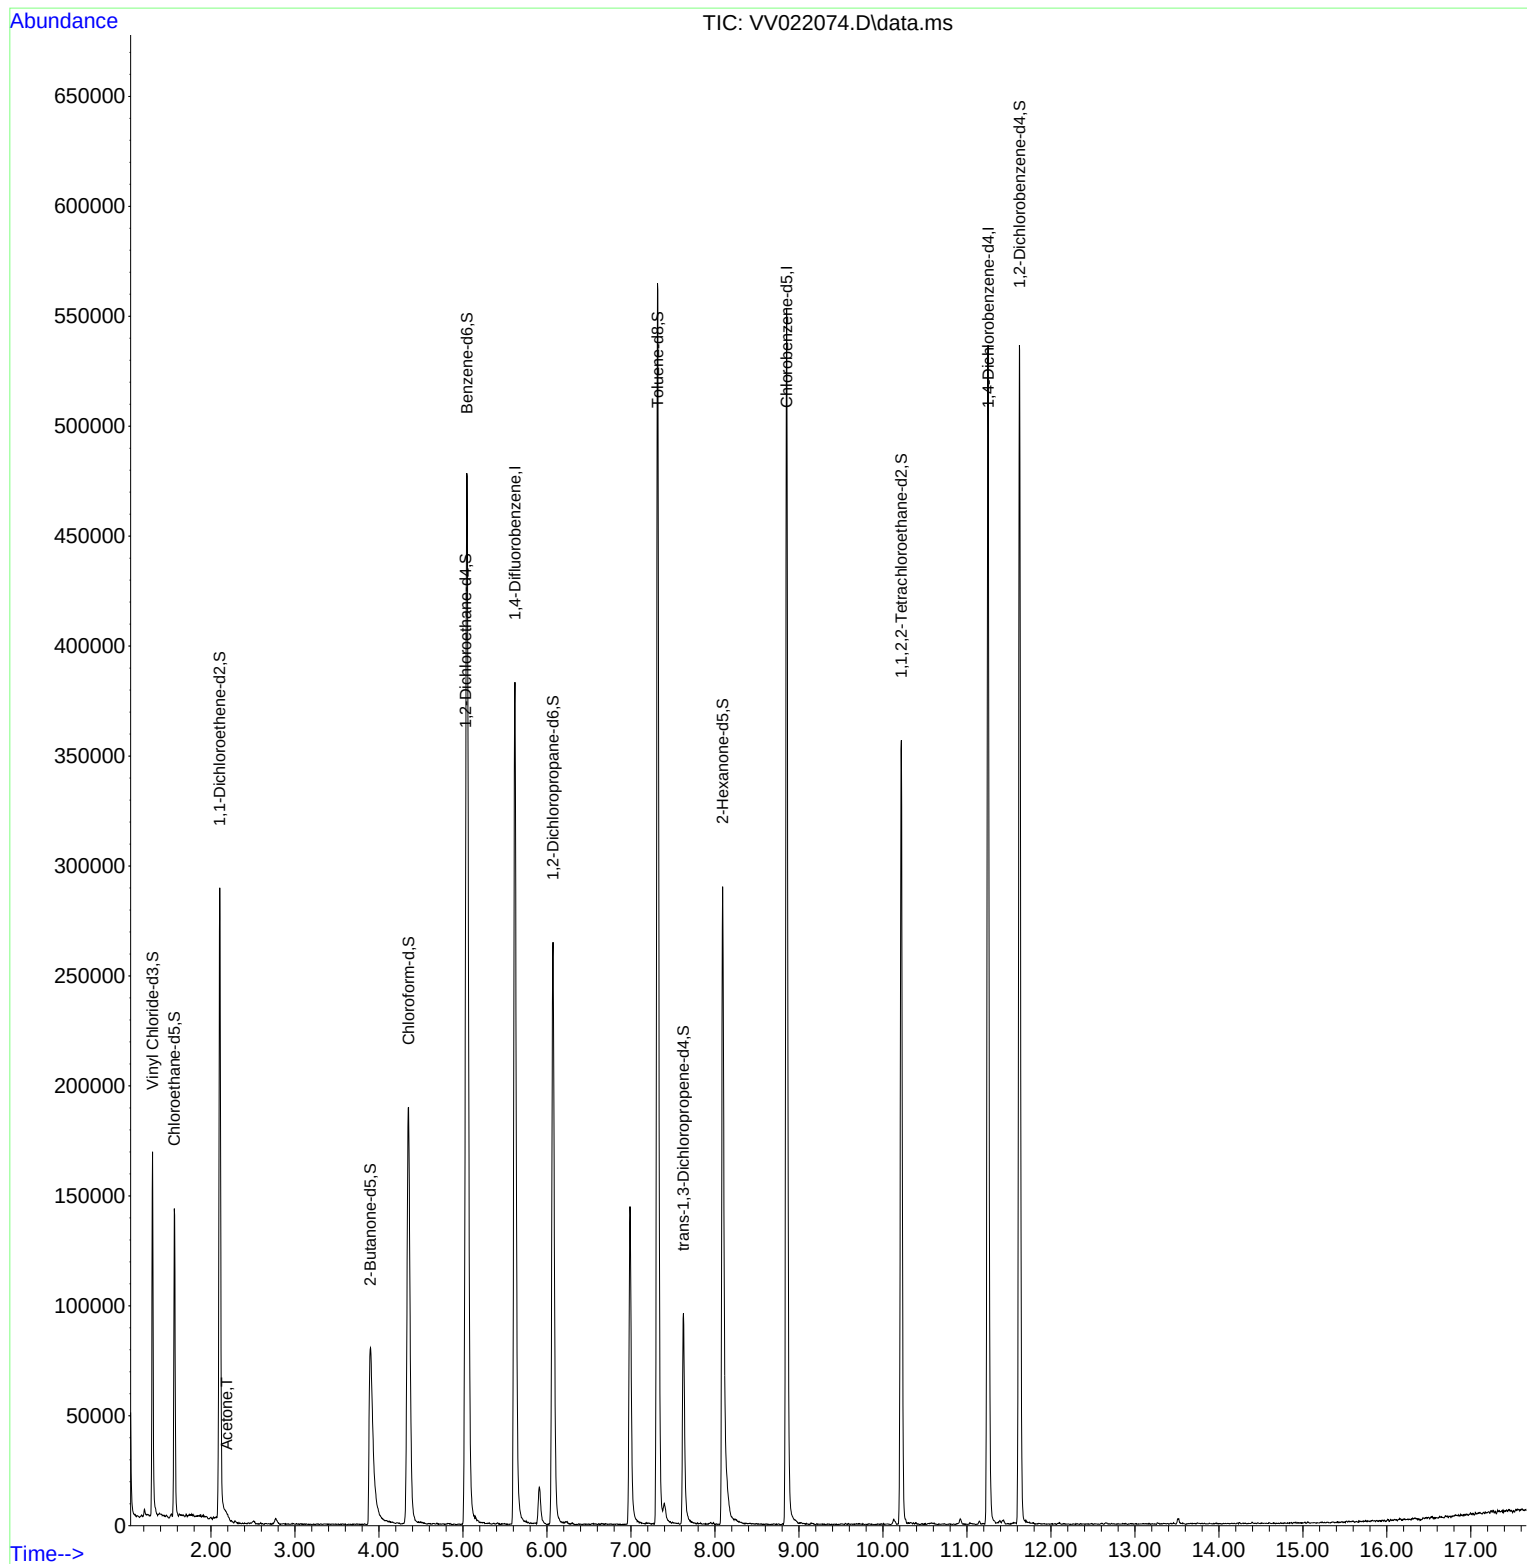

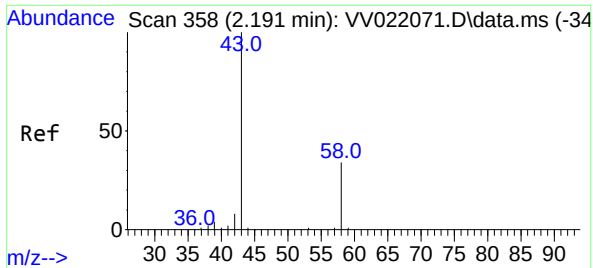

#13
Acetone
Concen: 2.439 ug/L
RT: 2.185 min Scan# 356
Delta R.T. -0.006 min
Lab File: VV022074.D
Acq: 02 Sep 2021 14:35

Instrument :
MSVOA_V
ClientSampleId :
DBKL4

Tgt Ion: 43 Resp: 3351
Ion Ratio Lower Upper
43 100
58 28.1 0.0 0.4#

