

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022081.D
 Acq On : 02 Sep 2021 17:23
 Operator : SY/MD
 Sample : M3608-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKK4

Quant Time: Sep 03 01:02:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 03 00:59:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	386974	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	356042	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	176862	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	102189	38.132	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	76.260%
7) Chloroethane-d5	1.564	69	81755	39.066	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	78.140%
11) 1,1-Dichloroethene-d2	2.105	63	145645	32.862	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.720%
21) 2-Butanone-d5	3.892	46	175730	95.615	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.620%
24) Chloroform-d	4.352	84	208685	42.707	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	85.420%
26) 1,2-Dichloroethane-d4	5.034	65	129686	45.058	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.120%
32) Benzene-d6	5.053	84	437351	45.288	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.580%
36) 1,2-Dichloropropane-d6	6.072	67	136094	44.812	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.620%
41) Toluene-d8	7.317	98	398726	43.739	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	87.480%
43) trans-1,3-Dichloroprop...	7.625	79	60245	41.678	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.360%
47) 2-Hexanone-d5	8.091	63	116581	100.044	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	100.040%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	185096	47.588	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	95.180%
66) 1,2-Dichlorobenzene-d4	11.625	152	160252	46.090	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	92.180%
Target Compounds						
33) Benzene	5.104	78	18123	1.750	ug/L	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022081.D
Acq On : 02 Sep 2021 17:23
Operator : SY/MD
Sample : M3608-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKK4

Quant Time: Sep 03 01:02:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 03 00:59:14 2021
Response via : Initial Calibration

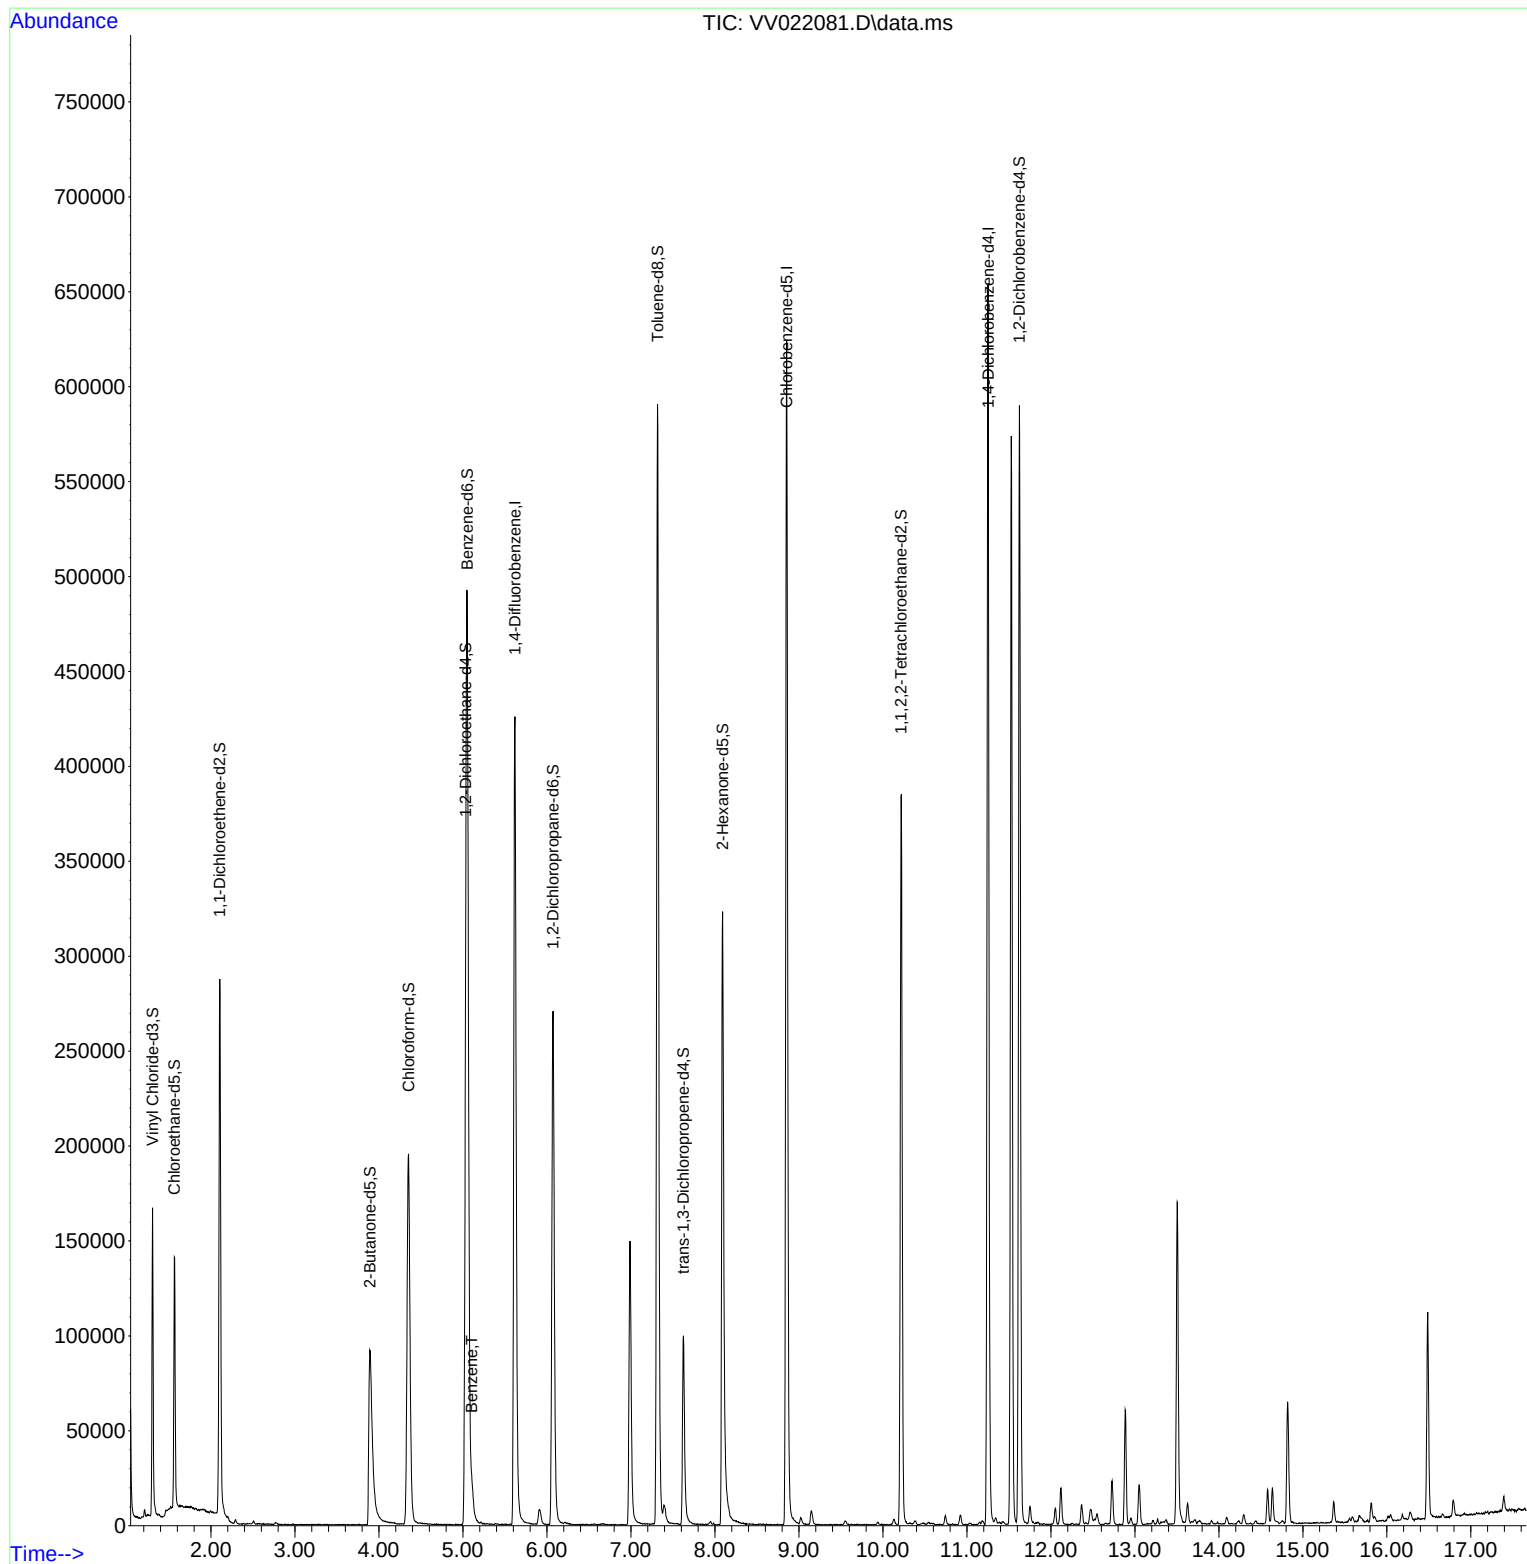

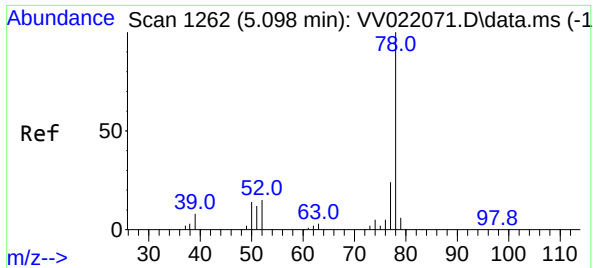

#33

Benzene

Concen: 1.750 ug/L

RT: 5.104 min Scan# 1264

Delta R.T. 0.006 min

Lab File: VV022081.D

Acq: 02 Sep 2021 17:23

Tgt Ion: 78 Resp: 18123

Instrument :
MSVOA_V
ClientSampleId :
DBKK4

