

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022086.D
 Acq On : 02 Sep 2021 19:24
 Operator : SY/MD
 Sample : M3608-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL1

Manual Integrations
 APPROVED

MMDadoda
 9/7/2021 8:50:06 AM

Quant Time: Sep 03 01:03:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 03 00:59:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	381196	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	345434	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	164594	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	104411	39.552	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	79.100%
7) Chloroethane-d5	1.565	69	86335	41.879	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.760%
11) 1,1-Dichloroethene-d2	2.105	63	145147	33.246	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	66.500%
21) 2-Butanone-d5	3.896	46	189724	104.794	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	104.790%
24) Chloroform-d	4.349	84	209094	43.439	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.880%
26) 1,2-Dichloroethane-d4	5.034	65	131704	46.453	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.900%
32) Benzene-d6	5.050	84	437485	46.693	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.380%
36) 1,2-Dichloropropane-d6	6.072	67	139827	47.455	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.900%
41) Toluene-d8	7.317	98	393632	44.506	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.020%
43) trans-1,3-Dichloroprop...	7.625	79	59231	42.235	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.460%
47) 2-Hexanone-d5	8.092	63	123287	109.048	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	109.050%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	185706	49.211	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.420%
66) 1,2-Dichlorobenzene-d4	11.625	152	153979	47.587	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	95.180%
Target Compounds						
13) Acetone	2.188	43	5055m	3.332	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022086.D
Acq On : 02 Sep 2021 19:24
Operator : SY/MD
Sample : M3608-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1


Instrument :
MSVOA_V
ClientSampleId :
DBKL1

Manual Integrations
APPROVED

MMDadoda
9/7/2021 8:50:06 AM


Quant Time: Sep 03 01:03:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 03 00:59:14 2021
Response via : Initial Calibration

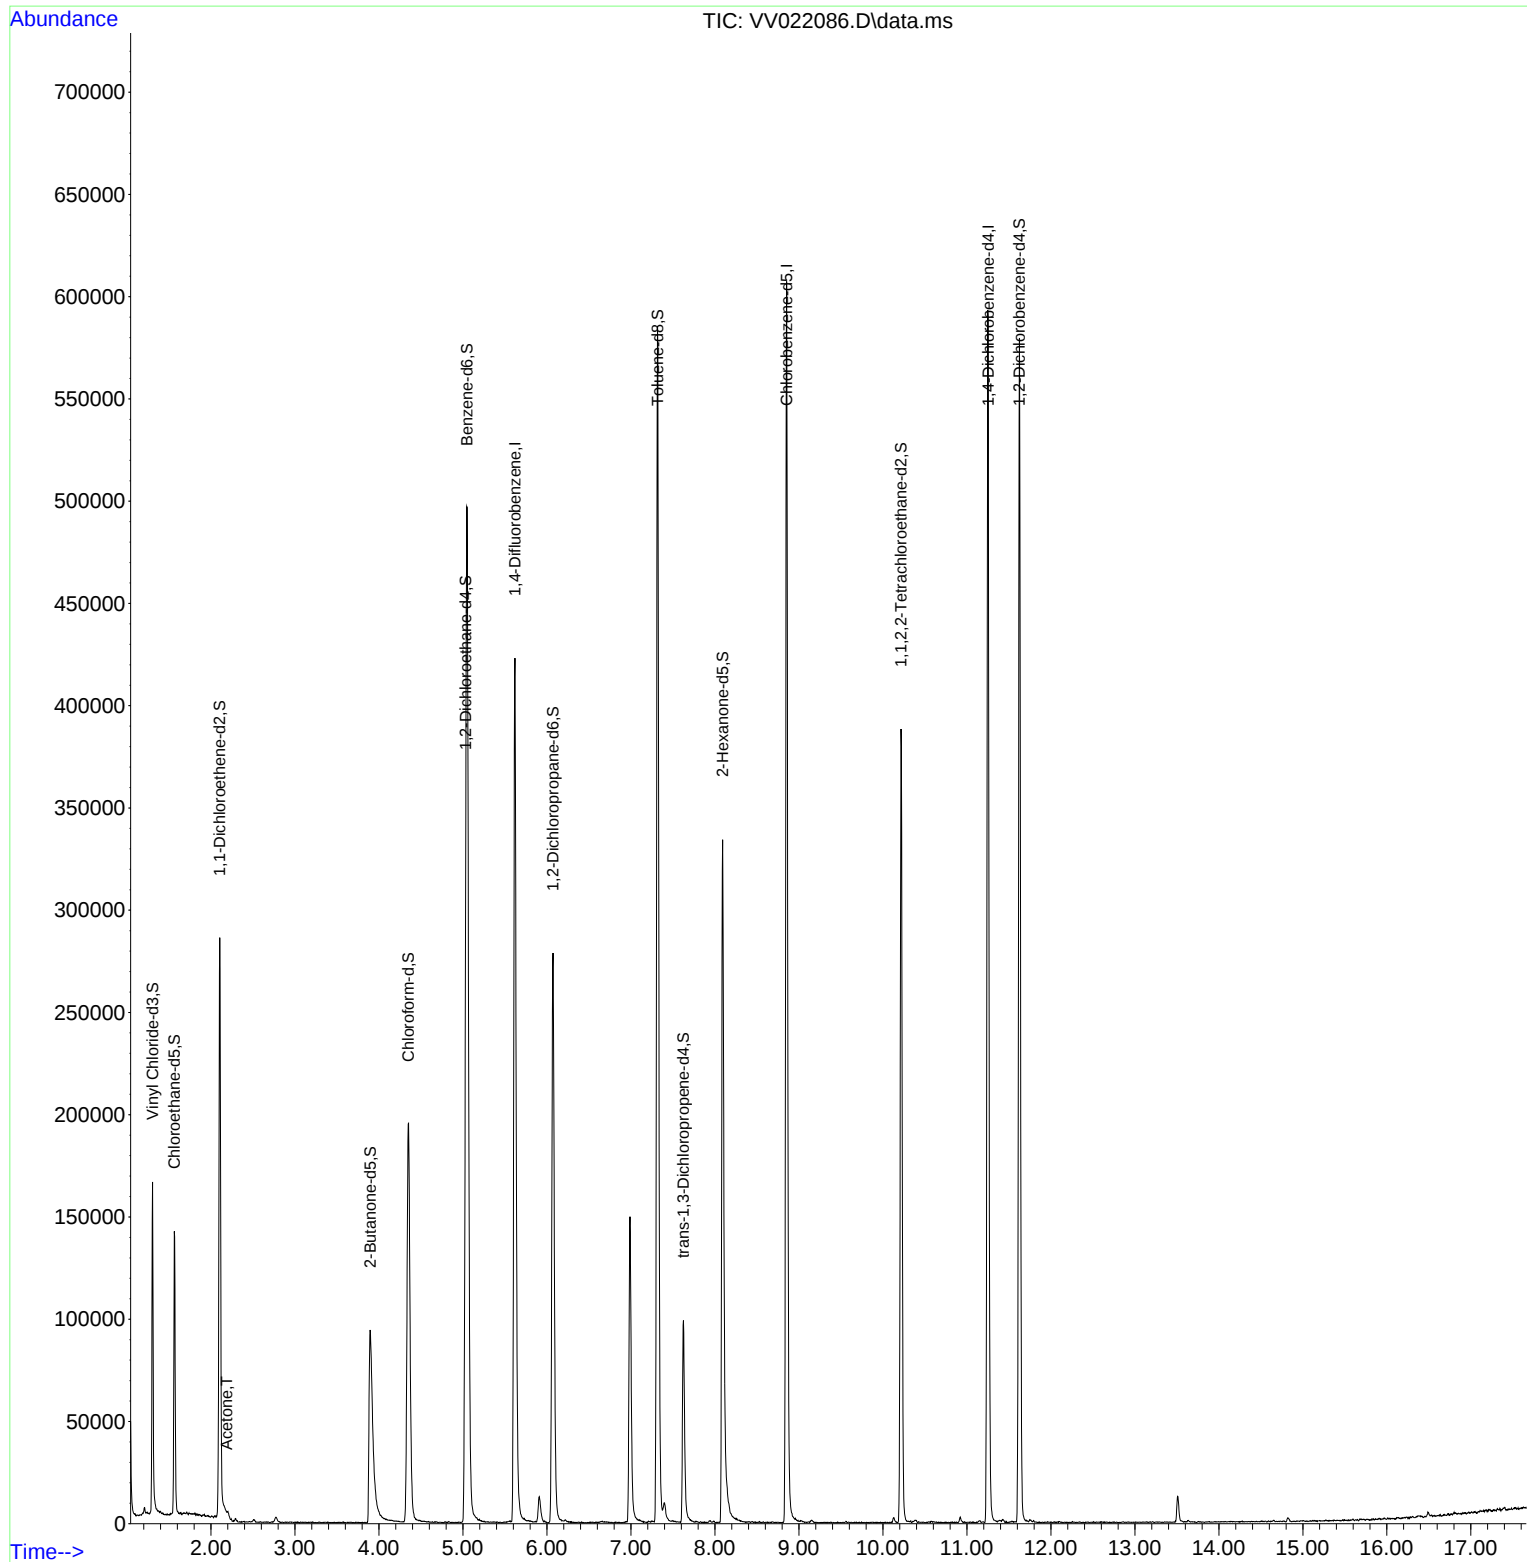

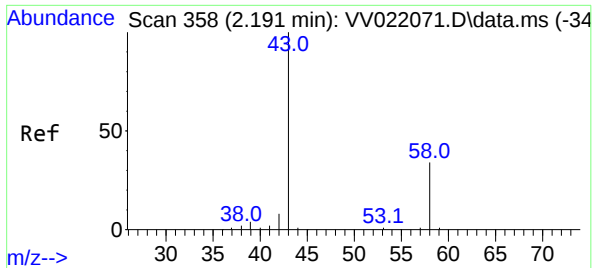

#13
 Acetone
 Concen: 3.332 ug/L m
 RT: 2.188 min Scan# 357
 Delta R.T. -0.003 min
 Lab File: VV022086.D
 Acq: 02 Sep 2021 19:24

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL1

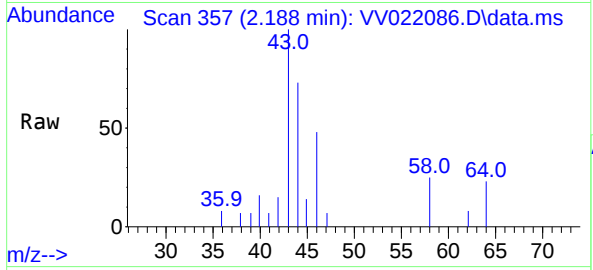

Tgt Ion: 43 Resp: 5055

Ion	Ratio	Lower	Upper
43	100		
58	11.7	0.0	0.4#

Manual Integrations
 APPROVED
 MMDadoda
 9/7/2021 8:50:06 AM

