

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022087.D
 Acq On : 02 Sep 2021 19:48
 Operator : SY/MD
 Sample : M3608-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL2

Quant Time: Sep 03 01:03:47 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 03 00:59:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	382527	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	354701	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	167510	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	102830	38.818	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.640%		
7) Chloroethane-d5	1.564	69	84129	40.667	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.340%		
11) 1,1-Dichloroethene-d2	2.105	63	146904	33.532	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.060%		
21) 2-Butanone-d5	3.896	46	181277	99.780	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	99.780%		
24) Chloroform-d	4.352	84	207973	43.056	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.120%		
26) 1,2-Dichloroethane-d4	5.034	65	131049	46.061	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.120%		
32) Benzene-d6	5.053	84	438465	45.575	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.160%		
36) 1,2-Dichloropropane-d6	6.072	67	137315	45.385	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	90.760%		
41) Toluene-d8	7.317	98	393610	43.341	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.680%		
43) trans-1,3-Dichloroprop...	7.625	79	58029	40.296	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.600%		
47) 2-Hexanone-d5	8.091	63	122504	105.524	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	105.520%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	187571	48.406	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	96.820%		
66) 1,2-Dichlorobenzene-d4	11.625	152	153668	46.664	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.320%		
Target Compounds					Qvalue	
13) Acetone	2.185	43	13908	9.137	ug/L	# 76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022087.D
Acq On : 02 Sep 2021 19:48
Operator : SY/MD
Sample : M3608-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL2

Quant Time: Sep 03 01:03:47 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 03 00:59:14 2021
Response via : Initial Calibration

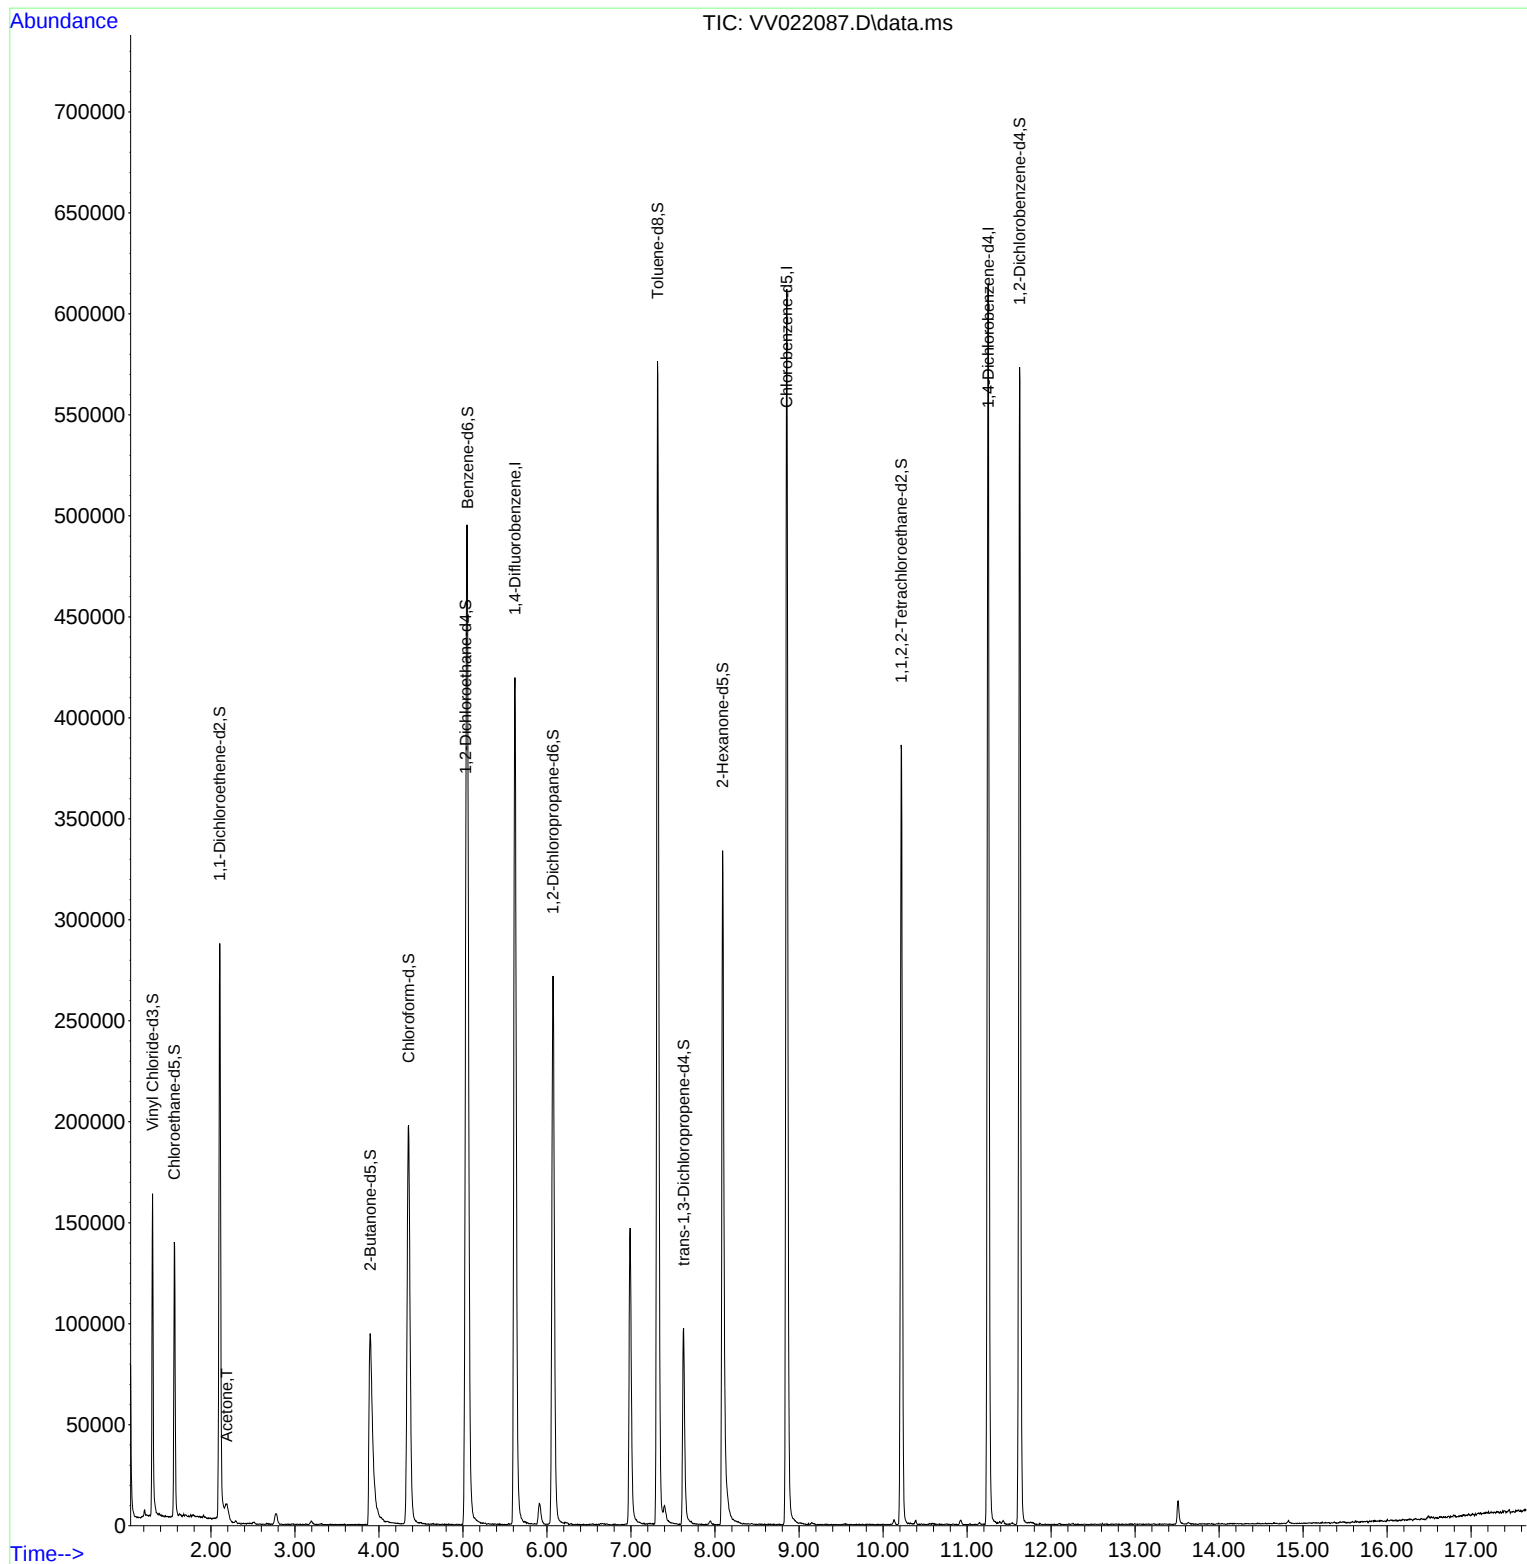

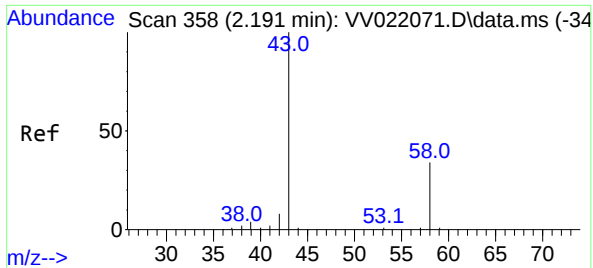

#13
Acetone
Concen: 9.137 ug/L
RT: 2.185 min Scan# 356
Delta R.T. -0.006 min
Lab File: VV022087.D
Acq: 02 Sep 2021 19:48

Instrument :
MSVOA_V
ClientSampleId :
DBKL2

Tgt Ion: 43 Resp: 13908
Ion Ratio Lower Upper
43 100
58 30.8 0.0 0.4#

