

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022091.D
 Acq On : 02 Sep 2021 22:13
 Operator : SY/MD
 Sample : M3647-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3W30

Quant Time: Sep 03 01:04:40 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Sep 03 00:59:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	374090	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	345491	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	159463	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	100548	38.812	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.620%		
7) Chloroethane-d5	1.564	69	82659	40.858	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	81.720%		
11) 1,1-Dichloroethene-d2	2.105	63	141788	33.094	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.180%		
21) 2-Butanone-d5	3.896	46	180677	101.693	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	101.690%		
24) Chloroform-d	4.349	84	203566	43.094	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.180%		
26) 1,2-Dichloroethane-d4	5.034	65	128134	46.052	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.100%		
32) Benzene-d6	5.053	84	427040	45.571	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.140%		
36) 1,2-Dichloropropane-d6	6.072	67	135238	45.890	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	91.780%		
41) Toluene-d8	7.317	98	381709	43.151	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	86.300%		
43) trans-1,3-Dichloroprop...	7.625	79	56347	40.171	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.340%		
47) 2-Hexanone-d5	8.092	63	113035	99.963	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	99.960%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	175025	46.373	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.740%		
66) 1,2-Dichlorobenzene-d4	11.625	152	148687	47.430	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.860%		
Target Compounds					Qvalue	
13) Acetone	2.185	43	20264	13.612	ug/L	# 74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022091.D
Acq On : 02 Sep 2021 22:13
Operator : SY/MD
Sample : M3647-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F3W30


Quant Time: Sep 03 01:04:40 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Sep 03 00:59:14 2021
Response via : Initial Calibration

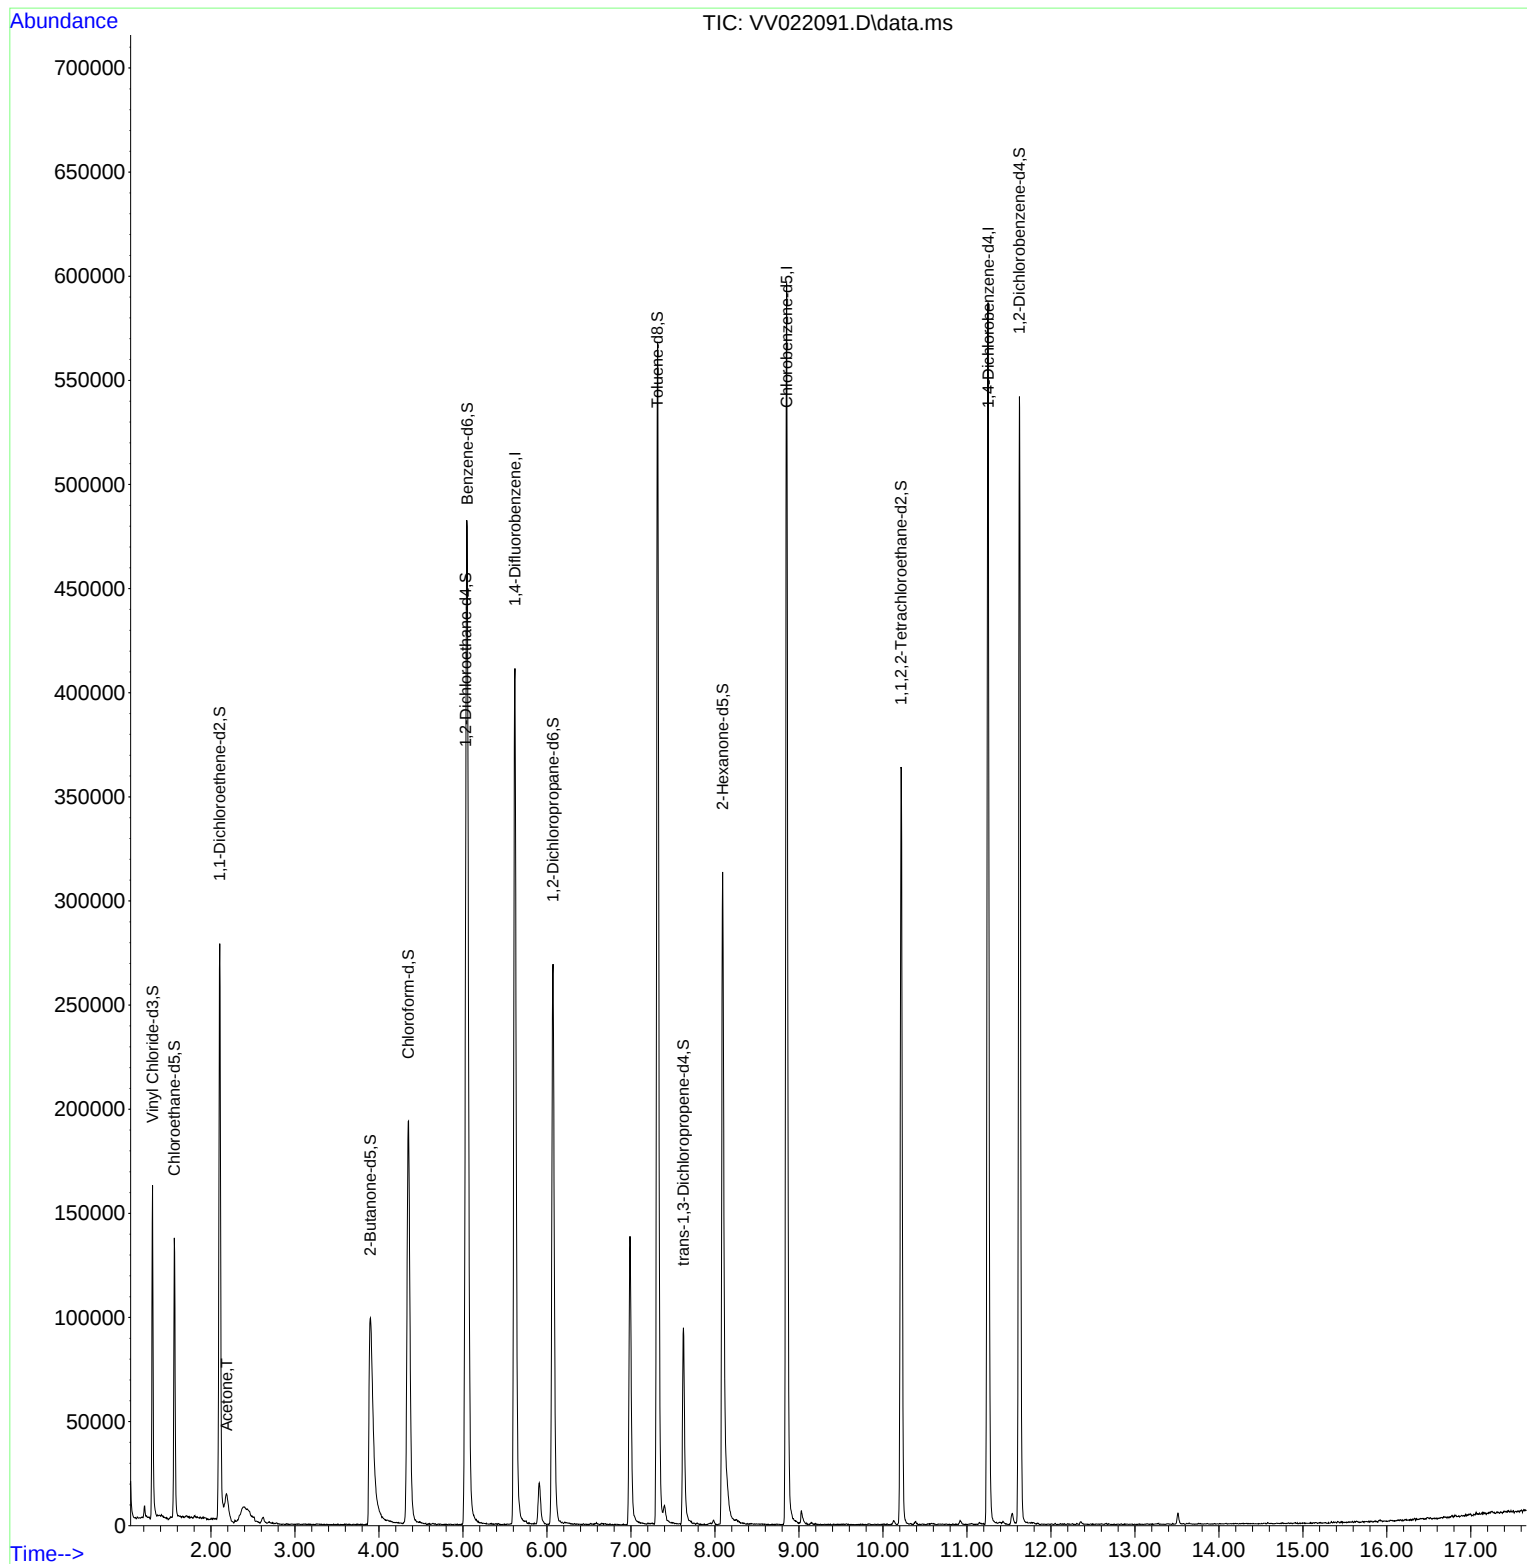

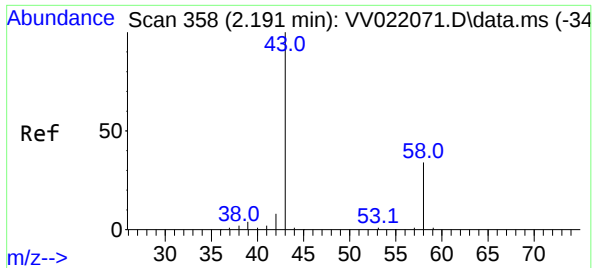

#13
Acetone
Concen: 13.612 ug/L
RT: 2.185 min Scan# 356
Delta R.T. -0.006 min
Lab File: VV022091.D
Acq: 02 Sep 2021 22:13

Instrument :
MSVOA_V
ClientSampleId :
F3W30

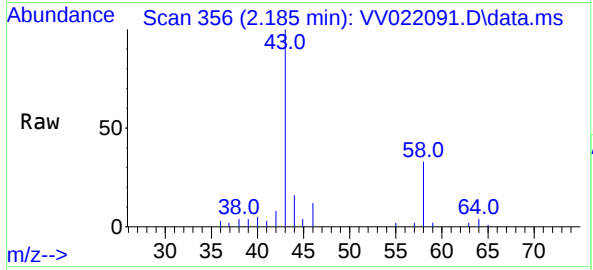

Tgt Ion: 43 Resp: 20264
Ion Ratio Lower Upper
43 100
58 34.1 0.0 0.4#

