

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022072.D
 Acq On : 02 Sep 2021 13:49
 Operator : SY/MD
 Sample : VV0902MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022072.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rBV	173771	177565	14.15%	1.859%
2	1.564	156	163	175	rVB	146997	165873	13.22%	1.737%
3	2.105	321	331	346	rBV	271197	387045	30.84%	4.052%
4	2.507	447	456	466	rVB4	5656	9118	0.73%	0.095%
5	2.680	507	510	518	rBV3	311	397	0.03%	0.004%
6	2.761	527	535	538	rBV4	855	1161	0.09%	0.012%
7	2.847	560	562	565	rBV	376	161	0.01%	0.002%
8	2.908	578	581	582	rBV	296	184	0.01%	0.002%
9	3.298	699	702	707	rBV3	363	239	0.02%	0.003%
10	3.323	707	710	711	rBV	303	185	0.01%	0.002%
11	3.400	732	734	739	rVB2	368	233	0.02%	0.002%
12	3.429	740	743	747	rBV	265	206	0.02%	0.002%
13	3.519	767	771	778	rVB3	307	375	0.03%	0.004%
14	3.577	783	789	792	rBV	227	304	0.02%	0.003%
15	3.609	795	799	802	rVV3	327	215	0.02%	0.002%
16	3.625	802	804	807	rVV	337	154	0.01%	0.002%
17	3.648	807	811	814	rVB	383	250	0.02%	0.003%
18	3.667	814	817	820	rVB3	302	148	0.01%	0.002%
19	3.687	820	823	827	rBV2	216	237	0.02%	0.002%
20	3.728	834	836	839	rBV2	223	139	0.01%	0.001%
21	3.905	880	891	927	rBV	66448	267049	21.28%	2.796%
22	4.349	1012	1029	1058	rBV	198411	495685	39.50%	5.190%
23	4.651	1119	1123	1127	rVB2	814	561	0.04%	0.006%
24	4.789	1163	1166	1170	rVB2	447	280	0.02%	0.003%
25	4.870	1189	1191	1193	rBV	244	167	0.01%	0.002%
26	4.976	1221	1224	1225	rBV	280	148	0.01%	0.002%
27	5.047	1228	1246	1275	rBV2	494655	1255017	100.00%	13.140%
28	5.561	1404	1406	1409	rVB	396	185	0.01%	0.002%
29	5.616	1409	1423	1454	rBV	387035	783955	62.47%	8.208%
30	5.777	1471	1473	1476	rBV2	671	351	0.03%	0.004%
31	5.908	1503	1514	1529	rBV3	16276	35143	2.80%	0.368%
32	6.069	1550	1564	1594	rBV	269294	558436	44.50%	5.847%
33	6.400	1665	1667	1671	rVB2	410	232	0.02%	0.002%
34	6.452	1681	1683	1687	rBV	216	154	0.01%	0.002%
35	6.526	1704	1706	1710	rBV3	322	191	0.02%	0.002%
36	6.603	1726	1730	1733	rBV3	176	167	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022072.D
 Acq On : 02 Sep 2021 13:49
 Operator : SY/MD
 Sample : VV0902MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.625	1736	1737	1740	rVB2	315	136	0.01%	0.001%
38	6.645	1740	1743	1746	rBV2	467	265	0.02%	0.003%
39	6.664	1746	1749	1751	rBV	474	301	0.02%	0.003%
40	6.696	1757	1759	1764	rVB3	567	311	0.02%	0.003%
41	6.731	1768	1770	1773	rVB2	269	138	0.01%	0.001%
42	6.754	1773	1777	1781	rBV3	345	265	0.02%	0.003%
43	6.783	1782	1786	1789	rBV	319	213	0.02%	0.002%
44	6.944	1834	1836	1839	rBV	309	163	0.01%	0.002%
45	6.985	1839	1849	1885	rVV	149882	283180	22.56%	2.965%
46	7.317	1939	1952	1970	rBV	577695	1012775	80.70%	10.603%
47	7.622	2036	2047	2074	rBV2	102966	184409	14.69%	1.931%
48	7.976	2152	2157	2158	rBV2	688	346	0.03%	0.004%
49	8.011	2165	2168	2170	rBV2	226	162	0.01%	0.002%
50	8.092	2182	2193	2230	rBV	291634	585797	46.68%	6.133%
51	8.625	2355	2359	2360	rBV2	551	387	0.03%	0.004%
52	8.854	2419	2430	2458	rBV	560731	920372	73.34%	9.636%
53	9.153	2512	2523	2529	rBV6	1315	2210	0.18%	0.023%
54	9.297	2564	2568	2571	rBV	522	333	0.03%	0.003%
55	9.362	2585	2588	2591	rVV3	416	237	0.02%	0.002%
56	9.551	2641	2647	2648	rBV2	598	504	0.04%	0.005%
57	9.577	2653	2655	2657	rBV	483	327	0.03%	0.003%
58	9.628	2669	2671	2674	rBV	404	194	0.02%	0.002%
59	9.715	2694	2698	2701	rVB3	357	266	0.02%	0.003%
60	9.821	2727	2731	2736	rBV2	358	339	0.03%	0.004%
61	9.844	2736	2738	2741	rVB2	320	172	0.01%	0.002%
62	9.886	2745	2751	2752	rBV2	180	185	0.01%	0.002%
63	9.934	2762	2766	2768	rBV3	508	464	0.04%	0.005%
64	10.001	2785	2787	2791	rBV2	275	135	0.01%	0.001%
65	10.030	2793	2796	2797	rBV	316	179	0.01%	0.002%
66	10.079	2809	2811	2814	rVV2	232	141	0.01%	0.001%
67	10.130	2819	2827	2835	rVV7	2388	3549	0.28%	0.037%
68	10.217	2842	2854	2875	rBV	368960	579324	46.16%	6.065%
69	10.390	2904	2908	2914	rVB3	700	710	0.06%	0.007%
70	10.416	2914	2916	2922	rVB	379	238	0.02%	0.002%
71	10.474	2931	2934	2938	rBV2	613	465	0.04%	0.005%
72	10.644	2983	2987	2989	rBV	356	199	0.02%	0.002%
73	10.693	2997	3002	3006	rVV4	472	452	0.04%	0.005%
74	10.725	3009	3012	3016	rVB2	331	230	0.02%	0.002%
75	10.792	3031	3033	3035	rBV2	195	137	0.01%	0.001%
76	10.828	3039	3044	3048	rBV3	417	488	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022072.D
 Acq On : 02 Sep 2021 13:49
 Operator : SY/MD
 Sample : VV0902MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK249

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.882	3059	3061	3062	rBV	403	186	0.01%	0.002%
78	10.924	3067	3074	3084	rVB8	3738	5601	0.45%	0.059%
79	11.069	3116	3119	3123	rBV	278	229	0.02%	0.002%
80	11.149	3135	3144	3150	rBV3	1215	1611	0.13%	0.017%
81	11.185	3150	3155	3157	rBV2	1503	1453	0.12%	0.015%
82	11.249	3164	3175	3196	rBV	570302	882687	70.33%	9.241%
83	11.554	3266	3270	3272	rBV2	602	355	0.03%	0.004%
84	11.625	3280	3292	3317	rVV	570497	893011	71.16%	9.350%
85	11.747	3327	3330	3335	rBV3	622	539	0.04%	0.006%
86	11.947	3390	3392	3393	rBV	359	136	0.01%	0.001%
87	12.001	3406	3409	3411	rBV	288	179	0.01%	0.002%
88	12.191	3467	3468	3471	rVB2	353	147	0.01%	0.002%
89	12.297	3497	3501	3504	rVB2	455	303	0.02%	0.003%
90	12.313	3504	3506	3509	rBV	284	179	0.01%	0.002%
91	12.509	3565	3567	3570	rVB	434	186	0.01%	0.002%
92	12.525	3570	3572	3575	rBV2	271	147	0.01%	0.002%
93	12.651	3603	3611	3621	rBV8	2907	5007	0.40%	0.052%
94	12.802	3655	3658	3662	rBV	326	321	0.03%	0.003%
95	12.918	3690	3694	3695	rBV2	377	276	0.02%	0.003%
96	13.033	3728	3730	3734	rBV3	466	256	0.02%	0.003%
97	13.075	3740	3743	3745	rBV	397	236	0.02%	0.002%
98	13.268	3795	3803	3815	rVB7	4897	7481	0.60%	0.078%
99	13.509	3870	3878	3892	rBV	13030	20520	1.64%	0.215%
100	13.750	3945	3953	3959	rBV3	5110	7696	0.61%	0.081%




Sum of corrected areas: 9551350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022072.D
Acq On : 02 Sep 2021 13:49
Operator : SY/MD
Sample : VV0902MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

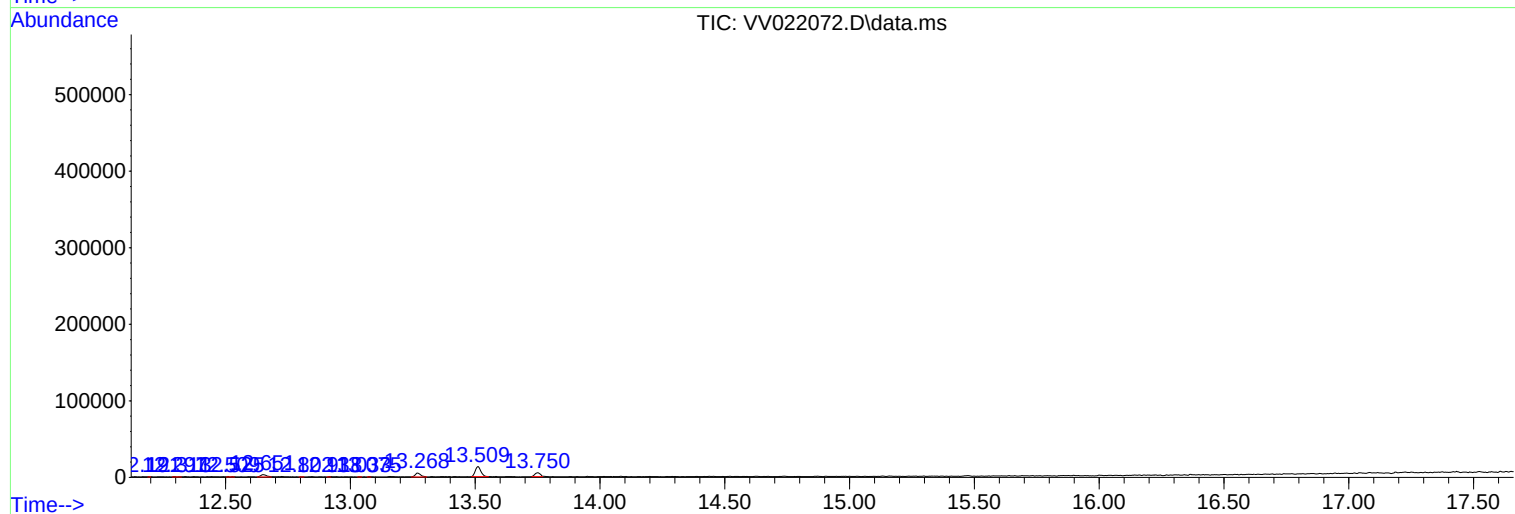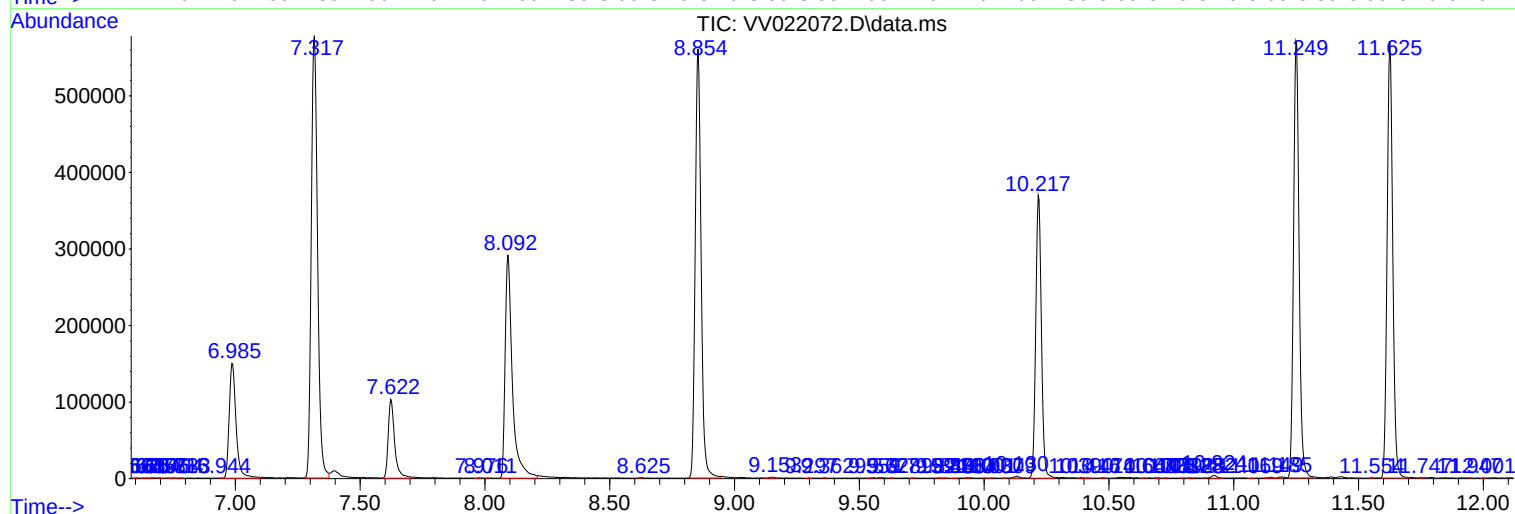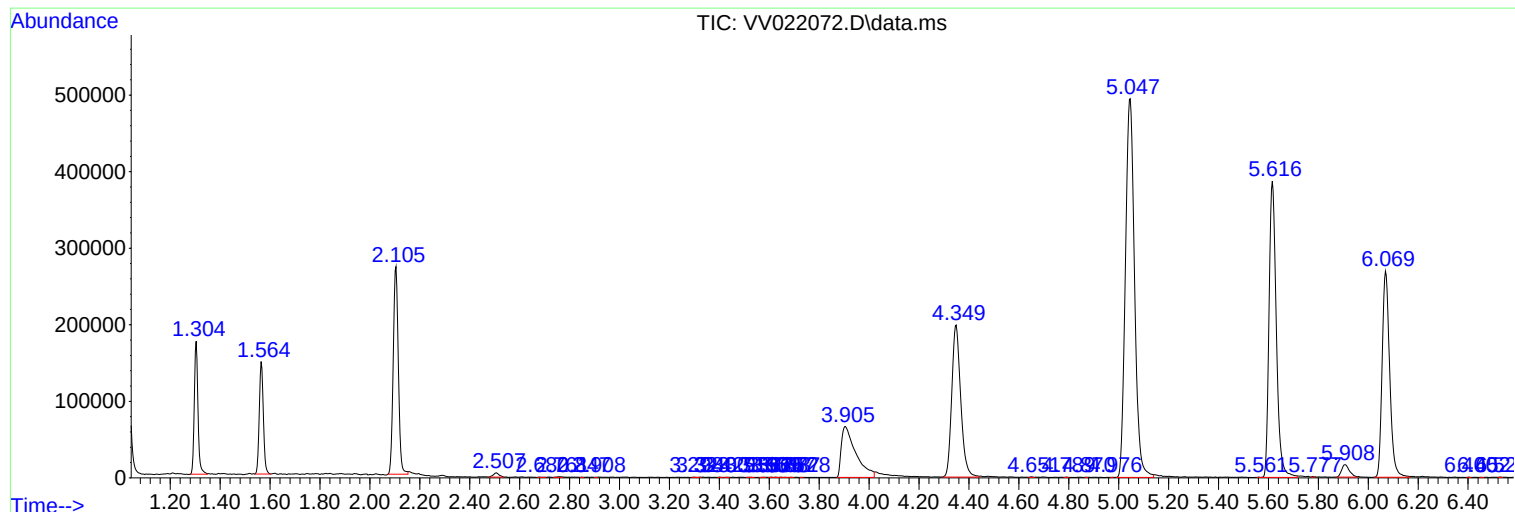

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022072.D
Acq On : 02 Sep 2021 13:49
Operator : SY/MD
Sample : VV0902MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022072.D
Acq On : 02 Sep 2021 13:49
Operator : SY/MD
Sample : VV0902MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK249

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
