

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022073.D
 Acq On : 02 Sep 2021 14:11
 Operator : SY/MD
 Sample : VV0902WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022073.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	104	rVB	158483	167086	13.69%	1.793%
2	1.568	157	164	180	rVB	139126	157428	12.90%	1.689%
3	2.105	322	331	346	rBV	259406	370849	30.39%	3.979%
4	2.477	445	447	449	rBV	409	249	0.02%	0.003%
5	2.506	449	456	468	rVB3	5939	9668	0.79%	0.104%
6	2.593	481	483	488	rVB2	515	325	0.03%	0.003%
7	2.619	488	491	494	rBV3	295	226	0.02%	0.002%
8	2.693	511	514	517	rVB	374	185	0.02%	0.002%
9	2.728	522	525	528	rVB3	779	419	0.03%	0.004%
10	2.902	576	579	583	rBV2	387	274	0.02%	0.003%
11	3.079	628	634	636	rBV3	270	274	0.02%	0.003%
12	3.410	733	737	739	rBV	423	185	0.02%	0.002%
13	3.432	740	744	745	rBV3	419	179	0.01%	0.002%
14	3.503	763	766	772	rBV2	165	166	0.01%	0.002%
15	3.751	839	843	847	rVB	398	279	0.02%	0.003%
16	3.780	847	852	857	rBV2	179	179	0.01%	0.002%
17	3.809	857	861	865	rBV3	285	288	0.02%	0.003%
18	3.908	881	892	940	rBV	74880	297318	24.36%	3.190%
19	4.355	1016	1031	1060	rVB	190453	474533	38.89%	5.092%
20	4.632	1115	1117	1120	rBV2	314	226	0.02%	0.002%
21	4.683	1131	1133	1136	rBV	342	204	0.02%	0.002%
22	4.841	1177	1182	1184	rBV2	314	205	0.02%	0.002%
23	4.924	1205	1208	1211	rBV2	407	290	0.02%	0.003%
24	5.050	1231	1247	1273	rBV2	481243	1220317	100.00%	13.094%
25	5.339	1335	1337	1340	rVB2	341	179	0.01%	0.002%
26	5.355	1340	1342	1348	rVB3	699	306	0.03%	0.003%
27	5.468	1374	1377	1382	rBV2	209	187	0.02%	0.002%
28	5.493	1382	1385	1388	rBV2	319	216	0.02%	0.002%
29	5.529	1394	1396	1400	rVB	279	170	0.01%	0.002%
30	5.555	1402	1404	1408	rVB2	398	181	0.01%	0.002%
31	5.622	1411	1425	1453	rBV	374303	753353	61.73%	8.083%
32	5.911	1503	1515	1534	rBV2	17190	37147	3.04%	0.399%
33	6.075	1549	1566	1595	rBV	269523	554625	45.45%	5.951%
34	6.336	1644	1647	1649	rBV2	386	205	0.02%	0.002%
35	6.349	1649	1651	1658	rVV3	284	176	0.01%	0.002%
36	6.384	1660	1662	1665	rVV2	330	170	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022073.D
 Acq On : 02 Sep 2021 14:11
 Operator : SY/MD
 Sample : VV0902WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.400	1665	1667	1671	rVB2	421	291	0.02%	0.003%
38	6.429	1671	1676	1680	rBV2	353	307	0.03%	0.003%
39	6.490	1690	1695	1697	rBV2	239	180	0.01%	0.002%
40	6.542	1703	1711	1713	rBV2	424	484	0.04%	0.005%
41	6.628	1736	1738	1742	rVB2	300	164	0.01%	0.002%
42	6.670	1746	1751	1752	rBV2	470	389	0.03%	0.004%
43	6.770	1779	1782	1785	rBV4	271	214	0.02%	0.002%
44	6.834	1797	1802	1804	rBV2	180	163	0.01%	0.002%
45	6.992	1838	1851	1876	rBV	149912	273587	22.42%	2.936%
46	7.320	1940	1953	1972	rBV	571243	981944	80.47%	10.536%
47	7.625	2037	2048	2070	rBV	98885	178100	14.59%	1.911%
48	7.812	2104	2106	2109	rVB2	552	257	0.02%	0.003%
49	7.834	2110	2113	2117	rVV3	450	381	0.03%	0.004%
50	7.863	2120	2122	2125	rVV2	590	239	0.02%	0.003%
51	7.953	2148	2150	2152	rVB2	439	179	0.01%	0.002%
52	8.095	2184	2194	2228	rBV	309577	603850	49.48%	6.479%
53	8.426	2295	2297	2300	rVB3	446	174	0.01%	0.002%
54	8.670	2372	2373	2377	rVB	327	165	0.01%	0.002%
55	8.805	2409	2415	2417	rBV3	258	232	0.02%	0.002%
56	8.853	2418	2430	2457	rBV	549450	898456	73.62%	9.640%
57	9.095	2503	2505	2507	rBV2	236	162	0.01%	0.002%
58	9.156	2519	2524	2526	rBV2	677	607	0.05%	0.007%
59	9.223	2543	2545	2551	rVB2	415	291	0.02%	0.003%
60	9.252	2551	2554	2556	rBV	243	154	0.01%	0.002%
61	9.307	2567	2571	2574	rBV2	265	205	0.02%	0.002%
62	9.342	2579	2582	2587	rVB2	198	158	0.01%	0.002%
63	9.374	2587	2592	2597	rBV	289	337	0.03%	0.004%
64	9.406	2600	2602	2606	rBV2	431	186	0.02%	0.002%
65	9.461	2615	2619	2625	rVB	357	301	0.02%	0.003%
66	9.493	2625	2629	2631	rBV2	221	161	0.01%	0.002%
67	9.551	2644	2647	2651	rBV3	418	318	0.03%	0.003%
68	9.654	2672	2679	2681	rBV	253	282	0.02%	0.003%
69	10.130	2820	2827	2837	rVV3	3004	4600	0.38%	0.049%
70	10.220	2843	2855	2876	rBV	366294	580868	47.60%	6.233%
71	10.377	2901	2904	2906	rBV2	388	258	0.02%	0.003%
72	10.432	2919	2921	2926	rVB2	420	289	0.02%	0.003%
73	10.461	2926	2930	2931	rBV2	372	256	0.02%	0.003%
74	10.525	2948	2950	2952	rBV	292	169	0.01%	0.002%
75	10.577	2960	2966	2974	rBV5	828	1491	0.12%	0.016%
76	10.667	2989	2994	2996	rBV2	477	423	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022073.D
 Acq On : 02 Sep 2021 14:11
 Operator : SY/MD
 Sample : VV0902WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK250

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.808	3036	3038	3044	rBV2	299	258	0.02%	0.003%
78	10.837	3044	3047	3050	rBV2	299	262	0.02%	0.003%
79	10.873	3056	3058	3062	rVB2	236	180	0.01%	0.002%
80	10.921	3062	3073	3082	rBV5	2819	4291	0.35%	0.046%
81	10.985	3091	3093	3097	rBV2	348	270	0.02%	0.003%
82	11.043	3106	3111	3115	rVV4	667	665	0.05%	0.007%
83	11.149	3137	3144	3147	rBV6	1137	1414	0.12%	0.015%
84	11.188	3153	3156	3159	rBV4	762	604	0.05%	0.006%
85	11.252	3163	3176	3202	rBV	549631	856392	70.18%	9.189%
86	11.529	3260	3262	3264	rBV2	291	156	0.01%	0.002%
87	11.625	3281	3292	3311	rBV	550711	865491	70.92%	9.287%
88	11.844	3357	3360	3361	rBV2	321	179	0.01%	0.002%
89	11.930	3385	3387	3391	rVB2	405	261	0.02%	0.003%
90	12.017	3411	3414	3417	rVB2	354	196	0.02%	0.002%
91	12.085	3432	3435	3437	rBV	315	221	0.02%	0.002%
92	12.239	3480	3483	3486	rVB2	327	212	0.02%	0.002%
93	12.651	3607	3611	3613	rBV3	665	508	0.04%	0.005%
94	12.773	3644	3649	3651	rBV	257	275	0.02%	0.003%
95	12.998	3715	3719	3726	rBV2	277	304	0.02%	0.003%
96	13.130	3757	3760	3762	rBV3	287	185	0.02%	0.002%
97	13.152	3764	3767	3769	rVB2	256	154	0.01%	0.002%
98	13.175	3769	3774	3775	rBV	275	234	0.02%	0.003%
99	13.516	3870	3880	3888	rBV2	4470	7216	0.59%	0.077%
100	13.718	3941	3943	3945	rBV	382	180	0.01%	0.002%




Sum of corrected areas: 9319647

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022073.D
Acq On : 02 Sep 2021 14:11
Operator : SY/MD
Sample : VV0902WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

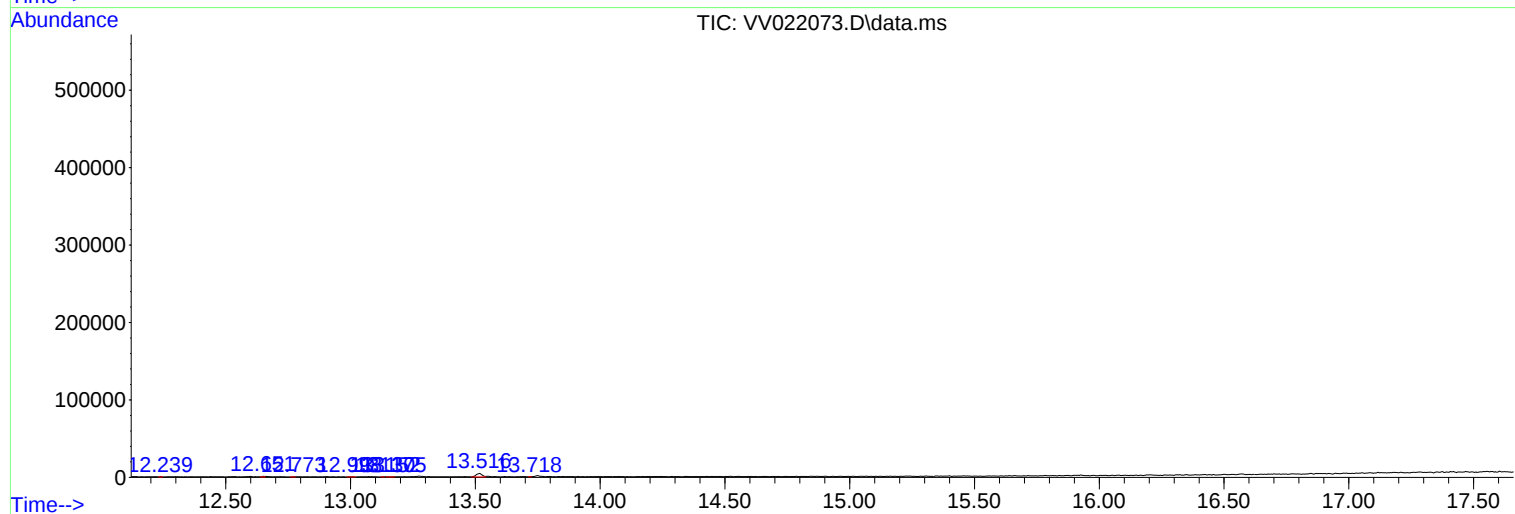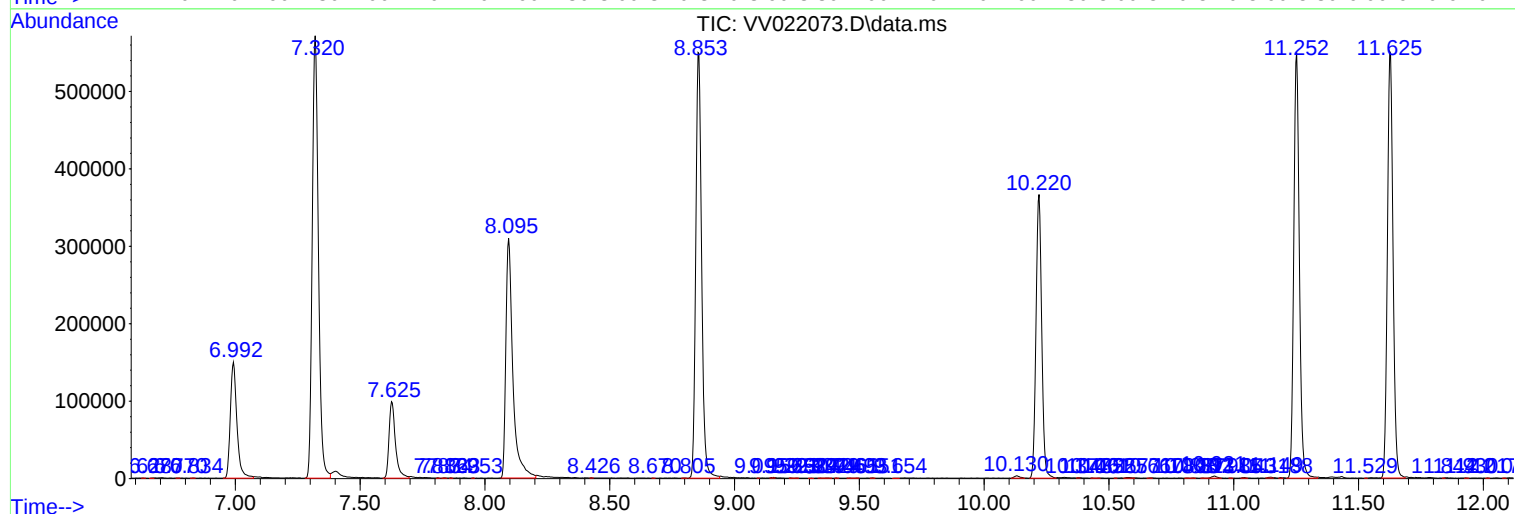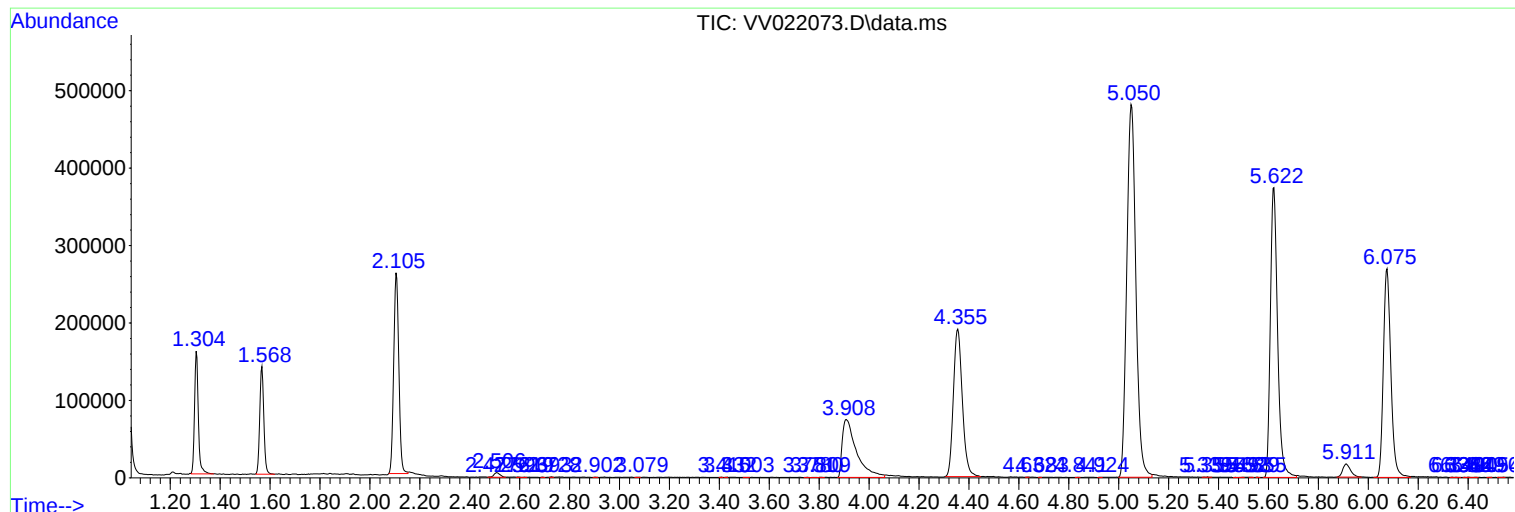

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022073.D
Acq On : 02 Sep 2021 14:11
Operator : SY/MD
Sample : VV0902WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022073.D
Acq On : 02 Sep 2021 14:11
Operator : SY/MD
Sample : VV0902WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK250

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
