

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\V090221\
 Data File : VV022085.D
 Acq On : 02 Sep 2021 19:00
 Operator : SY/MD
 Sample : M3608-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022085.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	167128	168601	13.44%	1.723%
2	1.564	156	163	181	rVB	137707	152873	12.19%	1.562%
3	2.105	322	331	356	rVB	283786	416261	33.18%	4.253%
4	2.555	468	471	474	rBV2	324	207	0.02%	0.002%
5	2.671	505	507	510	rBV	229	147	0.01%	0.002%
6	2.767	529	537	550	rVB7	2267	4844	0.39%	0.049%
7	2.998	607	609	614	rBV2	157	139	0.01%	0.001%
8	3.040	620	622	624	rBV	308	181	0.01%	0.002%
9	3.134	647	651	655	rBV	272	234	0.02%	0.002%
10	3.362	718	722	725	rVB	268	225	0.02%	0.002%
11	3.388	725	730	731	rBV	198	132	0.01%	0.001%
12	3.445	743	748	751	rBV2	143	155	0.01%	0.002%
13	3.555	779	782	785	rVB2	231	155	0.01%	0.002%
14	3.590	789	793	796	rVB3	206	131	0.01%	0.001%
15	3.613	797	800	802	rBV	240	167	0.01%	0.002%
16	3.892	876	887	920	rBV	95196	286550	22.84%	2.928%
17	4.349	1013	1029	1061	rBV	196249	489793	39.04%	5.005%
18	4.580	1098	1101	1104	rBV2	263	200	0.02%	0.002%
19	4.651	1120	1123	1126	rBV	380	182	0.01%	0.002%
20	4.696	1132	1137	1140	rVB	249	189	0.02%	0.002%
21	4.744	1149	1152	1155	rVB3	247	127	0.01%	0.001%
22	4.809	1169	1172	1174	rBV2	232	130	0.01%	0.001%
23	4.876	1190	1193	1196	rVB2	258	147	0.01%	0.002%
24	4.941	1207	1213	1216	rBV3	325	323	0.03%	0.003%
25	4.963	1218	1220	1226	rVB3	231	176	0.01%	0.002%
26	5.047	1229	1246	1274	rBV2	497179	1254459	100.00%	12.818%
27	5.323	1330	1332	1337	rVB3	342	218	0.02%	0.002%
28	5.349	1337	1340	1343	rVB3	395	284	0.02%	0.003%
29	5.375	1343	1348	1349	rBV3	345	267	0.02%	0.003%
30	5.439	1366	1368	1373	rVB2	232	175	0.01%	0.002%
31	5.490	1379	1384	1386	rBV	445	400	0.03%	0.004%
32	5.619	1411	1424	1451	rBV	420505	844224	67.30%	8.626%
33	5.912	1504	1515	1527	rBV3	10242	21218	1.69%	0.217%
34	6.072	1550	1565	1588	rBV	273232	562610	44.85%	5.749%
35	6.378	1654	1660	1662	rBV	252	303	0.02%	0.003%
36	6.410	1667	1670	1672	rBV	214	143	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022085.D
 Acq On : 02 Sep 2021 19:00
 Operator : SY/MD
 Sample : M3608-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.468	1685	1688	1691	rBV2	166	139	0.01%	0.001%
38	6.497	1695	1697	1701	rBV2	236	149	0.01%	0.002%
39	6.522	1701	1705	1706	rBV	206	146	0.01%	0.001%
40	6.641	1740	1742	1744	rVB3	342	134	0.01%	0.001%
41	6.699	1756	1760	1764	rVB2	403	185	0.01%	0.002%
42	6.818	1791	1797	1798	rBV2	179	130	0.01%	0.001%
43	6.866	1809	1812	1816	rVB2	279	180	0.01%	0.002%
44	6.940	1830	1835	1837	rBV2	355	323	0.03%	0.003%
45	6.989	1839	1850	1876	rBV	146525	270261	21.54%	2.762%
46	7.182	1905	1910	1913	rBV4	386	357	0.03%	0.004%
47	7.198	1913	1915	1919	rVB2	481	322	0.03%	0.003%
48	7.317	1941	1952	1970	rBV	592072	1022940	81.54%	10.452%
49	7.622	2038	2047	2066	rBV	98022	175184	13.96%	1.790%
50	7.889	2127	2130	2133	rVB	210	131	0.01%	0.001%
51	7.908	2134	2136	2139	rBV2	289	174	0.01%	0.002%
52	7.931	2139	2143	2145	rBV2	917	699	0.06%	0.007%
53	8.034	2170	2175	2177	rBV2	133	137	0.01%	0.001%
54	8.091	2182	2193	2235	rBV	325311	611218	48.72%	6.245%
55	8.616	2351	2356	2357	rBV2	228	162	0.01%	0.002%
56	8.635	2360	2362	2368	rVB2	278	189	0.02%	0.002%
57	8.715	2383	2387	2390	rVB2	229	195	0.02%	0.002%
58	8.738	2390	2394	2397	rBV	309	252	0.02%	0.003%
59	8.854	2418	2430	2451	rBV	612027	993864	79.23%	10.155%
60	9.063	2492	2495	2496	rBV	313	142	0.01%	0.001%
61	9.146	2515	2521	2526	rBV4	777	1059	0.08%	0.011%
62	9.201	2534	2538	2541	rVB2	281	175	0.01%	0.002%
63	9.272	2558	2560	2568	rVB2	433	335	0.03%	0.003%
64	9.310	2568	2572	2578	rBV3	320	341	0.03%	0.003%
65	9.426	2606	2608	2611	rBV2	296	166	0.01%	0.002%
66	9.542	2640	2644	2647	rBV3	268	217	0.02%	0.002%
67	9.632	2669	2672	2677	rBV2	281	184	0.01%	0.002%
68	9.699	2689	2693	2696	rVB2	377	257	0.02%	0.003%
69	9.831	2731	2734	2735	rBV	215	135	0.01%	0.001%
70	9.876	2745	2748	2752	rBV2	180	143	0.01%	0.001%
71	10.127	2818	2826	2834	rBV4	2215	3202	0.26%	0.033%
72	10.217	2842	2854	2879	rBV	391395	612226	48.80%	6.256%
73	10.381	2901	2905	2915	rVB4	1622	2308	0.18%	0.024%
74	10.580	2963	2967	2970	rBV4	679	730	0.06%	0.007%
75	10.664	2989	2993	3000	rBV2	304	346	0.03%	0.004%
76	10.773	3021	3027	3029	rBV	194	182	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022085.D
 Acq On : 02 Sep 2021 19:00
 Operator : SY/MD
 Sample : M3608-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.921	3064	3073	3082	rVB5	2408	4019	0.32%	0.041%
78	11.027	3103	3106	3107	rBV2	497	250	0.02%	0.003%
79	11.114	3129	3133	3135	rBV	414	291	0.02%	0.003%
80	11.143	3139	3142	3145	rBV4	975	815	0.06%	0.008%
81	11.249	3164	3175	3198	rBV	606346	938910	74.85%	9.594%
82	11.484	3245	3248	3251	rVB2	326	202	0.02%	0.002%
83	11.625	3279	3292	3317	rBV	581709	903040	71.99%	9.227%
84	11.831	3351	3356	3359	rBV2	178	204	0.02%	0.002%
85	11.850	3359	3362	3364	rBV3	534	286	0.02%	0.003%
86	11.908	3375	3380	3381	rBV	173	153	0.01%	0.002%
87	11.921	3381	3384	3386	rVV	606	304	0.02%	0.003%
88	11.947	3390	3392	3395	rVB2	455	181	0.01%	0.002%
89	12.140	3449	3452	3454	rVB	301	172	0.01%	0.002%
90	12.252	3482	3487	3489	rBV2	487	434	0.03%	0.004%
91	12.374	3522	3525	3529	rBV2	250	192	0.02%	0.002%
92	12.493	3559	3562	3569	rVB3	339	308	0.02%	0.003%
93	12.545	3575	3578	3581	rBV2	356	279	0.02%	0.003%
94	12.802	3655	3658	3660	rBV2	267	187	0.01%	0.002%
95	12.886	3682	3684	3687	rBV2	242	150	0.01%	0.002%
96	13.050	3732	3735	3738	rBV2	385	235	0.02%	0.002%
97	13.249	3795	3797	3802	rVB	266	171	0.01%	0.002%
98	13.509	3869	3878	3891	rBV	17603	29058	2.32%	0.297%
99	13.763	3952	3957	3960	rBV3	473	469	0.04%	0.005%
100	13.779	3960	3962	3967	rVV3	347	226	0.02%	0.002%




Sum of corrected areas: 9786725

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022085.D
Acq On : 02 Sep 2021 19:00
Operator : SY/MD
Sample : M3608-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

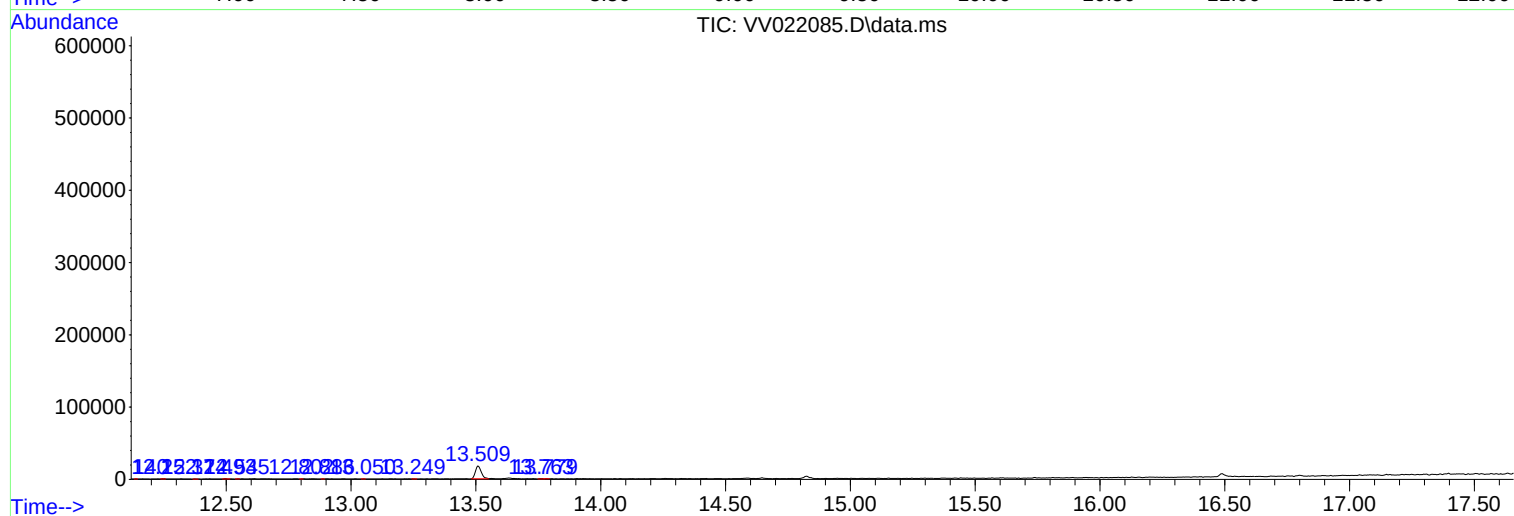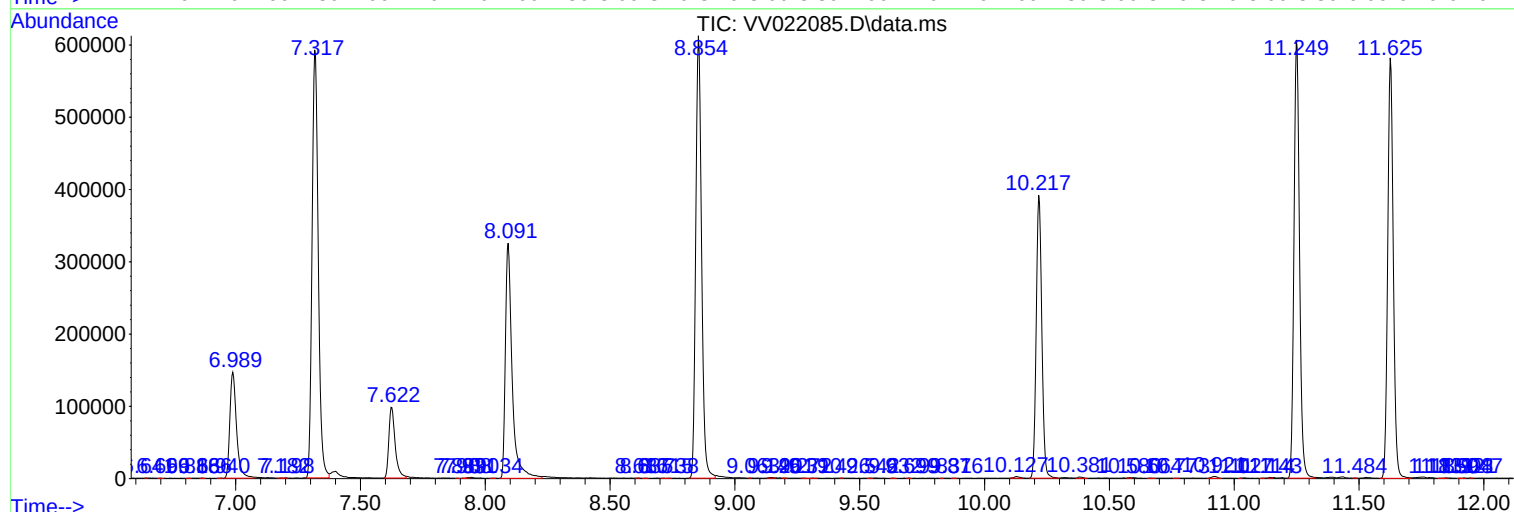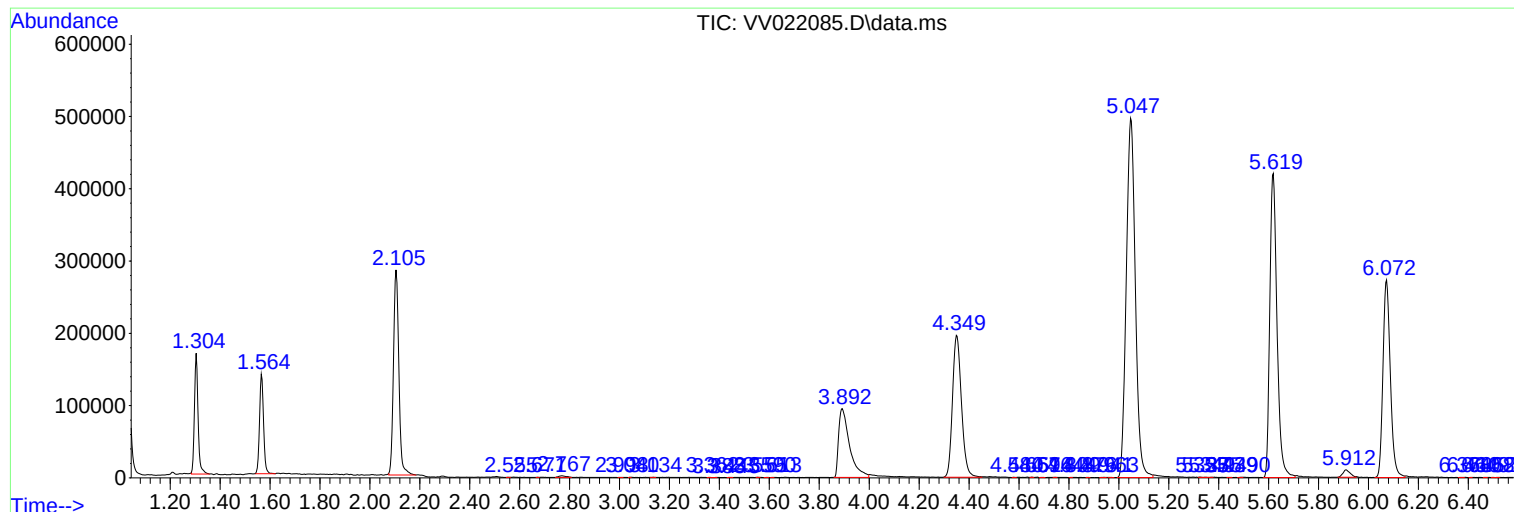

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022085.D
Acq On : 02 Sep 2021 19:00
Operator : SY/MD
Sample : M3608-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022085.D
Acq On : 02 Sep 2021 19:00
Operator : SY/MD
Sample : M3608-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
