

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022086.D
 Acq On : 02 Sep 2021 19:24
 Operator : SY/MD
 Sample : M3608-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M

Title : VOC Analysis

Signal : TIC: VV022086.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rBV	160307	161749	12.94%	1.656%
2	1.565	156	163	175	rBV	137645	154684	12.38%	1.583%
3	2.105	322	331	358	rVB	280948	407146	32.58%	4.167%
4	2.365	410	412	415	rBV2	296	124	0.01%	0.001%
5	2.774	528	539	551	rBV5	2480	5196	0.42%	0.053%
6	2.876	567	571	573	rBV	270	269	0.02%	0.003%
7	3.069	627	631	633	rBV	426	332	0.03%	0.003%
8	3.208	672	674	675	rBV	270	123	0.01%	0.001%
9	3.288	694	699	706	rVB3	309	373	0.03%	0.004%
10	3.696	821	826	830	rVB2	193	161	0.01%	0.002%
11	3.725	830	835	837	rBV2	313	224	0.02%	0.002%
12	3.860	872	877	878	rBV2	363	237	0.02%	0.002%
13	3.896	878	888	925	rBV2	94039	301562	24.13%	3.087%
14	4.352	1013	1030	1053	rBV	194878	488783	39.11%	5.003%
15	4.664	1125	1127	1129	rVB2	372	164	0.01%	0.002%
16	4.725	1140	1146	1149	rBV2	279	370	0.03%	0.004%
17	4.780	1159	1163	1164	rBV	396	235	0.02%	0.002%
18	4.825	1174	1177	1179	rBV	451	259	0.02%	0.003%
19	4.902	1199	1201	1203	rBV	306	172	0.01%	0.002%
20	4.947	1212	1215	1216	rBV	284	157	0.01%	0.002%
21	5.047	1230	1246	1281	rVV2	496443	1249608	100.00%	12.790%
22	5.442	1365	1369	1375	rVB3	294	313	0.03%	0.003%
23	5.484	1379	1382	1384	rBV2	266	171	0.01%	0.002%
24	5.526	1393	1395	1397	rBV2	363	198	0.02%	0.002%
25	5.619	1412	1424	1452	rBV	422097	835462	66.86%	8.551%
26	5.908	1504	1514	1531	rBV2	12380	26297	2.10%	0.269%
27	6.072	1549	1565	1591	rBV	278621	564511	45.18%	5.778%
28	6.291	1630	1633	1635	rVB3	552	320	0.03%	0.003%
29	6.310	1635	1639	1642	rBV3	377	286	0.02%	0.003%
30	6.407	1666	1669	1670	rBV	259	138	0.01%	0.001%
31	6.416	1670	1672	1674	rVB2	384	148	0.01%	0.002%
32	6.487	1688	1694	1698	rBV2	159	189	0.02%	0.002%
33	6.523	1703	1705	1708	rBV2	266	166	0.01%	0.002%
34	6.580	1721	1723	1726	rVV2	218	121	0.01%	0.001%
35	6.638	1737	1741	1742	rBV3	348	233	0.02%	0.002%
36	6.802	1790	1792	1795	rBV2	298	159	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022086.D
 Acq On : 02 Sep 2021 19:24
 Operator : SY/MD
 Sample : M3608-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.818	1795	1797	1800	rBV	288	181	0.01%	0.002%
38	6.851	1805	1807	1810	rVV	271	153	0.01%	0.002%
39	6.989	1839	1850	1877	rBV	149213	273440	21.88%	2.799%
40	7.150	1899	1900	1908	rVB2	447	325	0.03%	0.003%
41	7.198	1913	1915	1916	rBV2	359	162	0.01%	0.002%
42	7.246	1926	1930	1932	rBV	690	549	0.04%	0.006%
43	7.317	1940	1952	1970	rBV	584802	1013903	81.14%	10.378%
44	7.625	2037	2048	2073	rBV	98785	176539	14.13%	1.807%
45	7.831	2107	2112	2116	rVB4	563	530	0.04%	0.005%
46	7.873	2124	2125	2128	rBV	453	227	0.02%	0.002%
47	7.918	2135	2139	2140	rBV	215	168	0.01%	0.002%
48	7.934	2141	2144	2145	rBV2	651	372	0.03%	0.004%
49	8.092	2183	2193	2230	rBV	333750	629465	50.37%	6.443%
50	8.384	2282	2284	2285	rBV2	282	133	0.01%	0.001%
51	8.606	2350	2353	2356	rBV2	169	142	0.01%	0.001%
52	8.683	2374	2377	2378	rBV	328	199	0.02%	0.002%
53	8.854	2418	2430	2461	rBV	606744	984698	78.80%	10.079%
54	9.153	2515	2523	2530	rBV6	1232	2122	0.17%	0.022%
55	9.346	2580	2583	2585	rBV2	185	131	0.01%	0.001%
56	9.407	2600	2602	2608	rVB	157	133	0.01%	0.001%
57	9.461	2616	2619	2624	rBV2	377	263	0.02%	0.003%
58	9.522	2636	2638	2643	rVB2	200	159	0.01%	0.002%
59	9.561	2644	2650	2654	rVB3	689	673	0.05%	0.007%
60	9.590	2654	2659	2664	rBV2	299	338	0.03%	0.003%
61	9.809	2724	2727	2730	rBV	232	173	0.01%	0.002%
62	9.847	2735	2739	2742	rBV	333	217	0.02%	0.002%
63	9.973	2775	2778	2781	rVB	261	131	0.01%	0.001%
64	10.082	2809	2812	2817	rBV3	338	266	0.02%	0.003%
65	10.104	2817	2819	2821	rBV	381	207	0.02%	0.002%
66	10.130	2821	2827	2836	rVV4	2277	3261	0.26%	0.033%
67	10.217	2841	2854	2879	rBV	388084	614048	49.14%	6.285%
68	10.358	2894	2898	2899	rBV3	599	436	0.03%	0.004%
69	10.426	2917	2919	2925	rVB3	460	289	0.02%	0.003%
70	10.542	2952	2955	2956	rBV2	404	208	0.02%	0.002%
71	10.574	2962	2965	2970	rBV3	655	590	0.05%	0.006%
72	10.661	2989	2992	2997	rVB4	284	174	0.01%	0.002%
73	10.873	3055	3058	3061	rBV2	312	226	0.02%	0.002%
74	10.921	3065	3073	3084	rBV6	2779	4110	0.33%	0.042%
75	11.117	3131	3134	3136	rBV2	260	131	0.01%	0.001%
76	11.156	3137	3146	3150	rVB3	878	1428	0.11%	0.015%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022086.D
 Acq On : 02 Sep 2021 19:24
 Operator : SY/MD
 Sample : M3608-15
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	11.249	3164	3175	3203	rBV	592891	935732	74.88%	9.577%
78	11.465	3240	3242	3247	rVB3	528	292	0.02%	0.003%
79	11.535	3262	3264	3270	rVB3	573	436	0.03%	0.004%
80	11.558	3270	3271	3274	rBV3	275	153	0.01%	0.002%
81	11.625	3280	3292	3314	rBV	579046	896204	71.72%	9.173%
82	11.747	3326	3330	3332	rBV3	987	761	0.06%	0.008%
83	11.857	3360	3364	3365	rBV	274	158	0.01%	0.002%
84	11.866	3365	3367	3371	rVB2	317	166	0.01%	0.002%
85	11.963	3395	3397	3400	rBV	288	166	0.01%	0.002%
86	12.059	3425	3427	3430	rBV2	376	224	0.02%	0.002%
87	12.098	3437	3439	3441	rBV	470	285	0.02%	0.003%
88	12.159	3453	3458	3462	rBV	319	364	0.03%	0.004%
89	12.217	3473	3476	3477	rBV	207	130	0.01%	0.001%
90	12.255	3485	3488	3494	rBV4	440	306	0.02%	0.003%
91	12.304	3500	3503	3507	rBV2	174	139	0.01%	0.001%
92	12.542	3574	3577	3581	rBV3	313	300	0.02%	0.003%
93	12.603	3593	3596	3601	rVB2	422	332	0.03%	0.003%
94	12.625	3601	3603	3605	rBV	260	120	0.01%	0.001%
95	12.641	3605	3608	3611	rVV	295	138	0.01%	0.001%
96	12.728	3633	3635	3637	rBV	216	122	0.01%	0.001%
97	13.509	3870	3878	3890	rBV2	12457	21367	1.71%	0.219%
98	13.593	3901	3904	3906	rBV2	389	257	0.02%	0.003%
99	13.747	3949	3952	3953	rBV	254	150	0.01%	0.002%
100	14.249	4106	4108	4111	rBV3	411	277	0.02%	0.003%




Sum of corrected areas: 9770119

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022086.D
Acq On : 02 Sep 2021 19:24
Operator : SY/MD
Sample : M3608-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

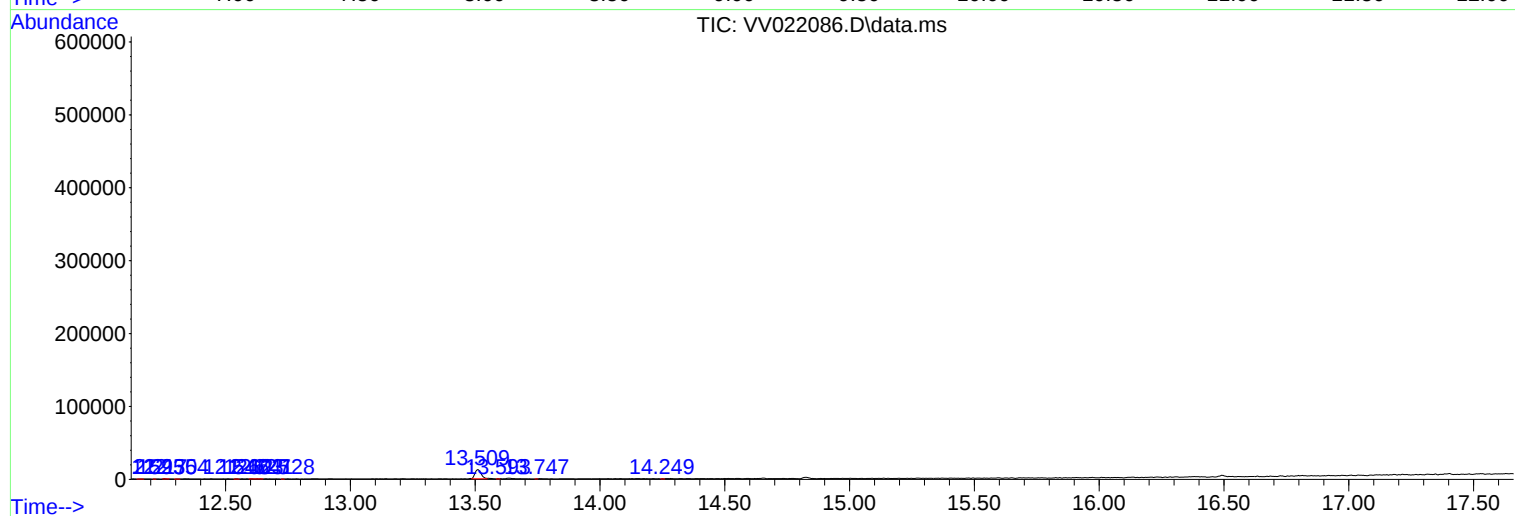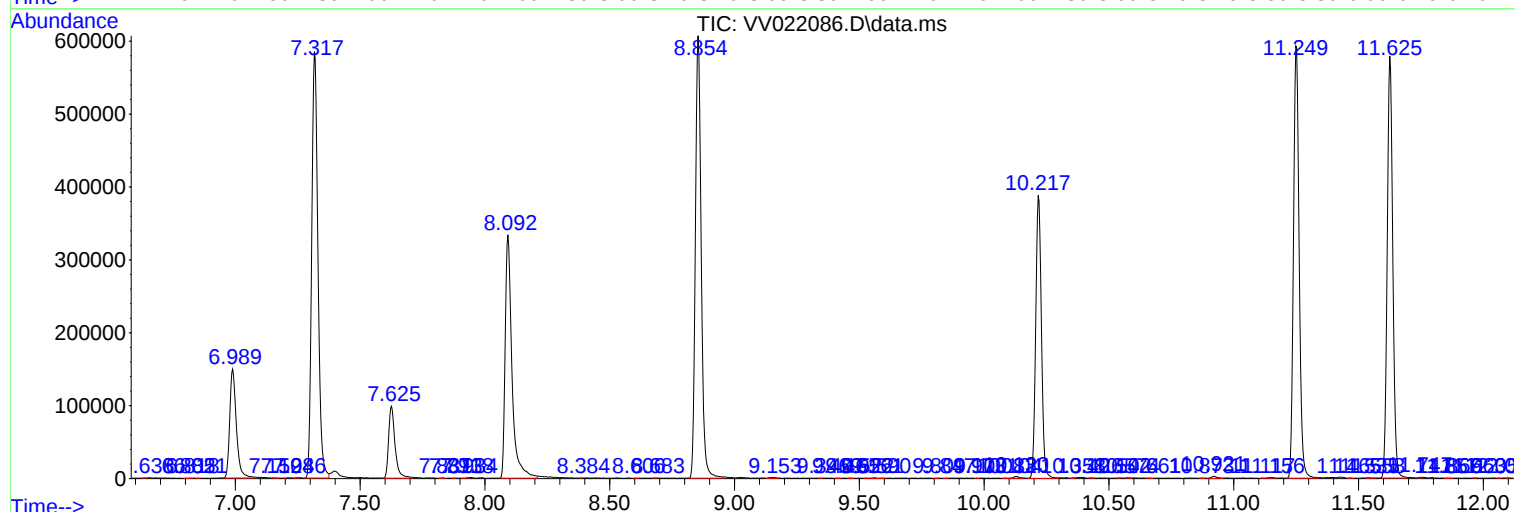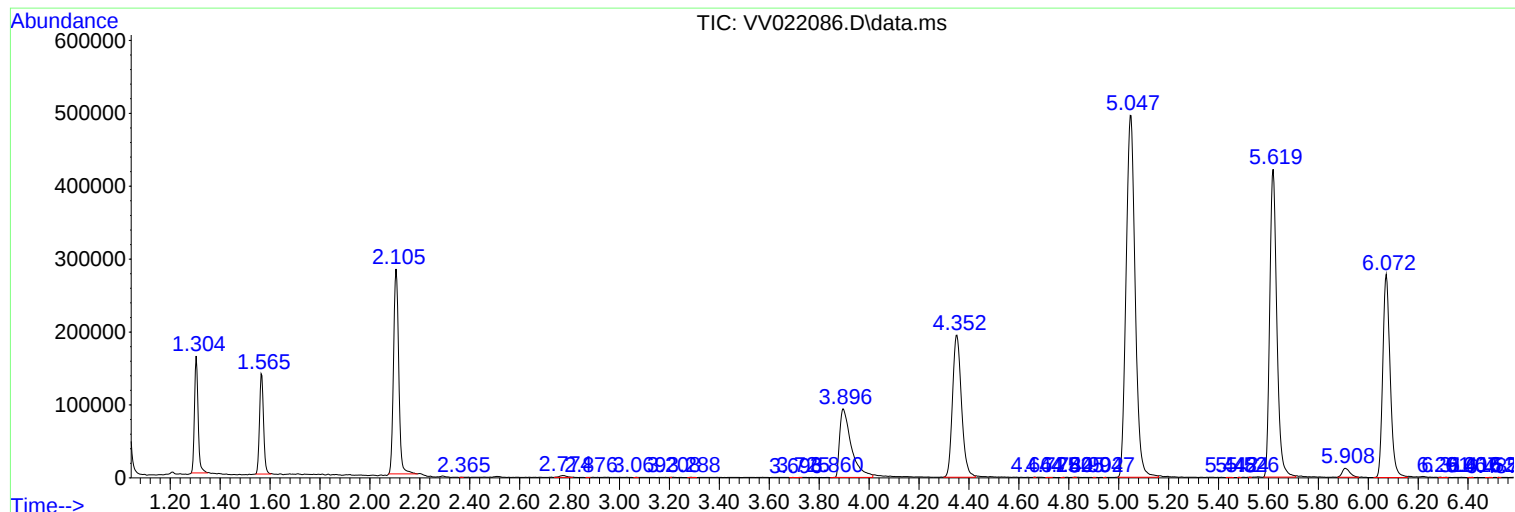

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022086.D
Acq On : 02 Sep 2021 19:24
Operator : SY/MD
Sample : M3608-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022086.D
Acq On : 02 Sep 2021 19:24
Operator : SY/MD
Sample : M3608-15
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
