

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022087.D
 Acq On : 02 Sep 2021 19:48
 Operator : SY/MD
 Sample : M3608-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022087.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rBV	158279	161482	12.96%	1.653%
2	1.564	157	163	177	rVB	135457	154655	12.42%	1.583%
3	2.105	322	331	348	rBV	283306	409015	32.84%	4.186%
4	2.368	411	413	416	rBV2	436	276	0.02%	0.003%
5	2.429	430	432	435	rBV	466	330	0.03%	0.003%
6	2.667	504	506	510	rBV3	390	218	0.02%	0.002%
7	2.773	526	539	553	rVB4	5334	12636	1.01%	0.129%
8	2.957	592	596	597	rBV	372	248	0.02%	0.003%
9	3.127	647	649	653	rVB2	418	276	0.02%	0.003%
10	3.146	653	655	659	rVB2	195	106	0.01%	0.001%
11	3.195	660	670	683	rBV5	1785	3456	0.28%	0.035%
12	3.291	697	700	701	rBV	249	138	0.01%	0.001%
13	3.426	740	742	745	rVB2	279	119	0.01%	0.001%
14	3.445	745	748	753	rBV	215	200	0.02%	0.002%
15	3.587	790	792	794	rVB2	317	118	0.01%	0.001%
16	3.642	807	809	811	rBV	164	111	0.01%	0.001%
17	3.757	843	845	847	rBV	286	115	0.01%	0.001%
18	3.896	877	888	927	rBV	94630	299181	24.02%	3.062%
19	4.352	1015	1030	1056	rBV	196522	480904	38.61%	4.921%
20	4.751	1150	1154	1156	rBV	250	192	0.02%	0.002%
21	4.780	1161	1163	1166	rBV2	253	127	0.01%	0.001%
22	4.799	1166	1169	1172	rVV3	231	128	0.01%	0.001%
23	4.828	1176	1178	1181	rVB	393	218	0.02%	0.002%
24	4.870	1189	1191	1193	rVB2	294	141	0.01%	0.001%
25	4.895	1195	1199	1203	rBV2	210	186	0.01%	0.002%
26	4.957	1217	1218	1222	rVB2	267	109	0.01%	0.001%
27	4.982	1224	1226	1230	rBV2	247	186	0.01%	0.002%
28	5.047	1230	1246	1274	rBV2	495031	1245536	100.00%	12.746%
29	5.375	1346	1348	1350	rBV	322	172	0.01%	0.002%
30	5.432	1364	1366	1369	rBV3	432	246	0.02%	0.003%
31	5.468	1375	1377	1383	rBV3	236	223	0.02%	0.002%
32	5.497	1383	1386	1391	rBV2	218	157	0.01%	0.002%
33	5.542	1397	1400	1404	rBV3	594	466	0.04%	0.005%
34	5.619	1412	1424	1457	rBV	418654	841987	67.60%	8.617%
35	5.908	1504	1514	1532	rBV7	10258	22940	1.84%	0.235%
36	6.002	1538	1543	1546	rBV3	318	344	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022087.D
 Acq On : 02 Sep 2021 19:48
 Operator : SY/MD
 Sample : M3608-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.072	1546	1565	1594	rBV	271604	559903	44.95%	5.730%
38	6.281	1627	1630	1631	rBV	346	207	0.02%	0.002%
39	6.387	1660	1663	1667	rBV3	229	205	0.02%	0.002%
40	6.436	1676	1678	1681	rVB2	272	109	0.01%	0.001%
41	6.587	1722	1725	1727	rBV3	232	151	0.01%	0.002%
42	6.638	1736	1741	1744	rBV4	638	678	0.05%	0.007%
43	6.793	1783	1789	1791	rBV2	355	289	0.02%	0.003%
44	6.809	1792	1794	1800	rVB2	436	354	0.03%	0.004%
45	6.838	1800	1803	1808	rBV	187	150	0.01%	0.002%
46	6.989	1838	1850	1873	rBV	146674	271400	21.79%	2.777%
47	7.175	1905	1908	1909	rBV2	324	180	0.01%	0.002%
48	7.214	1916	1920	1922	rBV2	391	321	0.03%	0.003%
49	7.317	1940	1952	1972	rBV	575848	1009920	81.08%	10.335%
50	7.580	2032	2034	2036	rVB2	362	119	0.01%	0.001%
51	7.625	2037	2048	2072	rBV	97252	174693	14.03%	1.788%
52	7.889	2124	2130	2133	rBV3	387	384	0.03%	0.004%
53	7.947	2140	2148	2154	rBV3	1695	2576	0.21%	0.026%
54	7.982	2157	2159	2163	rVB2	486	244	0.02%	0.002%
55	8.046	2177	2179	2182	rBV	199	104	0.01%	0.001%
56	8.091	2183	2193	2230	rBV	333625	623097	50.03%	6.377%
57	8.593	2344	2349	2352	rBV3	398	286	0.02%	0.003%
58	8.632	2356	2361	2362	rBV2	240	179	0.01%	0.002%
59	8.661	2366	2370	2371	rBV2	276	151	0.01%	0.002%
60	8.693	2378	2380	2382	rBV	256	141	0.01%	0.001%
61	8.706	2382	2384	2389	rVB2	375	296	0.02%	0.003%
62	8.854	2416	2430	2455	rBV	611738	999242	80.23%	10.226%
63	9.095	2501	2505	2508	rBV3	284	217	0.02%	0.002%
64	9.111	2508	2510	2513	rBV2	529	254	0.02%	0.003%
65	9.233	2545	2548	2549	rBV	203	104	0.01%	0.001%
66	9.313	2570	2573	2575	rBV	256	188	0.02%	0.002%
67	9.342	2579	2582	2585	rVB2	325	178	0.01%	0.002%
68	9.365	2585	2589	2590	rBV	167	117	0.01%	0.001%
69	9.526	2636	2639	2640	rBV	282	133	0.01%	0.001%
70	9.680	2685	2687	2692	rVB2	301	148	0.01%	0.002%
71	9.709	2692	2696	2698	rBV2	214	145	0.01%	0.001%
72	9.747	2702	2708	2710	rBV2	199	222	0.02%	0.002%
73	9.812	2726	2728	2733	rVV2	267	223	0.02%	0.002%
74	9.870	2744	2746	2749	rBV2	255	128	0.01%	0.001%
75	9.886	2749	2751	2757	rVB	209	162	0.01%	0.002%
76	9.937	2764	2767	2769	rVB	290	132	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022087.D
 Acq On : 02 Sep 2021 19:48
 Operator : SY/MD
 Sample : M3608-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DBKL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	9.960	2769	2774	2777	rBV2	207	216	0.02%	0.002%
78	10.095	2813	2816	2819	rBV3	259	206	0.02%	0.002%
79	10.217	2841	2854	2876	rBV	385956	612019	49.14%	6.263%
80	10.362	2897	2899	2901	rBV	380	195	0.02%	0.002%
81	10.387	2902	2907	2915	rVB6	2163	2664	0.21%	0.027%
82	10.432	2917	2921	2925	rBV2	302	203	0.02%	0.002%
83	10.458	2925	2929	2933	rVB	377	370	0.03%	0.004%
84	10.580	2965	2967	2970	rBV2	491	361	0.03%	0.004%
85	10.831	3040	3045	3046	rBV	381	294	0.02%	0.003%
86	10.924	3066	3074	3083	rBB6	2223	3623	0.29%	0.037%
87	11.149	3137	3144	3150	rBV6	1098	1215	0.10%	0.012%
88	11.252	3164	3176	3199	rBV	614465	946465	75.99%	9.686%
89	11.538	3257	3265	3275	rVB7	883	1406	0.11%	0.014%
90	11.625	3280	3292	3310	rBV	572979	896030	71.94%	9.170%
91	11.866	3365	3367	3375	rBV4	613	479	0.04%	0.005%
92	12.091	3433	3437	3438	rBV	398	289	0.02%	0.003%
93	12.294	3497	3500	3503	rBV2	222	168	0.01%	0.002%
94	12.612	3596	3599	3602	rVB3	562	318	0.03%	0.003%
95	13.101	3749	3751	3754	rVB2	283	153	0.01%	0.002%
96	13.467	3860	3865	3868	rBV3	403	401	0.03%	0.004%
97	13.513	3868	3879	3891	rVV	11577	19109	1.53%	0.196%
98	13.622	3910	3913	3914	rBV	610	302	0.02%	0.003%
99	13.763	3953	3957	3959	rBV	420	328	0.03%	0.003%
100	13.995	4027	4029	4032	rBV2	470	205	0.02%	0.002%




Sum of corrected areas: 9771691

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022087.D
Acq On : 02 Sep 2021 19:48
Operator : SY/MD
Sample : M3608-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

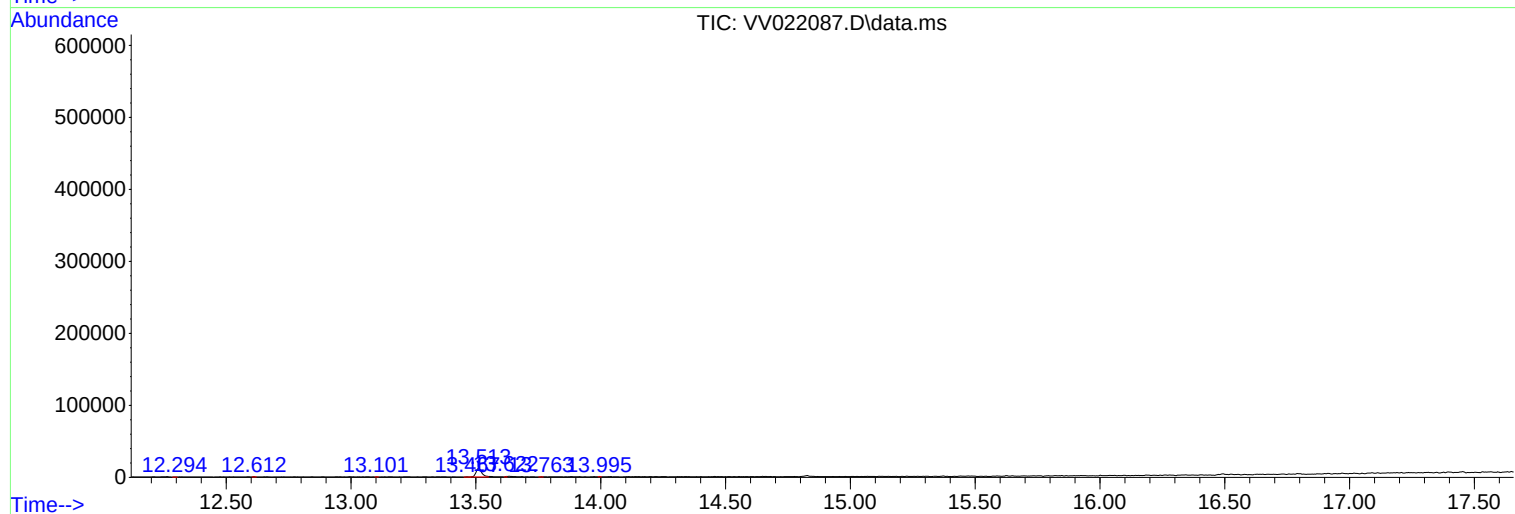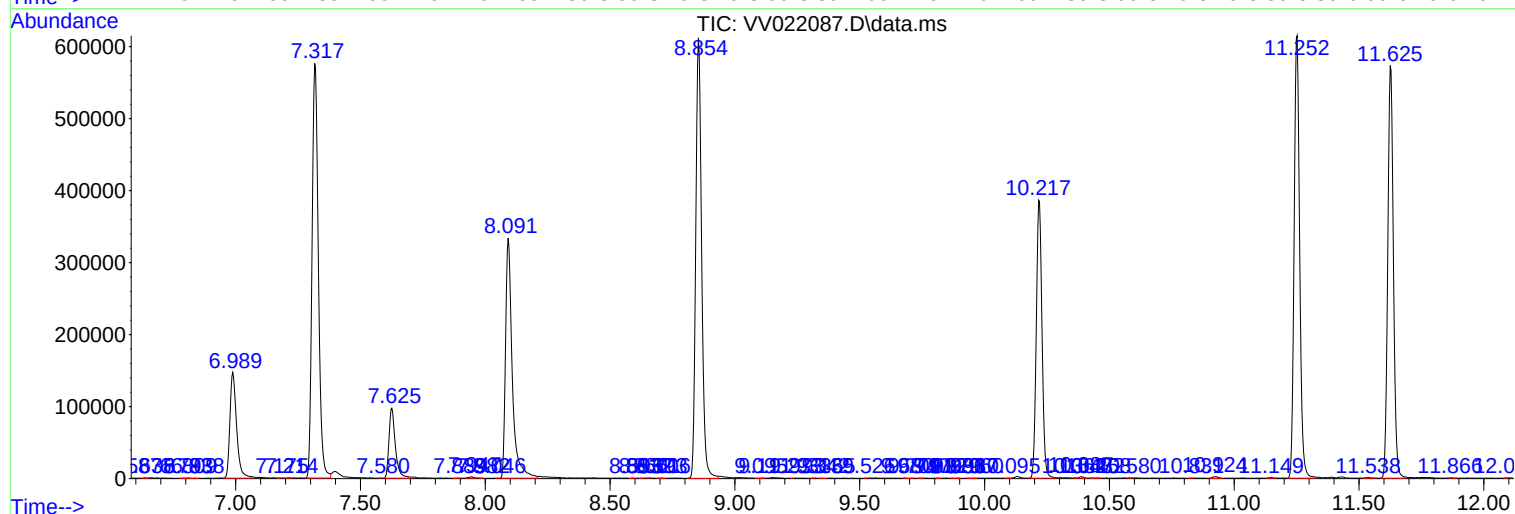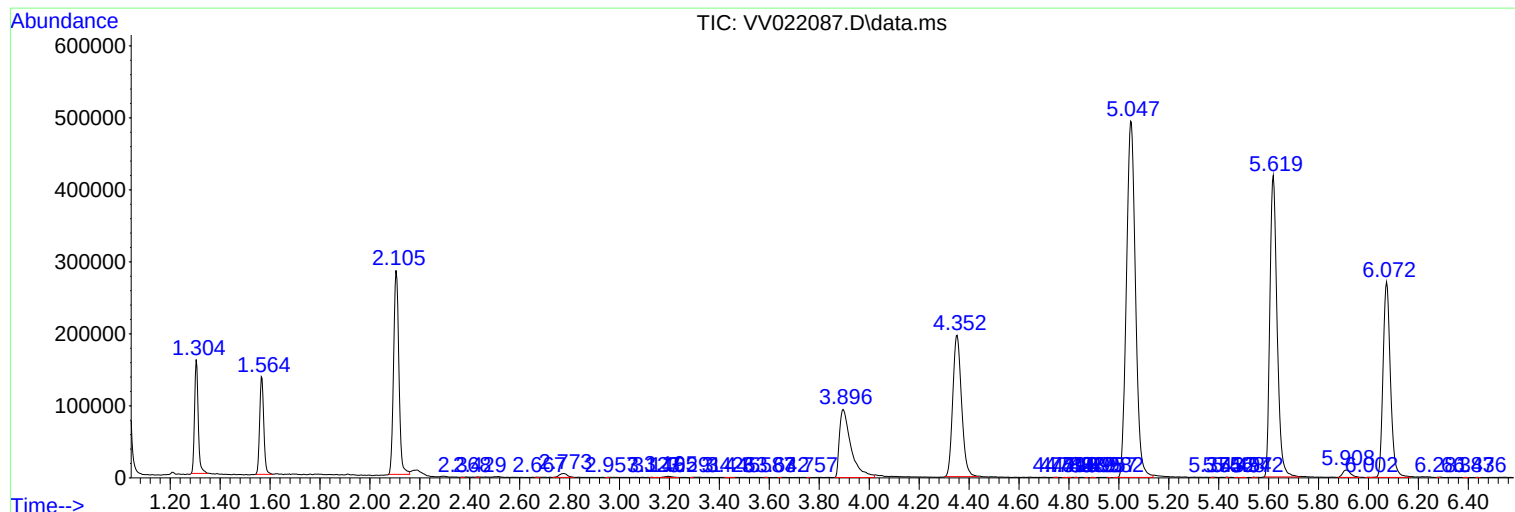

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022087.D
Acq On : 02 Sep 2021 19:48
Operator : SY/MD
Sample : M3608-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022087.D
Acq On : 02 Sep 2021 19:48
Operator : SY/MD
Sample : M3608-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DBKL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
