

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022088.D
 Acq On : 02 Sep 2021 21:01
 Operator : SY/MD
 Sample : M3647-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3W25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022088.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	100	rBV	152789	162097	7.40%	1.380%
2	1.565	156	163	178	rVB	134144	149663	6.83%	1.274%
3	2.105	321	331	357	rVB	271576	402493	18.38%	3.426%
4	2.288	382	388	397	rBV2	1567	2321	0.11%	0.020%
5	2.732	522	526	529	rBV3	391	349	0.02%	0.003%
6	2.770	530	538	553	rVB3	4470	9238	0.42%	0.079%
7	2.860	563	566	568	rBV	274	168	0.01%	0.001%
8	3.005	610	611	615	rBV	288	171	0.01%	0.001%
9	3.076	630	633	636	rBV2	309	158	0.01%	0.001%
10	3.195	668	670	674	rVB2	253	139	0.01%	0.001%
11	3.404	731	735	740	rBV2	275	306	0.01%	0.003%
12	3.471	748	756	758	rBV2	292	321	0.01%	0.003%
13	3.503	765	766	768	rBV	280	138	0.01%	0.001%
14	3.613	796	800	805	rVB2	358	252	0.01%	0.002%
15	3.684	819	822	825	rVB2	343	228	0.01%	0.002%
16	3.819	862	864	867	rVB	307	149	0.01%	0.001%
17	3.899	877	889	932	rBV3	98887	350702	16.01%	2.985%
18	4.349	1015	1029	1064	rVB	189687	475650	21.72%	4.048%
19	4.616	1110	1112	1119	rVB2	800	579	0.03%	0.005%
20	4.651	1119	1123	1124	rBV	290	210	0.01%	0.002%
21	4.941	1207	1213	1216	rBV3	386	407	0.02%	0.003%
22	5.047	1229	1246	1278	rBV2	480652	1217289	55.59%	10.361%
23	5.455	1370	1373	1376	rBV3	435	296	0.01%	0.003%
24	5.494	1378	1385	1388	rBV2	390	486	0.02%	0.004%
25	5.523	1392	1394	1397	rBV	262	186	0.01%	0.002%
26	5.555	1402	1404	1408	rVB	363	191	0.01%	0.002%
27	5.619	1411	1424	1451	rBV	412562	821685	37.52%	6.994%
28	5.912	1504	1515	1535	rVB7	16342	37107	1.69%	0.316%
29	6.072	1551	1565	1600	rBV	267842	549247	25.08%	4.675%
30	6.343	1647	1649	1652	rVB	560	242	0.01%	0.002%
31	6.378	1658	1660	1663	rBV	352	192	0.01%	0.002%
32	6.436	1675	1678	1681	rBV2	281	189	0.01%	0.002%
33	6.616	1730	1734	1737	rBV3	193	161	0.01%	0.001%
34	6.658	1737	1747	1752	rBV4	672	1230	0.06%	0.010%
35	6.735	1769	1771	1774	rBV2	408	252	0.01%	0.002%
36	6.754	1775	1777	1781	rVB2	319	181	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022088.D
 Acq On : 02 Sep 2021 21:01
 Operator : SY/MD
 Sample : M3647-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3W25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.777	1781	1784	1788	rBV	377	309	0.01%	0.003%
38	6.876	1811	1815	1821	rBB3	237	190	0.01%	0.002%
39	6.908	1821	1825	1828	rBV	633	430	0.02%	0.004%
40	6.989	1838	1850	1871	rBV	143594	260386	11.89%	2.216%
41	7.317	1939	1952	1970	rBV	558886	984146	44.94%	8.376%
42	7.625	2038	2048	2073	rBV	95268	169072	7.72%	1.439%
43	7.822	2106	2109	2113	rBV3	470	411	0.02%	0.003%
44	7.928	2140	2142	2144	rBV	231	139	0.01%	0.001%
45	7.976	2144	2157	2182	rBV	1310440	2189872	100.00%	18.639%
46	8.092	2184	2193	2228	rVB	327375	606763	27.71%	5.164%
47	8.394	2284	2287	2288	rBV2	445	249	0.01%	0.002%
48	8.506	2319	2322	2327	rVB3	428	337	0.02%	0.003%
49	8.539	2327	2332	2334	rBV	344	309	0.01%	0.003%
50	8.551	2334	2336	2338	rBV2	355	170	0.01%	0.001%
51	8.590	2345	2348	2351	rBV3	247	195	0.01%	0.002%
52	8.687	2375	2378	2380	rBV2	299	143	0.01%	0.001%
53	8.706	2380	2384	2386	rBV3	224	138	0.01%	0.001%
54	8.796	2410	2412	2415	rVB	428	244	0.01%	0.002%
55	8.854	2417	2430	2450	rBV	591982	965851	44.11%	8.221%
56	9.114	2506	2511	2514	rBV3	417	396	0.02%	0.003%
57	9.156	2516	2524	2530	rVB2	1384	1829	0.08%	0.016%
58	9.191	2530	2535	2537	rBV2	455	345	0.02%	0.003%
59	9.204	2537	2539	2543	rVV	287	170	0.01%	0.001%
60	9.265	2556	2558	2563	rVB2	319	167	0.01%	0.001%
61	9.555	2641	2648	2651	rBV2	523	644	0.03%	0.005%
62	9.809	2725	2727	2730	rBV	236	135	0.01%	0.001%
63	9.934	2764	2766	2769	rBV	257	190	0.01%	0.002%
64	9.969	2773	2777	2779	rBV2	240	197	0.01%	0.002%
65	9.998	2784	2786	2792	rVB2	346	220	0.01%	0.002%
66	10.127	2820	2826	2827	rBV2	1821	1526	0.07%	0.013%
67	10.217	2843	2854	2874	rBV	372933	593112	27.08%	5.048%
68	10.426	2914	2919	2923	rVB	215	212	0.01%	0.002%
69	10.465	2924	2931	2934	rBV2	430	372	0.02%	0.003%
70	10.484	2935	2937	2944	rVB3	303	257	0.01%	0.002%
71	10.551	2952	2958	2959	rBV2	823	755	0.03%	0.006%
72	10.606	2973	2975	2978	rVB3	517	285	0.01%	0.002%
73	10.770	3019	3026	3028	rBV2	169	176	0.01%	0.001%
74	10.838	3044	3047	3051	rVB	448	295	0.01%	0.003%
75	10.924	3066	3074	3082	rVB4	2334	3549	0.16%	0.030%
76	11.024	3100	3105	3109	rBV	421	438	0.02%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022088.D
 Acq On : 02 Sep 2021 21:01
 Operator : SY/MD
 Sample : M3647-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3W25

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	11.146	3140	3143	3144	rBV2	508	316	0.01%	0.003%
78	11.191	3150	3157	3161	rBV3	877	1113	0.05%	0.009%
79	11.252	3164	3176	3197	rBV	573575	900620	41.13%	7.665%
80	11.529	3257	3262	3263	rBV3	359	252	0.01%	0.002%
81	11.625	3280	3292	3315	rBV	544605	854238	39.01%	7.271%
82	11.818	3350	3352	3354	rBV	259	153	0.01%	0.001%
83	11.831	3354	3356	3360	rVV2	491	314	0.01%	0.003%
84	11.860	3363	3365	3371	rVB	306	215	0.01%	0.002%
85	11.911	3378	3381	3383	rVB	284	154	0.01%	0.001%
86	12.005	3408	3410	3414	rVB2	313	180	0.01%	0.002%
87	12.329	3508	3511	3513	rBV	250	168	0.01%	0.001%
88	12.526	3568	3572	3573	rBV	240	165	0.01%	0.001%
89	12.561	3580	3583	3585	rBV	334	190	0.01%	0.002%
90	12.612	3597	3599	3603	rBV2	335	243	0.01%	0.002%
91	12.648	3605	3610	3612	rBV4	870	790	0.04%	0.007%
92	13.111	3751	3754	3759	rVB2	200	181	0.01%	0.002%
93	13.227	3785	3790	3794	rBV2	410	331	0.02%	0.003%
94	13.275	3798	3805	3816	rVB7	1370	2088	0.10%	0.018%
95	13.509	3868	3878	3889	rBV2	8859	15108	0.69%	0.129%
96	13.670	3923	3928	3929	rBV	327	254	0.01%	0.002%
97	13.747	3947	3952	3961	rBV5	1435	1806	0.08%	0.015%
98	13.915	4000	4004	4006	rBV	298	244	0.01%	0.002%
99	14.072	4047	4053	4055	rBV2	404	435	0.02%	0.004%
100	14.265	4110	4113	4118	rVB2	370	282	0.01%	0.002%




Sum of corrected areas: 11749137

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022088.D
Acq On : 02 Sep 2021 21:01
Operator : SY/MD
Sample : M3647-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F3W25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

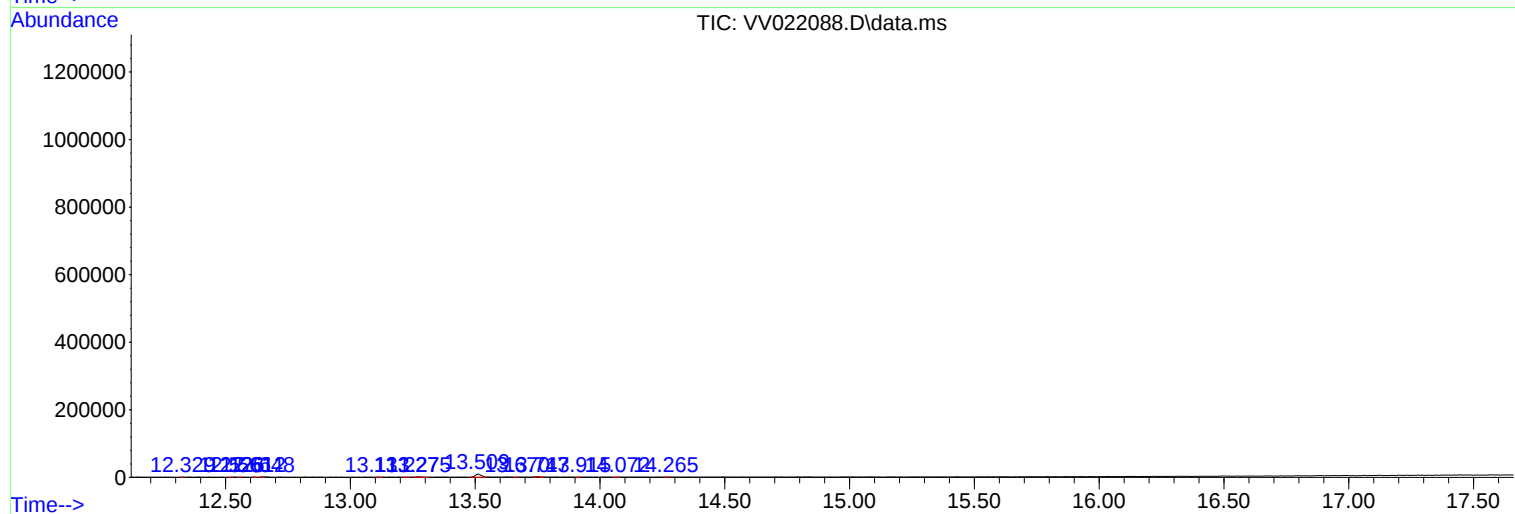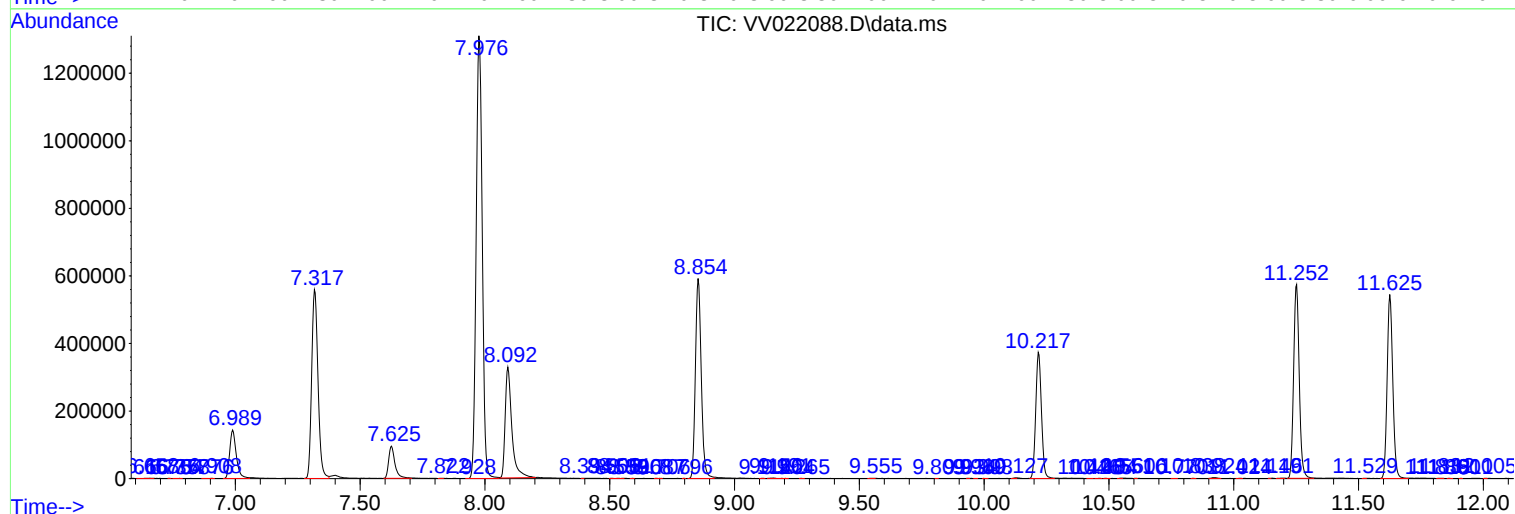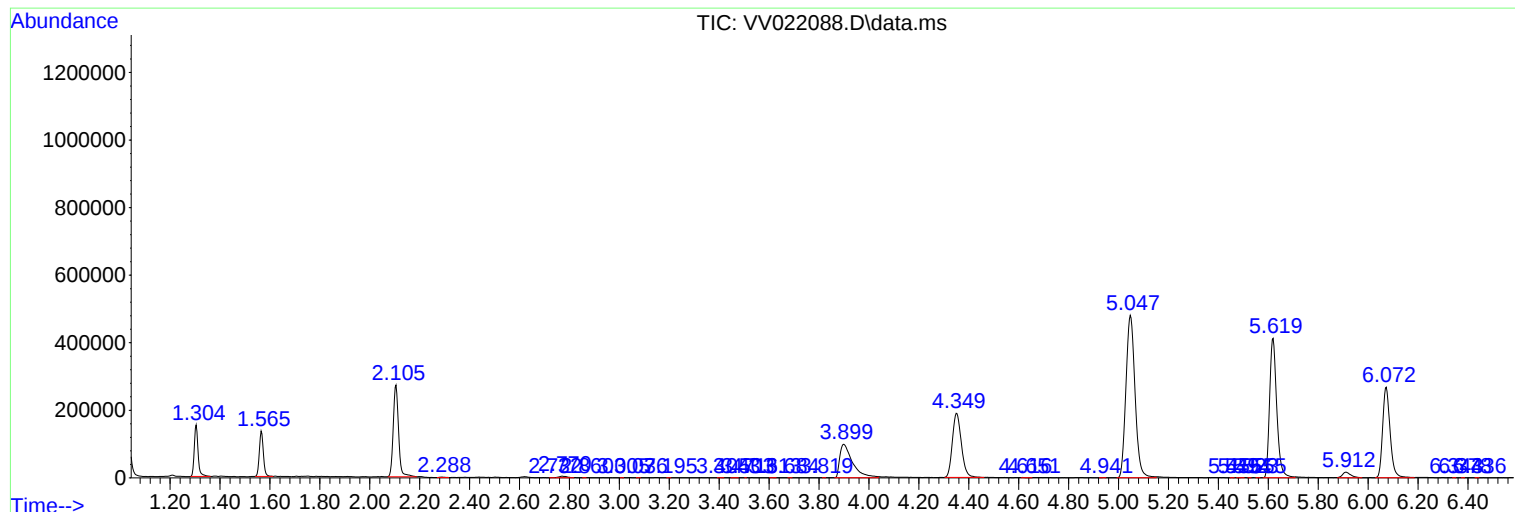

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022088.D
Acq On : 02 Sep 2021 21:01
Operator : SY/MD
Sample : M3647-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F3W25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022088.D
Acq On : 02 Sep 2021 21:01
Operator : SY/MD
Sample : M3647-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F3W25

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
