

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022089.D
 Acq On : 02 Sep 2021 21:25
 Operator : SY/MD
 Sample : M3647-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3W28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

Signal : TIC: VV022089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	156242	159737	13.22%	1.642%
2	1.564	156	163	179	rVB	134145	150797	12.48%	1.550%
3	2.105	321	331	356	rVB	275087	400071	33.11%	4.113%
4	2.291	382	389	391	rBV4	1344	1431	0.12%	0.015%
5	2.670	504	507	508	rBV	265	131	0.01%	0.001%
6	2.966	597	599	604	rBV3	448	232	0.02%	0.002%
7	2.995	606	608	612	rVB	431	201	0.02%	0.002%
8	3.095	634	639	641	rBV	221	142	0.01%	0.001%
9	3.114	642	645	649	rVV2	246	206	0.02%	0.002%
10	3.291	694	700	701	rBV3	265	257	0.02%	0.003%
11	3.330	710	712	714	rBV2	338	153	0.01%	0.002%
12	3.481	756	759	763	rBV	198	141	0.01%	0.001%
13	3.577	787	789	795	rVB2	300	262	0.02%	0.003%
14	3.622	800	803	806	rBV2	260	185	0.02%	0.002%
15	3.703	825	828	831	rBV	221	135	0.01%	0.001%
16	3.896	877	888	928	rBV3	94570	330109	27.32%	3.393%
17	4.352	1012	1030	1055	rBV	191790	475995	39.39%	4.893%
18	4.600	1106	1107	1110	rBV	351	192	0.02%	0.002%
19	4.622	1110	1114	1115	rBV2	426	197	0.02%	0.002%
20	4.777	1159	1162	1164	rBV	204	141	0.01%	0.001%
21	4.818	1170	1175	1176	rBV	249	183	0.02%	0.002%
22	4.879	1188	1194	1197	rBV3	391	389	0.03%	0.004%
23	4.931	1206	1210	1216	rBV	294	241	0.02%	0.002%
24	5.047	1226	1246	1274	rBV2	477435	1208425	100.00%	12.422%
25	5.452	1369	1372	1375	rBV3	252	224	0.02%	0.002%
26	5.497	1382	1386	1390	rBV2	309	343	0.03%	0.004%
27	5.561	1402	1406	1410	rBV3	272	259	0.02%	0.003%
28	5.619	1411	1424	1455	rBV	399379	806923	66.77%	8.295%
29	5.979	1534	1536	1539	rVB2	782	334	0.03%	0.003%
30	6.072	1551	1565	1594	rBV	267343	541725	44.83%	5.569%
31	6.317	1639	1641	1644	rBV2	490	367	0.03%	0.004%
32	6.381	1656	1661	1664	rBV3	474	360	0.03%	0.004%
33	6.403	1664	1668	1672	rVB2	313	211	0.02%	0.002%
34	6.429	1672	1676	1678	rBV	171	149	0.01%	0.002%
35	6.516	1695	1703	1711	rBV5	847	1501	0.12%	0.015%
36	6.577	1719	1722	1724	rBV3	335	265	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022089.D
 Acq On : 02 Sep 2021 21:25
 Operator : SY/MD
 Sample : M3647-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3W28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

37	6.629	1736	1738	1741	rBV3	313	193	0.02%	0.002%
38	6.651	1741	1745	1747	rBV2	420	279	0.02%	0.003%
39	6.789	1784	1788	1790	rBV2	178	118	0.01%	0.001%
40	6.989	1839	1850	1878	rBV	139079	258336	21.38%	2.656%
41	7.194	1912	1914	1915	rBV2	337	114	0.01%	0.001%
42	7.249	1929	1931	1933	rVB	362	155	0.01%	0.002%
43	7.268	1933	1937	1938	rBV2	206	143	0.01%	0.001%
44	7.317	1939	1952	1971	rBV	554040	972586	80.48%	9.998%
45	7.625	2035	2048	2072	rBV	90909	166092	13.74%	1.707%
46	7.834	2111	2113	2115	rVB	292	132	0.01%	0.001%
47	7.854	2115	2119	2120	rBV	263	181	0.01%	0.002%
48	7.866	2120	2123	2127	rVB2	521	316	0.03%	0.003%
49	7.892	2127	2131	2133	rBV	359	253	0.02%	0.003%
50	7.979	2145	2158	2174	rBV	219254	378090	31.29%	3.887%
51	8.091	2183	2193	2229	rBV	316080	592488	49.03%	6.091%
52	8.535	2327	2331	2333	rBV2	202	146	0.01%	0.002%
53	8.580	2344	2345	2347	rBV2	241	120	0.01%	0.001%
54	8.638	2359	2363	2365	rBV3	381	258	0.02%	0.003%
55	8.680	2373	2376	2379	rBV2	219	167	0.01%	0.002%
56	8.780	2404	2407	2412	rBV3	254	235	0.02%	0.002%
57	8.805	2413	2415	2418	rBV2	233	140	0.01%	0.001%
58	8.854	2418	2430	2456	rBV	580434	943985	78.12%	9.704%
59	9.153	2516	2523	2531	rBV4	860	1404	0.12%	0.014%
60	9.220	2542	2544	2549	rVB2	234	167	0.01%	0.002%
61	9.461	2614	2619	2624	rBV2	304	333	0.03%	0.003%
62	9.519	2632	2637	2639	rBV3	216	192	0.02%	0.002%
63	9.554	2644	2648	2655	rBV2	660	651	0.05%	0.007%
64	9.599	2660	2662	2664	rBV	262	143	0.01%	0.001%
65	9.628	2668	2671	2676	rVB3	330	241	0.02%	0.002%
66	9.780	2715	2718	2724	rVB2	440	375	0.03%	0.004%
67	9.818	2727	2730	2733	rBV2	192	153	0.01%	0.002%
68	9.915	2757	2760	2762	rBV2	470	221	0.02%	0.002%
69	10.088	2810	2814	2817	rVB2	234	150	0.01%	0.002%
70	10.133	2817	2828	2835	rBV6	1999	3765	0.31%	0.039%
71	10.220	2842	2855	2877	rBV	368467	579139	47.93%	5.953%
72	10.538	2951	2954	2956	rBV	310	208	0.02%	0.002%
73	10.661	2986	2992	2994	rBV2	423	361	0.03%	0.004%
74	10.776	3024	3028	3029	rBV2	304	220	0.02%	0.002%
75	10.786	3029	3031	3034	rVB2	239	145	0.01%	0.001%
76	10.921	3065	3073	3084	rVB5	2049	3127	0.26%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022089.D
 Acq On : 02 Sep 2021 21:25
 Operator : SY/MD
 Sample : M3647-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F3W28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis

77	10.966	3084	3087	3092	rVB	356	274	0.02%	0.003%
78	10.992	3092	3095	3099	rBV2	311	254	0.02%	0.003%
79	11.033	3104	3108	3112	rBV3	391	352	0.03%	0.004%
80	11.191	3153	3157	3159	rBV	535	333	0.03%	0.003%
81	11.252	3164	3176	3197	rBV	565740	874234	72.34%	8.987%
82	11.625	3278	3292	3313	rBV	537442	849228	70.28%	8.730%
83	11.847	3360	3361	3365	rVB3	359	212	0.02%	0.002%
84	11.950	3391	3393	3397	rVB2	384	205	0.02%	0.002%
85	12.037	3416	3420	3421	rBV	248	146	0.01%	0.002%
86	12.091	3434	3437	3439	rBV	201	125	0.01%	0.001%
87	12.156	3454	3457	3460	rBV2	205	134	0.01%	0.001%
88	12.464	3550	3553	3557	rBV	252	210	0.02%	0.002%
89	12.538	3574	3576	3579	rBV2	250	123	0.01%	0.001%
90	12.677	3617	3619	3623	rBV	175	141	0.01%	0.001%
91	12.763	3643	3646	3647	rBV	218	114	0.01%	0.001%
92	12.969	3707	3710	3713	rBV2	217	114	0.01%	0.001%
93	13.223	3786	3789	3790	rBV	294	189	0.02%	0.002%
94	13.275	3800	3805	3810	rBV5	745	897	0.07%	0.009%
95	13.448	3854	3859	3861	rBV2	340	230	0.02%	0.002%
96	13.512	3869	3879	3889	rBV2	7377	11227	0.93%	0.115%
97	13.603	3905	3907	3909	rVB	441	201	0.02%	0.002%
98	13.619	3909	3912	3913	rBV2	366	178	0.01%	0.002%
99	13.734	3945	3948	3949	rBV2	397	223	0.02%	0.002%
100	13.815	3970	3973	3978	rVB3	455	395	0.03%	0.004%




Sum of corrected areas: 9727875

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022089.D
Acq On : 02 Sep 2021 21:25
Operator : SY/MD
Sample : M3647-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F3W28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

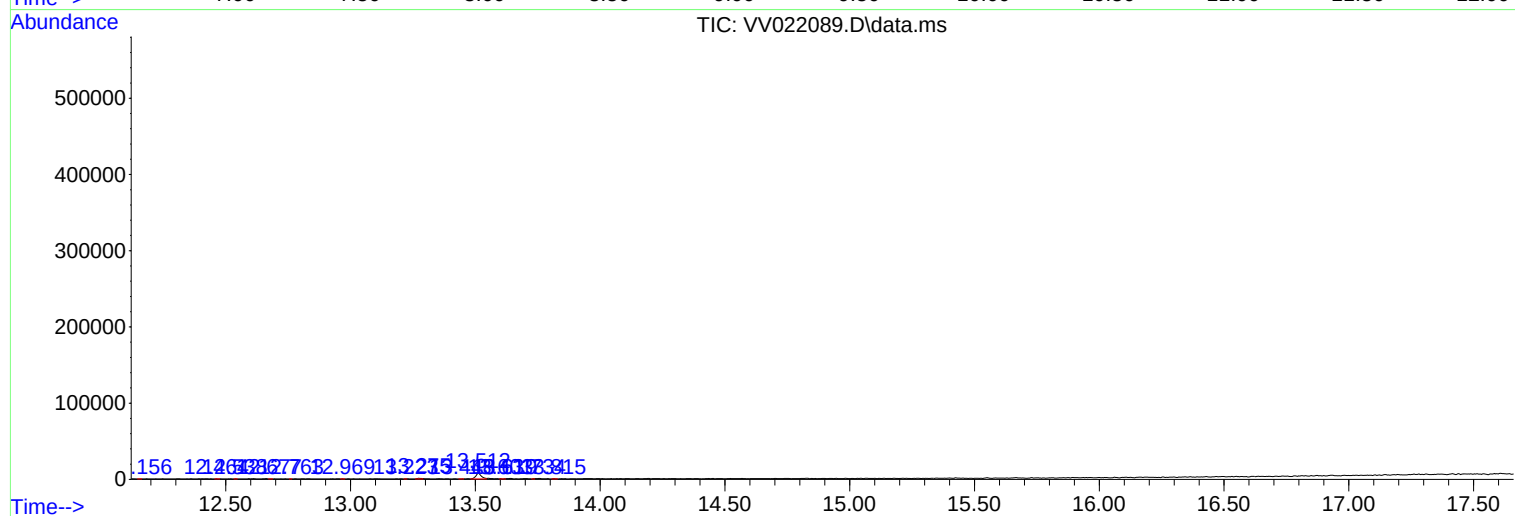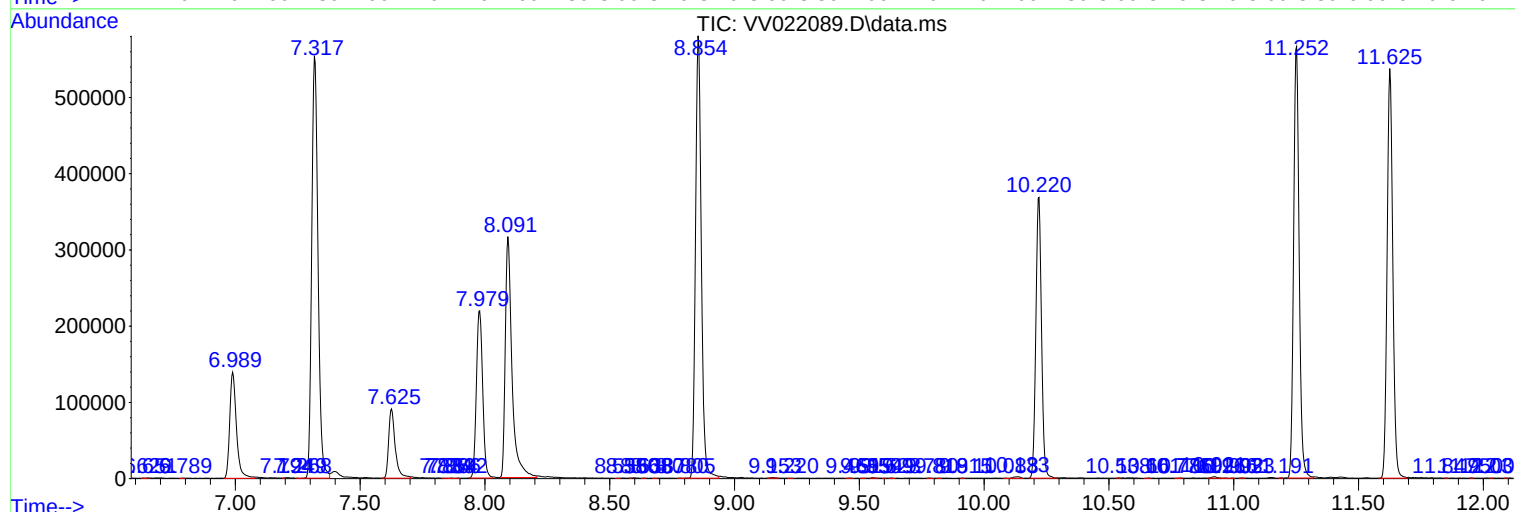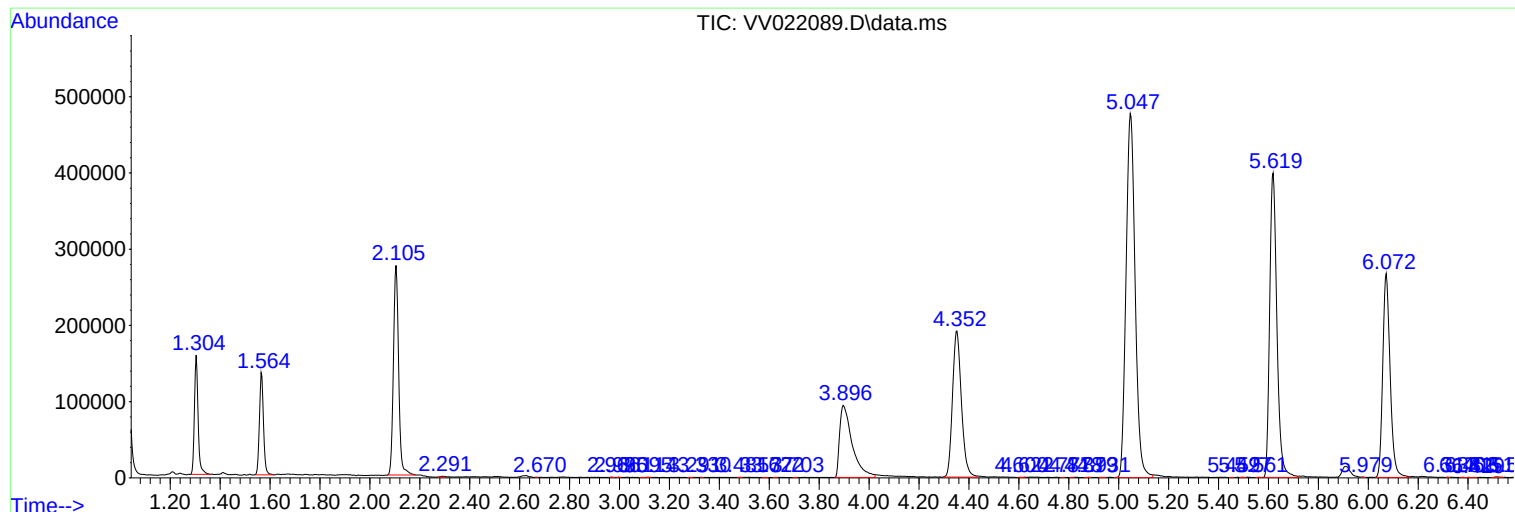

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022089.D
Acq On : 02 Sep 2021 21:25
Operator : SY/MD
Sample : M3647-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F3W28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
Data File : VV022089.D
Acq On : 02 Sep 2021 21:25
Operator : SY/MD
Sample : M3647-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F3W28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------