
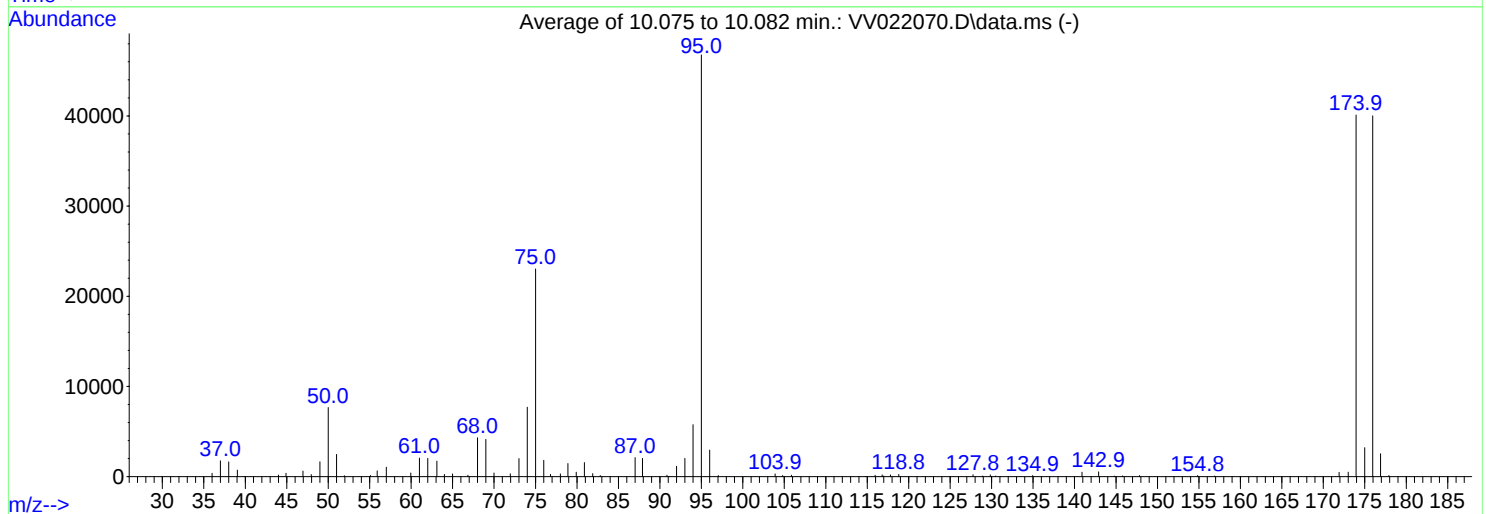


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV090221\
 Data File : VV022070.D
 Acq On : 02 Sep 2021 12:53
 Operator : SY/MD
 Sample : BFB227
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB227

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM082721WMA.M
 Title : VOC Analysis
 Last Update : Wed Sep 08 01:14:49 2021

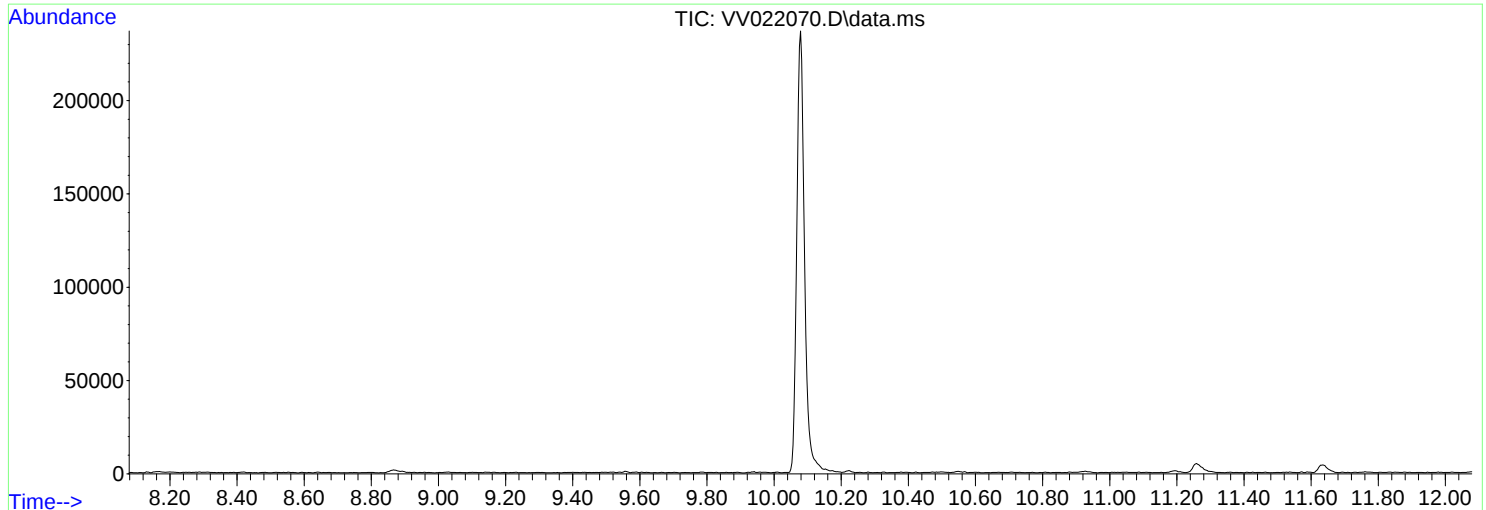

AutoFind: Scans 2810, 2811, 2812; Background Corrected with Scan 2799

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	7666	PASS
75	95	30	80	49.2	23032	PASS
95	95	100	100	100.0	46773	PASS
96	95	5	9	6.3	2944	PASS
173	174	0.00	2	1.3	506	PASS
174	95	50	120	85.7	40099	PASS
175	174	5	9	8.0	3214	PASS
176	174	95	105	99.8	40019	PASS
177	176	5	10	6.4	2546	PASS

m/z	Abundance
36.00	388.0
37.00	1634.0
38.00	1603.0
39.00	702.0
40.00	222.0
44.00	632.0
44.90	365.0
47.00	567.0
48.00	227.0
49.00	1654.0
50.00	7221.0
51.00	2347.0
52.00	106.0
55.10	103.0
55.90	597.0
57.00	1028.0
60.00	390.0
61.00	2070.0
62.00	1872.0
63.10	1590.0
64.10	256.0
65.00	288.0
66.90	150.0
68.00	4186.0
69.00	4112.0
70.00	360.0
72.00	297.0
73.00	1858.0
74.00	7318.0
75.00	22088.0
76.00	1705.0
76.80	205.0
78.00	321.0
78.90	1468.0
79.90	497.0
80.90	1590.0
81.90	295.0
82.80	115.0
87.00	2042.0
87.90	1836.0
90.80	130.0
91.20	130.0
92.00	1146.0
93.00	1929.0
94.00	5553.0
95.00	44848.0
96.00	2671.0
97.10	104.0
103.90	276.0
104.80	109.0
105.80	162.0
114.80	104.0
116.00	140.0
117.00	218.0
117.80	170.0
118.80	216.0
127.80	224.0
128.90	113.0
129.80	183.0
130.50	112.0
134.90	118.0
140.90	447.0
142.90	573.0
147.80	126.0
154.90	103.0
171.90	491.0
173.00	490.0
173.90	39760.0
175.00	3095.0
175.90	39208.0
176.90	2440.0
177.90	106.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

Scan 2799 (10.040 min): VV022070.D\data.ms
BFB227

m/z	Abundance
39.90	218.0
44.00	529.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

m/z	Abundance
36.00	338.0
37.00	1843.0
38.00	1622.0
39.00	716.0
40.00	235.0
44.00	756.0
44.90	372.0
46.90	673.0
47.90	220.0
49.00	1550.0
50.00	7873.0
51.00	2500.0
51.90	120.0
55.10	136.0
55.90	667.0
57.00	1042.0
59.90	414.0
61.00	1970.0
62.00	2087.0
63.10	1796.0
63.90	254.0
65.00	303.0
66.80	153.0
68.00	4305.0
69.00	4018.0
70.00	429.0
71.90	312.0
73.00	2070.0
74.00	7768.0
75.00	23256.0
76.00	1909.0
76.80	299.0
78.00	282.0
78.90	1414.0
79.90	451.0
80.90	1472.0
81.90	362.0
82.80	116.0
87.00	2049.0
87.90	2168.0
90.90	171.0
92.00	1136.0
93.00	2049.0
94.00	5780.0
95.00	47040.0
96.00	3127.0
97.10	133.0
103.90	313.0
104.80	110.0
105.90	174.0
115.90	174.0
116.80	346.0
117.80	209.0
118.80	275.0
127.70	186.0
129.90	208.0
135.00	117.0
140.90	518.0
142.90	459.0
144.80	113.0
145.80	125.0
147.90	124.0
154.80	147.0
156.90	110.0
171.90	434.0
173.00	516.0
174.00	39128.0
175.00	3237.0
176.00	39368.0
176.90	2597.0
177.90	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227

m/z	Abundance
36.00	400.0
37.00	1805.0
38.00	1660.0
39.10	753.0
40.00	235.0
44.00	708.0
44.90	402.0
46.90	645.0
48.00	236.0
49.00	1728.0
50.00	7903.0
51.00	2552.0
51.90	109.0
55.10	124.0
55.90	670.0
57.00	1054.0
59.90	425.0
61.00	2132.0
62.00	2122.0
63.10	1789.0
64.00	236.0
65.00	319.0
66.90	163.0
68.00	4438.0
69.00	4248.0
70.00	423.0
71.90	332.0
73.00	2080.0
74.00	8004.0
75.00	23752.0
76.00	1843.0
76.80	260.0
78.00	327.0
78.90	1490.0
79.90	534.0
80.90	1601.0
81.90	347.0
82.80	146.0
87.00	2227.0
87.90	2081.0
90.80	169.0
92.00	1168.0
93.00	2105.0
94.00	5965.0
95.00	48432.0
96.00	3035.0
97.00	155.0
103.90	308.0
104.80	132.0
105.90	168.0
115.90	164.0
116.80	270.0
117.80	225.0
118.80	272.0
127.70	224.0
128.90	120.0
129.90	198.0
130.50	108.0
135.00	129.0
140.90	527.0
142.90	543.0
144.80	115.0
145.80	129.0
147.80	132.0
154.90	130.0
156.90	108.0
171.90	516.0
173.00	512.0
174.00	41408.0
175.00	3309.0
176.00	41480.0
176.90	2600.0
177.90	126.0

Instrument :
MSVOA_V
ClientSampleId :
BFB227