

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090319\
 Data File : VV012552.D
 Acq On : 03 Sep 2019 17:15
 Operator : SY/MD
 Sample : K4607-09DL 5X
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFD65DL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.1
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
 Title : TRACE VOA SOM01.0

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.116	5	8	18	rVB4	11314	13088	2.17%	0.228%
2	1.315	63	70	82	rVB	113423	121120	20.10%	2.107%
3	1.582	146	153	166	rVB	104007	116752	19.37%	2.031%
4	2.129	314	323	338	rVB2	212854	316924	52.59%	5.514%
5	3.962	875	893	925	rBV2	80274	282822	46.93%	4.921%
6	4.399	1013	1029	1050	rBV2	102647	251844	41.79%	4.382%
7	5.093	1228	1245	1268	rBV2	226496	552572	91.70%	9.614%
8	5.662	1408	1422	1445	rBV	174930	358248	59.45%	6.233%
9	5.958	1500	1514	1530	rBV	214369	424609	70.46%	7.388%
10	6.116	1550	1563	1583	rBV2	136179	272441	45.21%	4.740%
11	7.029	1836	1847	1860	rBV	59454	110286	18.30%	1.919%
12	7.360	1936	1950	1968	rBV	230221	415134	68.89%	7.223%
13	7.666	2033	2045	2055	rBV2	35501	65010	10.79%	1.131%
14	8.016	2136	2154	2175	rBV	349179	602593	100.00%	10.485%
15	8.141	2182	2193	2229	rBV2	218762	534239	88.66%	9.295%
16	8.894	2413	2427	2444	rBV	280750	467042	77.51%	8.126%
17	10.260	2842	2852	2865	rBV	87338	139646	23.17%	2.430%
18	10.421	2894	2902	2910	rBV6	9399	15367	2.55%	0.267%
19	11.292	3160	3173	3193	rBV	202346	348168	57.78%	6.058%
20	11.669	3279	3290	3308	rBV	203517	339418	56.33%	5.906%


Sum of corrected areas: 5747323

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090319\
Data File : VV012552.D
Acq On : 03 Sep 2019 17:15
Operator : SY/MD
Sample : K4607-09DL 5X
Misc : 25mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD65DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

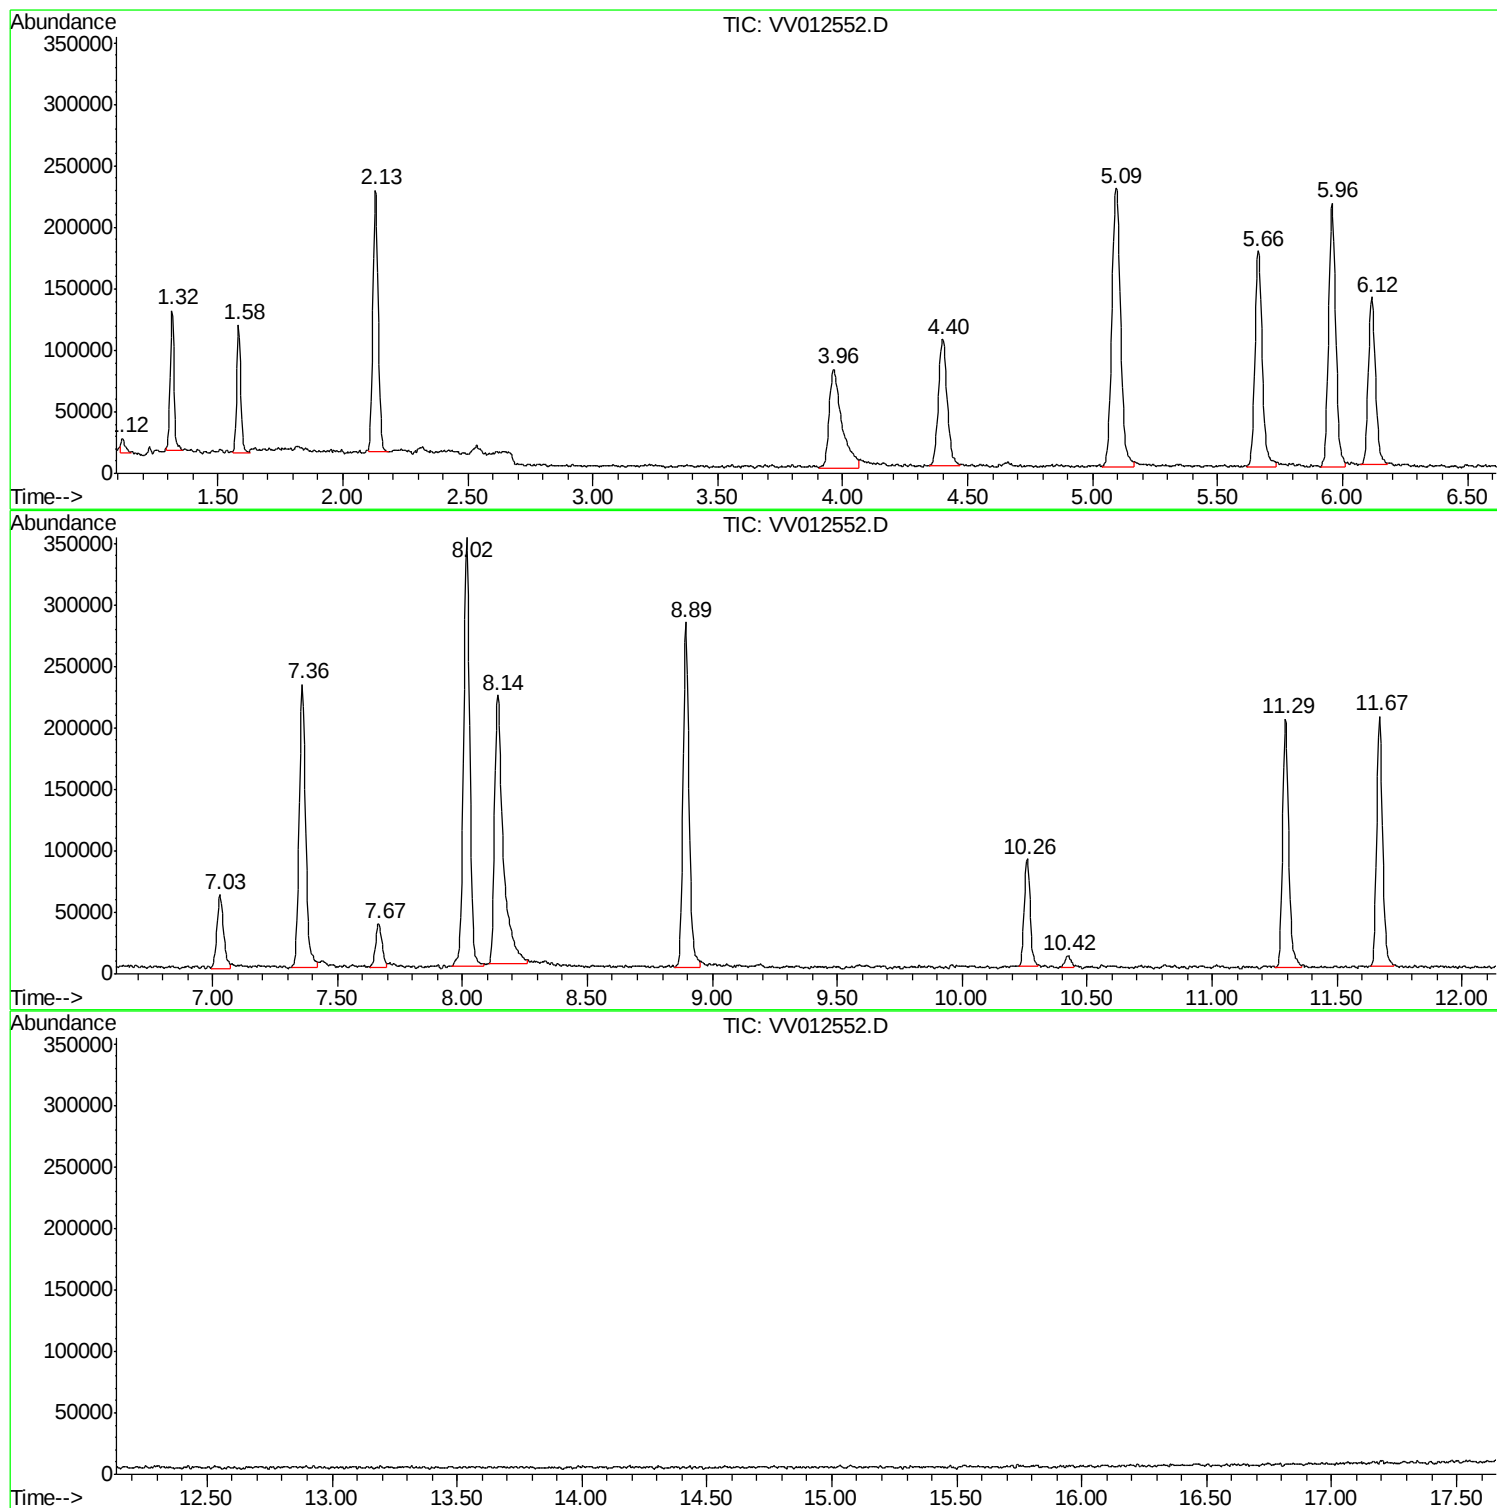

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090319\
Data File : VV012552.D
Acq On : 03 Sep 2019 17:15
Operator : SY/MD
Sample : K4607-09DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD65DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090319\
Data File : VV012552.D
Acq On : 03 Sep 2019 17:15
Operator : SY/MD
Sample : K4607-09DL 5X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD65DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
Quant Title : TRACE VOA SOM01.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc