


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV090319\
Data File : VV012544.D
Acq On : 03 Sep 2019 08:33
Operator : SY/MD
Sample : BFB59
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB59

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Sep 05 14:43:13 2019

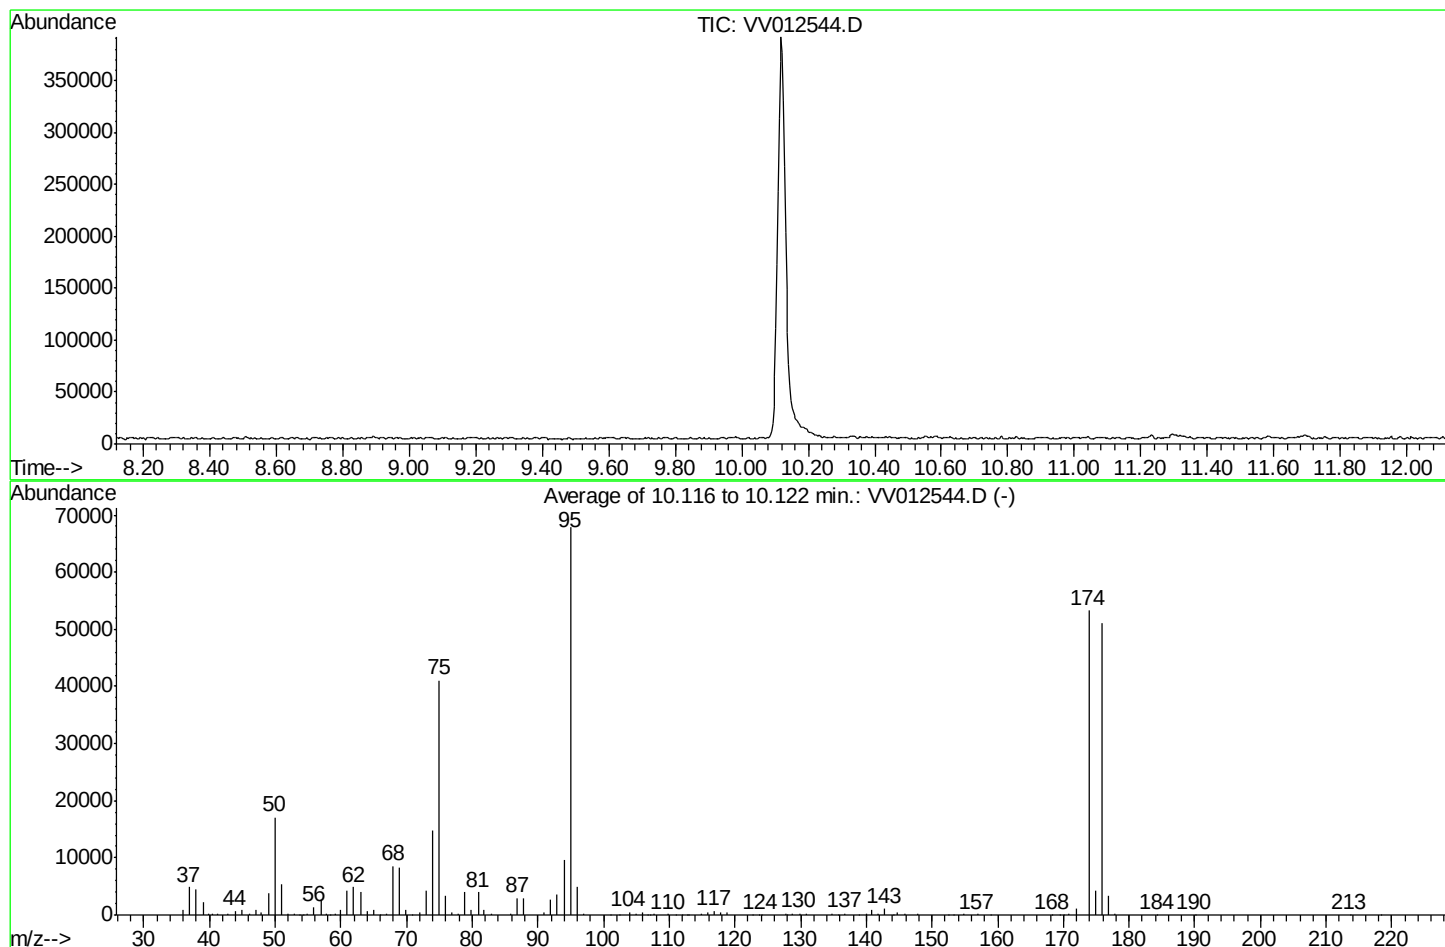

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2794

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.1	17036	PASS
75	95	30	80	60.6	41112	PASS
95	95	100	100	100.0	67845	PASS
96	95	5	9	7.3	4924	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.5	53264	PASS
175	174	5	9	8.1	4318	PASS
176	174	95	101	95.7	50989	PASS
177	176	5	9	6.8	3457	PASS

m/z	Abundance
35.20	174.0
35.80	176.0
36.40	147.0
36.80	145.0
37.90	239.0
38.70	228.0
40.00	511.0
41.80	232.0
42.40	146.0
43.90	488.0
45.00	141.0
47.40	113.0
47.80	129.0
48.50	166.0
50.20	113.0
51.60	115.0
52.10	108.0
52.70	138.0
53.70	121.0
56.30	121.0
59.60	115.0
63.20	128.0
64.30	162.0
65.70	107.0
68.50	125.0
74.50	113.0
75.50	112.0
76.70	109.0
77.90	110.0
80.00	173.0
81.20	103.0
83.10	129.0
86.60	111.0
87.70	106.0
93.80	116.0
120.90	103.0
189.30	110.0
211.70	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

m/z	Abundance
35.20	159.0
35.90	1046.0
37.00	4989.0
38.00	4683.0
39.00	2210.0
39.90	800.0
40.40	308.0
41.10	108.0
42.00	128.0
42.90	169.0
44.00	1166.0
45.00	913.0
46.20	187.0
47.00	840.0
47.90	649.0
49.00	3770.0
50.00	16872.0
51.00	5195.0
51.90	339.0
53.00	267.0
53.80	126.0
54.30	131.0
54.90	358.0
55.90	1472.0
57.00	2501.0
57.90	119.0
59.10	133.0
60.00	854.0
61.00	4202.0
61.90	4842.0
63.00	3801.0
64.00	702.0
65.00	871.0
66.90	283.0
68.00	8365.0
69.00	7812.0
69.90	782.0
72.00	518.0
73.00	4084.0
74.00	14489.0
75.00	39992.0
76.00	3437.0
77.00	524.0
77.80	391.0
78.90	3852.0
79.90	1092.0
80.90	3918.0
81.90	935.0
82.90	210.0
86.00	179.0
86.90	2918.0
87.90	2856.0
90.90	492.0
92.00	2583.0
93.00	3612.0
94.00	9251.0
95.00	66256.0
96.00	4838.0
96.90	156.0
101.00	103.0
103.90	475.0
105.10	153.0
105.80	450.0
106.80	125.0
107.70	111.0
109.90	108.0
111.00	164.0
112.10	114.0
112.70	152.0
114.90	172.0
115.80	505.0
116.90	737.0
117.80	327.0
118.80	435.0
127.80	311.0
128.80	249.0
129.80	303.0
130.90	181.0
134.80	196.0
136.80	237.0
138.80	152.0
140.10	161.0
140.80	908.0
141.90	192.0
142.90	1042.0
144.10	104.0
144.80	389.0
145.70	168.0
148.00	164.0
154.80	175.0
156.90	188.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

159.00	108.0
168.30	110.0
170.80	254.0
171.90	1065.0
173.90	51520.0
174.90	4150.0
175.90	49016.0
176.90	3302.0
177.80	182.0
218.30	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

m/z	Abundance
35.20	134.0
36.00	1072.0
37.00	5165.0
38.00	4969.0
39.00	2393.0
39.90	757.0
40.50	250.0
41.20	119.0
42.00	156.0
42.80	189.0
44.00	1220.0
45.00	1005.0
46.10	253.0
47.00	909.0
47.90	709.0
49.00	4060.0
50.00	17592.0
51.00	5557.0
51.90	329.0
52.90	272.0
53.80	145.0
54.90	325.0
55.90	1517.0
57.00	2677.0
57.90	135.0
59.10	165.0
60.00	909.0
61.00	4419.0
61.90	5041.0
63.00	4237.0
64.00	751.0
65.00	960.0
66.90	288.0
68.00	8853.0
69.00	8488.0
69.90	824.0
70.90	106.0
72.00	503.0
73.00	4439.0
74.00	15453.0
75.00	42624.0
76.00	3571.0
77.00	463.0
77.90	424.0
78.90	4161.0
79.90	1142.0
80.90	4090.0
81.90	970.0
82.90	221.0
86.00	145.0
86.90	3056.0
87.90	3032.0
90.90	551.0
92.00	2690.0
92.90	3814.0
94.00	10049.0
95.00	70152.0
96.00	5153.0
96.90	173.0
101.10	104.0
103.90	514.0
105.10	185.0
105.90	441.0
106.80	128.0
107.70	132.0
109.80	130.0
110.90	121.0
112.10	126.0
112.70	182.0
114.90	169.0
115.80	545.0
116.80	754.0
117.80	382.0
118.90	530.0
122.60	107.0
123.60	122.0
124.10	121.0
127.80	292.0
128.80	241.0
129.90	315.0
130.80	172.0
134.70	178.0
136.80	259.0
138.80	127.0
140.10	184.0
140.90	929.0
141.90	169.0
142.80	1070.0
144.80	455.0
145.80	196.0
147.90	165.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

154.70	182.0
156.90	239.0
159.00	118.0
169.50	119.0
170.00	107.0
170.70	314.0
171.90	1075.0
173.90	55216.0
174.90	4485.0
175.90	52680.0
176.90	3518.0
177.90	230.0
184.30	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

m/z	Abundance
35.10	148.0
36.00	999.0
37.00	4778.0
38.00	4750.0
39.00	2252.0
39.90	679.0
40.60	178.0
41.20	148.0
42.00	151.0
42.80	216.0
44.00	1163.0
45.00	1003.0
46.00	278.0
47.00	1006.0
48.00	715.0
49.00	3717.0
50.00	16984.0
51.00	5384.0
51.90	293.0
53.00	238.0
53.80	162.0
55.00	264.0
55.90	1316.0
57.00	2655.0
57.80	148.0
58.30	130.0
59.10	155.0
60.00	941.0
61.00	4184.0
61.90	4708.0
63.00	4280.0
64.00	739.0
65.00	884.0
66.00	113.0
66.90	246.0
68.00	8404.0
69.00	8381.0
70.00	796.0
70.90	152.0
72.00	503.0
73.00	4196.0
74.00	14633.0
75.00	40720.0
76.00	3386.0
76.90	414.0
77.90	423.0
78.90	4117.0
79.90	1125.0
80.90	3814.0
81.80	928.0
82.90	178.0
83.20	124.0
85.80	129.0
86.00	139.0
86.90	2889.0
87.90	2973.0
90.90	475.0
91.90	2594.0
92.90	3511.0
94.00	9878.0
95.00	67128.0
96.00	4783.0
97.00	175.0
102.50	125.0
103.90	482.0
105.00	175.0
105.90	404.0
107.00	114.0
107.80	117.0
109.90	136.0
112.00	114.0
112.90	178.0
114.90	181.0
115.80	475.0
116.80	703.0
117.80	356.0
118.90	512.0
122.60	108.0
124.00	148.0
128.00	261.0
128.80	248.0
129.80	279.0
130.80	172.0
134.80	191.0
135.80	124.0
136.80	243.0
140.10	154.0
140.90	910.0
141.80	153.0
142.80	1096.0
144.80	417.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59

145.90	185.0
147.80	208.0
152.50	105.0
153.20	123.0
154.70	177.0
156.90	250.0
159.00	123.0
169.50	105.0
170.00	129.0
170.70	320.0
171.90	968.0
173.90	53056.0
174.90	4319.0
175.90	51272.0
176.90	3552.0
177.90	232.0
184.30	123.0
190.10	108.0
213.60	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB59