


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV090320\
 Data File : VV018147.D
 Acq On : 03 Sep 2020 09:17
 Operator : SY/MD
 Sample : BFB601
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB601

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMVLM080619W.M
 Title : VOC Analysis
 Last Update : Fri Sep 04 02:12:05 2020

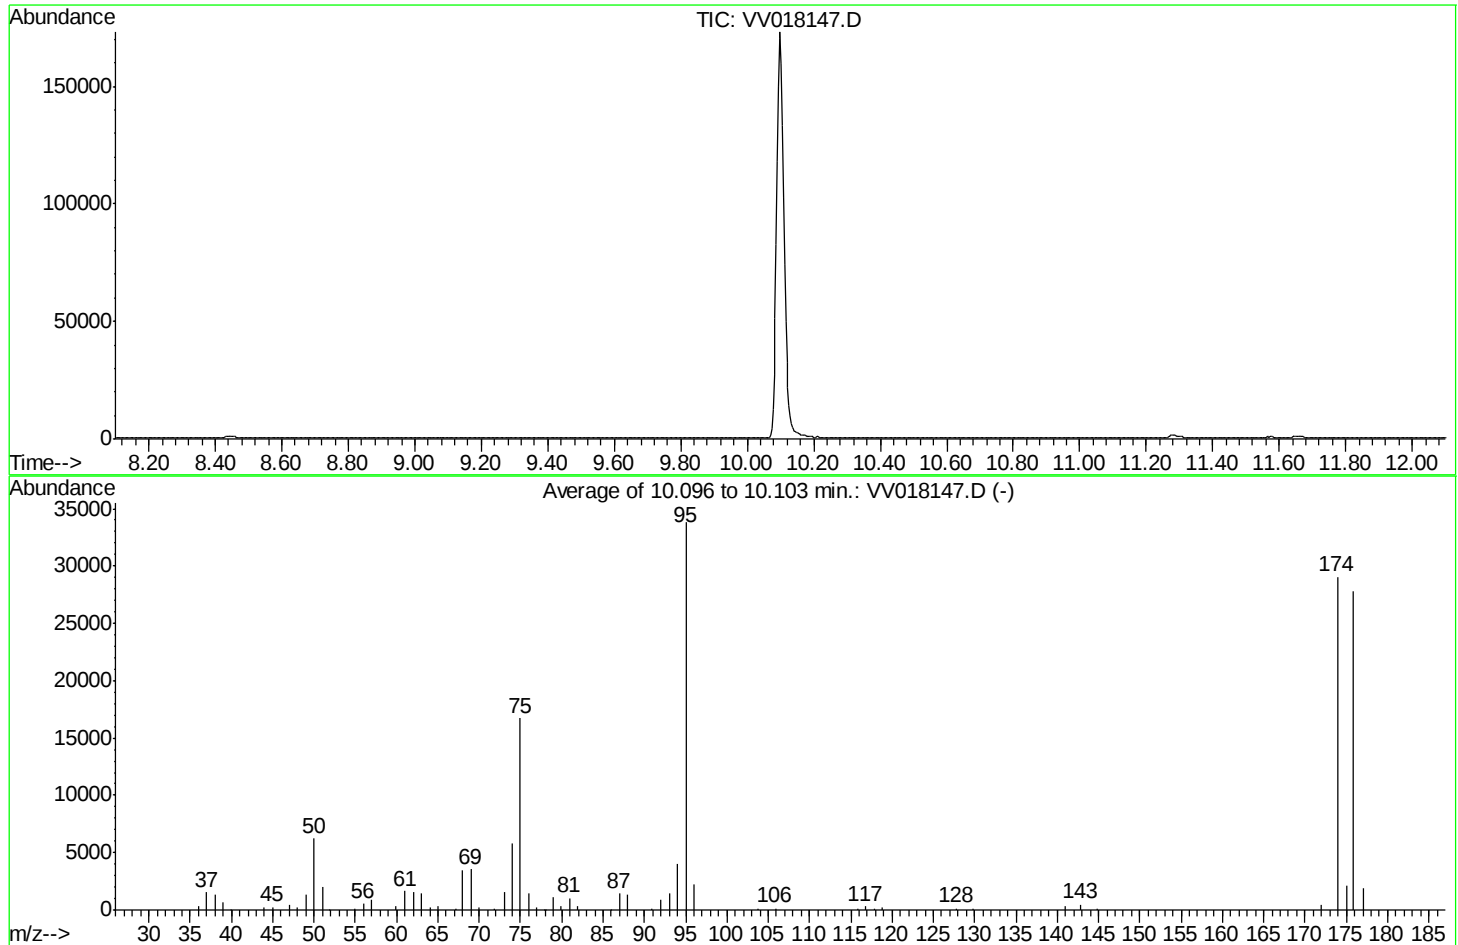

AutoFind: Scans 2801, 2802, 2803; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	6222	PASS
75	95	30	80	49.5	16734	PASS
95	95	100	100	100.0	33810	PASS
96	95	5	9	6.8	2292	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.9	29034	PASS
175	174	5	9	7.3	2123	PASS
176	174	95	101	95.8	27818	PASS
177	176	5	9	6.7	1869	PASS

m/z	Abundance
35.90	339.0
37.00	1561.0
38.00	1506.0
39.00	706.0
39.90	198.0
43.90	661.0
44.90	283.0
47.00	444.0
47.90	194.0
49.00	1472.0
50.00	6336.0
51.00	2071.0
51.90	102.0
55.00	119.0
56.00	538.0
57.00	960.0
59.90	384.0
61.00	1652.0
62.00	1620.0
63.00	1326.0
64.00	216.0
65.00	334.0
67.10	140.0
68.00	3452.0
69.00	3703.0
70.00	287.0
71.90	137.0
73.00	1584.0
74.00	6001.0
75.00	17280.0
76.00	1498.0
76.90	323.0
77.80	141.0
78.10	130.0
78.90	1141.0
79.90	323.0
80.90	1051.0
81.90	300.0
85.90	101.0
87.00	1480.0
87.90	1411.0
90.90	147.0
92.00	919.0
93.00	1600.0
94.00	4139.0
95.00	34608.0
96.00	2344.0
103.70	122.0
105.90	137.0
115.90	124.0
116.80	294.0
117.90	152.0
118.90	222.0
127.80	127.0
129.90	122.0
140.90	299.0
142.80	433.0
144.90	140.0
171.90	532.0
173.90	28760.0
175.00	2113.0
175.90	27656.0
177.00	1872.0

Instrument :
MSVOA_V
ClientSampleId :
BFB601

m/z	Abundance
36.00	347.0
37.00	1572.0
38.00	1431.0
39.00	709.0
39.90	201.0
43.90	603.0
45.00	268.0
46.90	438.0
48.00	197.0
49.00	1437.0
50.00	6466.0
51.00	2086.0
55.00	130.0
56.00	569.0
57.00	912.0
59.90	376.0
61.00	1738.0
62.00	1588.0
63.00	1463.0
64.00	187.0
65.00	293.0
67.10	139.0
68.00	3549.0
69.00	3665.0
70.00	254.0
71.80	156.0
73.00	1571.0
74.00	6017.0
75.00	17336.0
76.00	1528.0
77.00	293.0
78.90	1182.0
79.90	336.0
80.90	1068.0
81.90	317.0
87.00	1496.0
87.90	1365.0
90.90	175.0
92.00	917.0
93.00	1529.0
94.00	4103.0
95.00	34960.0
96.00	2384.0
103.70	124.0
105.90	147.0
115.80	130.0
116.80	293.0
117.90	166.0
118.90	235.0
127.80	119.0
129.90	119.0
140.90	329.0
142.90	475.0
144.90	162.0
171.90	496.0
173.90	30112.0
175.00	2179.0
175.90	28792.0
177.00	1940.0

Instrument :
MSVOA_V
ClientSampleId :
BFB601

m/z	Abundance
36.00	303.0
37.00	1440.0
38.00	1257.0
39.00	634.0
39.90	261.0
44.00	530.0
45.00	259.0
46.90	423.0
48.00	203.0
49.00	1282.0
50.00	5864.0
51.00	1896.0
55.00	124.0
56.00	508.0
57.00	803.0
59.90	326.0
61.00	1637.0
62.00	1479.0
63.00	1433.0
64.00	169.0
65.00	278.0
67.10	105.0
68.00	3338.0
69.00	3277.0
70.00	214.0
71.90	170.0
73.00	1413.0
74.00	5467.0
75.00	15587.0
76.00	1378.0
77.00	228.0
78.90	1079.0
79.90	339.0
80.90	999.0
81.90	283.0
87.00	1335.0
87.90	1244.0
90.90	169.0
92.00	890.0
93.00	1347.0
94.00	3679.0
95.00	31864.0
96.00	2149.0
103.70	114.0
105.90	148.0
115.80	139.0
116.80	277.0
117.90	158.0
118.80	213.0
127.80	113.0
129.80	116.0
140.90	332.0
142.90	482.0
144.90	158.0
171.90	410.0
173.90	28232.0
175.00	2077.0
175.90	27008.0
177.00	1796.0

Instrument :
MSVOA_V
ClientSampleId :
BFB601

Scan 2790 (10.061 min): VV018147.D
BFB601

m/z	Abundance
39.90	175.0
44.00	422.0

Instrument :
MSVOA_V
ClientSampleId :
BFB601