

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
 Data File : VV007343.D
 Acq On : 04 Sep 2018 22:02
 Operator : SY/MD
 Sample : VV0904WBL01
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK72

Quant Time: Sep 05 01:28:29 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 05 01:26:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	554214	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	522845	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	199111	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	178266	45.03	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	90.06%
7) Chloroethane-d5	1.57	69	107663	41.52	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	83.04%
11) 1,1-Dichloroethene-d2	2.13	63	242757	34.81	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	69.62%
21) 2-Butanone-d5	3.96	46	290962	90.36	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	90.36%
24) Chloroform-d	4.41	84	366763	44.79	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	89.58%
26) 1,2-Dichloroethane-d4	5.09	65	228671	46.29	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.58%
32) Benzene-d6	5.10	84	742530	47.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.24%
36) 1,2-Dichloropropane-d6	6.12	67	247889	46.94	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.88%
41) Toluene-d8	7.37	98	605182	44.61	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.22%
43) trans-1,3-Dichloropropene-	7.67	79	98572	43.82	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	87.64%
47) 2-Hexanone-d5	8.14	63	190288	91.92	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.92%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	318411	44.14	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.28%
64) 1,2-Dichlorobenzene-d4	11.68	152	216813	50.67	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.34%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
59) 1,2,3-Trichloropropane	11.30	75	23358	4.273	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007343.D
Acq On : 04 Sep 2018 22:02
Operator : SY/MD
Sample : VV0904WBL01
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK72

Quant Time: Sep 05 01:28:29 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 05 01:26:02 2018
Response via : Initial Calibration

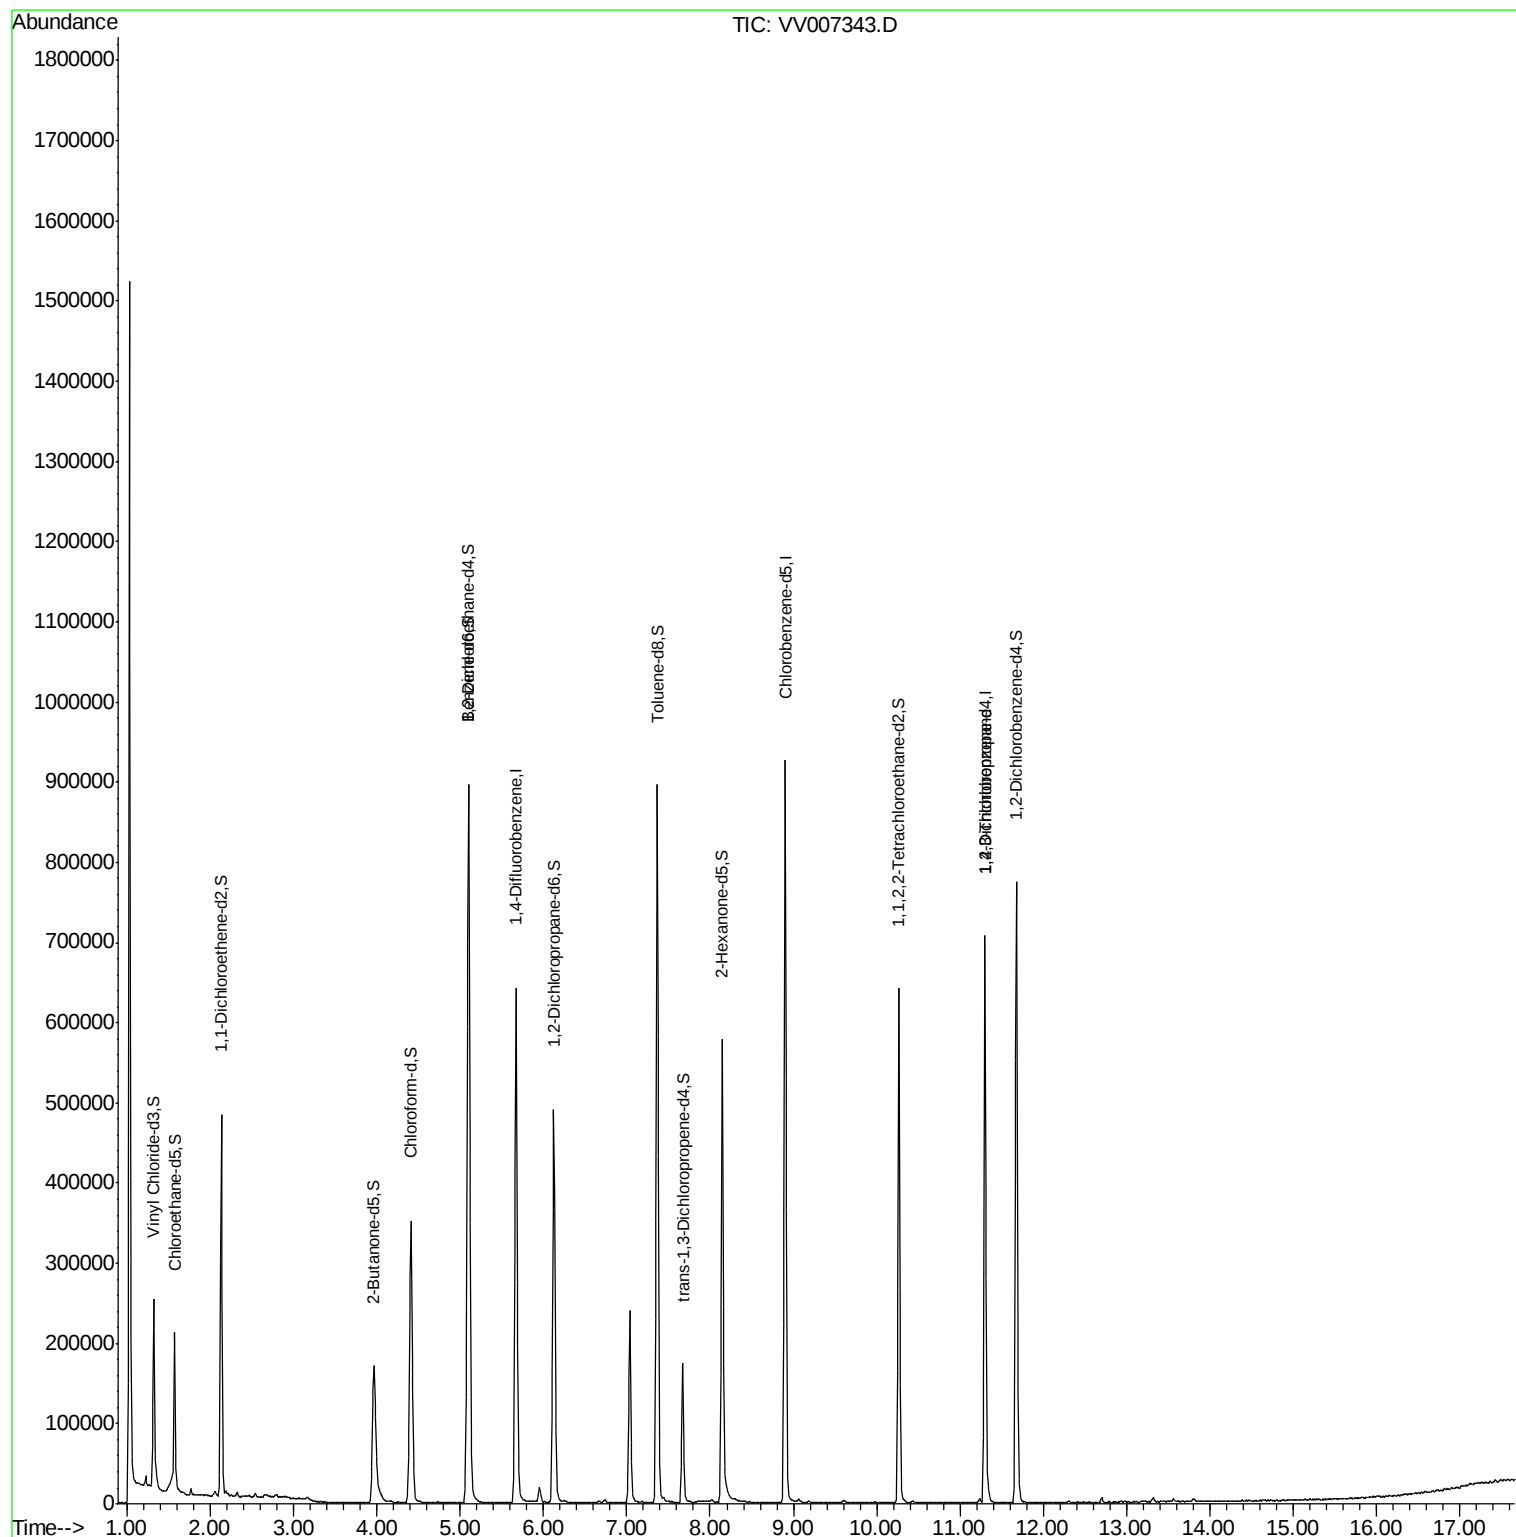

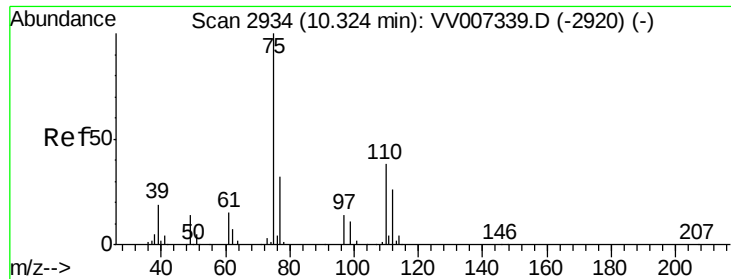

#59

1,2,3-Trichloropropane

Concen: 4.273 ug/L

RT: 11.30 min Scan# 3237

Delta R.T. 0.97 min

Lab File: VV007343.D

Acq: 04 Sep 2018 22:02

Instrument :

MSVOA_V

ClientSampleId :

VBLK72

Tgt Ion: 75 Resp: 23358

Ion Ratio Lower Upper

75 100

77 33.1 25.5 38.3

