

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007347.D
 Acq On : 04 Sep 2018 23:41
 Operator : SY/MD
 Sample : J4695-02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.945	11	17	19	rBV2	591	469	0.002%	0.0002%
2	0.974	23	26	28	rVB2	469	242	0.001%	0.0001%
3	1.029	28	43	66	rBV	2226183	2689927	100.00%	12.982%
4	1.321	128	134	152	rVB	234911	291054	10.82%	1.405%
5	1.569	206	211	227	rVB	204831	248614	9.24%	1.200%
6	2.131	376	386	398	rBV	450095	626897	23.31%	3.025%
7	2.199	401	407	418	rVB	25524	39172	1.46%	0.189%
8	2.794	584	592	605	rVB	26850	45856	1.70%	0.221%
9	3.437	789	792	796	rVB3	739	518	0.002%	0.0002%
10	3.466	798	801	802	rBV2	714	332	0.001%	0.0002%
11	3.498	809	811	815	rVV3	551	199	0.001%	0.0001%
12	3.517	815	817	820	rVB2	679	375	0.001%	0.0002%
13	3.533	820	822	826	rBV2	274	180	0.001%	0.0001%
14	3.678	864	867	870	rBV2	329	265	0.001%	0.0001%
15	3.832	913	915	918	rVB2	398	225	0.001%	0.0001%
16	3.868	924	926	930	rBV3	559	448	0.002%	0.0002%
17	3.900	933	936	937	rVV2	716	392	0.001%	0.0002%
18	3.967	938	957	1004	rVV2	903300	2287628	85.04%	11.040%
19	4.408	1073	1094	1119	rBV	341029	820233	30.49%	3.958%
20	4.607	1154	1156	1158	rBV	382	182	0.001%	0.0001%
21	4.623	1158	1161	1164	rBV3	434	327	0.001%	0.0002%
22	4.729	1183	1194	1205	rVV6	7512	16129	0.60%	0.078%
23	4.790	1210	1213	1216	rBV4	648	402	0.001%	0.0002%
24	4.864	1232	1236	1238	rBV2	360	271	0.001%	0.0001%
25	4.877	1238	1240	1243	rVV2	395	240	0.001%	0.0001%
26	5.099	1290	1309	1354	rBV2	857801	2078695	77.28%	10.032%
27	5.308	1372	1374	1381	rVB4	886	870	0.003%	0.0004%
28	5.353	1386	1388	1392	rVB2	489	269	0.001%	0.0001%
29	5.389	1397	1399	1403	rBV3	480	348	0.001%	0.0002%
30	5.446	1415	1417	1419	rBV2	496	198	0.001%	0.0001%
31	5.504	1433	1435	1437	rBV2	513	293	0.001%	0.0001%
32	5.671	1472	1487	1512	rBV	582838	1149474	42.73%	5.547%
33	5.964	1562	1578	1595	rBV	212694	415781	15.46%	2.007%
34	6.125	1613	1628	1648	rBV	474100	948257	35.25%	4.576%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007347.D
 Acq On : 04 Sep 2018 23:41
 Operator : SY/MD
 Sample : J4695-02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.321	1686	1689	1692	rBV3	647	389	0.01%	0.002%
36	6.343	1693	1696	1700	rVV3	695	484	0.02%	0.002%
37	6.604	1772	1777	1779	rBV3	562	449	0.02%	0.002%
38	6.646	1785	1790	1798	rBV7	924	1365	0.05%	0.007%
39	6.726	1807	1815	1826	rBV4	2826	5855	0.22%	0.028%
40	6.942	1878	1882	1885	rVB5	550	425	0.02%	0.002%
41	7.035	1898	1911	1929	rBV	224048	398189	14.80%	1.922%
42	7.144	1943	1945	1948	rBV2	741	488	0.02%	0.002%
43	7.208	1962	1965	1968	rBV3	813	461	0.02%	0.002%
44	7.266	1978	1983	1985	rBV3	747	535	0.02%	0.003%
45	7.289	1986	1990	1992	rBV	983	725	0.03%	0.003%
46	7.366	2000	2014	2031	rBV	808509	1418709	52.74%	6.847%
47	7.668	2097	2108	2135	rVB	163867	278045	10.34%	1.342%
48	7.797	2144	2148	2151	rBV3	572	472	0.02%	0.002%
49	8.022	2203	2218	2238	rVB	710344	1186811	44.12%	5.728%
50	8.144	2243	2256	2285	rBV	565026	1022329	38.01%	4.934%
51	8.658	2412	2416	2418	rBV3	724	547	0.02%	0.003%
52	8.697	2424	2428	2431	rBV3	620	536	0.02%	0.003%
53	8.768	2447	2450	2454	rVV3	958	703	0.03%	0.003%
54	8.822	2464	2467	2472	rBV6	524	463	0.02%	0.002%
55	8.900	2478	2491	2513	rBV	836474	1350847	50.22%	6.519%
56	9.179	2570	2578	2580	rBV7	1705	1968	0.07%	0.009%
57	9.231	2591	2594	2595	rBV2	919	458	0.02%	0.002%
58	9.475	2668	2670	2674	rVB	514	286	0.01%	0.001%
59	9.511	2679	2681	2686	rVB4	481	312	0.01%	0.002%
60	9.646	2717	2723	2727	rBV4	873	1103	0.04%	0.005%
61	9.765	2755	2760	2763	rVB4	1018	926	0.03%	0.004%
62	9.855	2785	2788	2791	rBV3	285	198	0.01%	0.001%
63	9.887	2795	2798	2801	rBV3	455	373	0.01%	0.002%
64	9.951	2815	2818	2821	rBV	371	295	0.01%	0.001%
65	9.980	2821	2827	2834	rVB4	473	608	0.02%	0.003%
66	10.038	2843	2845	2847	rBV2	394	186	0.01%	0.001%
67	10.118	2868	2870	2874	rVB3	362	232	0.01%	0.001%
68	10.266	2903	2916	2948	rBV	640856	1019466	37.90%	4.920%
69	10.427	2953	2966	2977	rBV5	4406	8611	0.32%	0.042%
70	10.469	2977	2979	2981	rBV2	380	233	0.01%	0.001%
71	10.536	2998	3000	3005	rVB	399	288	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007347.D
 Acq On : 04 Sep 2018 23:41
 Operator : SY/MD
 Sample : J4695-02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.584	3012	3015	3018	rVB4	460	283	0.01%	0.001%
73	10.617	3022	3025	3028	rBV4	436	240	0.01%	0.001%
74	10.681	3043	3045	3049	rVB2	365	234	0.01%	0.001%
75	10.761	3064	3070	3076	rBV3	623	809	0.03%	0.004%
76	10.867	3100	3103	3108	rVB3	402	317	0.01%	0.002%
77	10.909	3108	3116	3127	rBV6	2469	4686	0.17%	0.023%
78	11.089	3170	3172	3174	rBV2	430	194	0.01%	0.001%
79	11.154	3182	3192	3194	rBV5	2409	3390	0.13%	0.016%
80	11.234	3210	3217	3223	rVB5	2148	2616	0.10%	0.013%
81	11.298	3224	3237	3265	rBV	659822	1081326	40.20%	5.218%
82	11.453	3282	3285	3288	rBV4	793	458	0.02%	0.002%
83	11.504	3299	3301	3305	rVB3	609	277	0.01%	0.001%
84	11.559	3314	3318	3319	rBV	506	372	0.01%	0.002%
85	11.588	3322	3327	3329	rBV4	1179	1173	0.04%	0.006%
86	11.678	3342	3355	3380	rBV	772575	1245391	46.30%	6.010%
87	11.797	3389	3392	3394	rBV2	441	251	0.01%	0.001%
88	11.838	3402	3405	3407	rBV	690	341	0.01%	0.002%
89	11.893	3420	3422	3427	rVB2	717	339	0.01%	0.002%
90	11.935	3432	3435	3437	rBV3	499	303	0.01%	0.001%
91	12.237	3527	3529	3533	rBV2	564	457	0.02%	0.002%
92	12.282	3540	3543	3545	rBV2	781	569	0.02%	0.003%
93	12.395	3576	3578	3584	rVB3	1249	1049	0.04%	0.005%
94	12.459	3595	3598	3600	rBV3	669	402	0.01%	0.002%
95	12.938	3744	3747	3752	rBV4	999	933	0.03%	0.005%
96	12.983	3757	3761	3767	rBV3	632	818	0.03%	0.004%
97	13.121	3802	3804	3806	rBV2	651	250	0.01%	0.001%
98	13.317	3860	3865	3872	rVB7	1193	1648	0.06%	0.008%
99	13.485	3914	3917	3919	rBV3	692	374	0.01%	0.002%
100	14.430	4203	4211	4216	rBV7	1491	2540	0.09%	0.012%


Sum of corrected areas: 20721172

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090418\
Data File : VV007347.D
Acq On : 04 Sep 2018 23:41
Operator : SY/MD
Sample : J4695-02
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

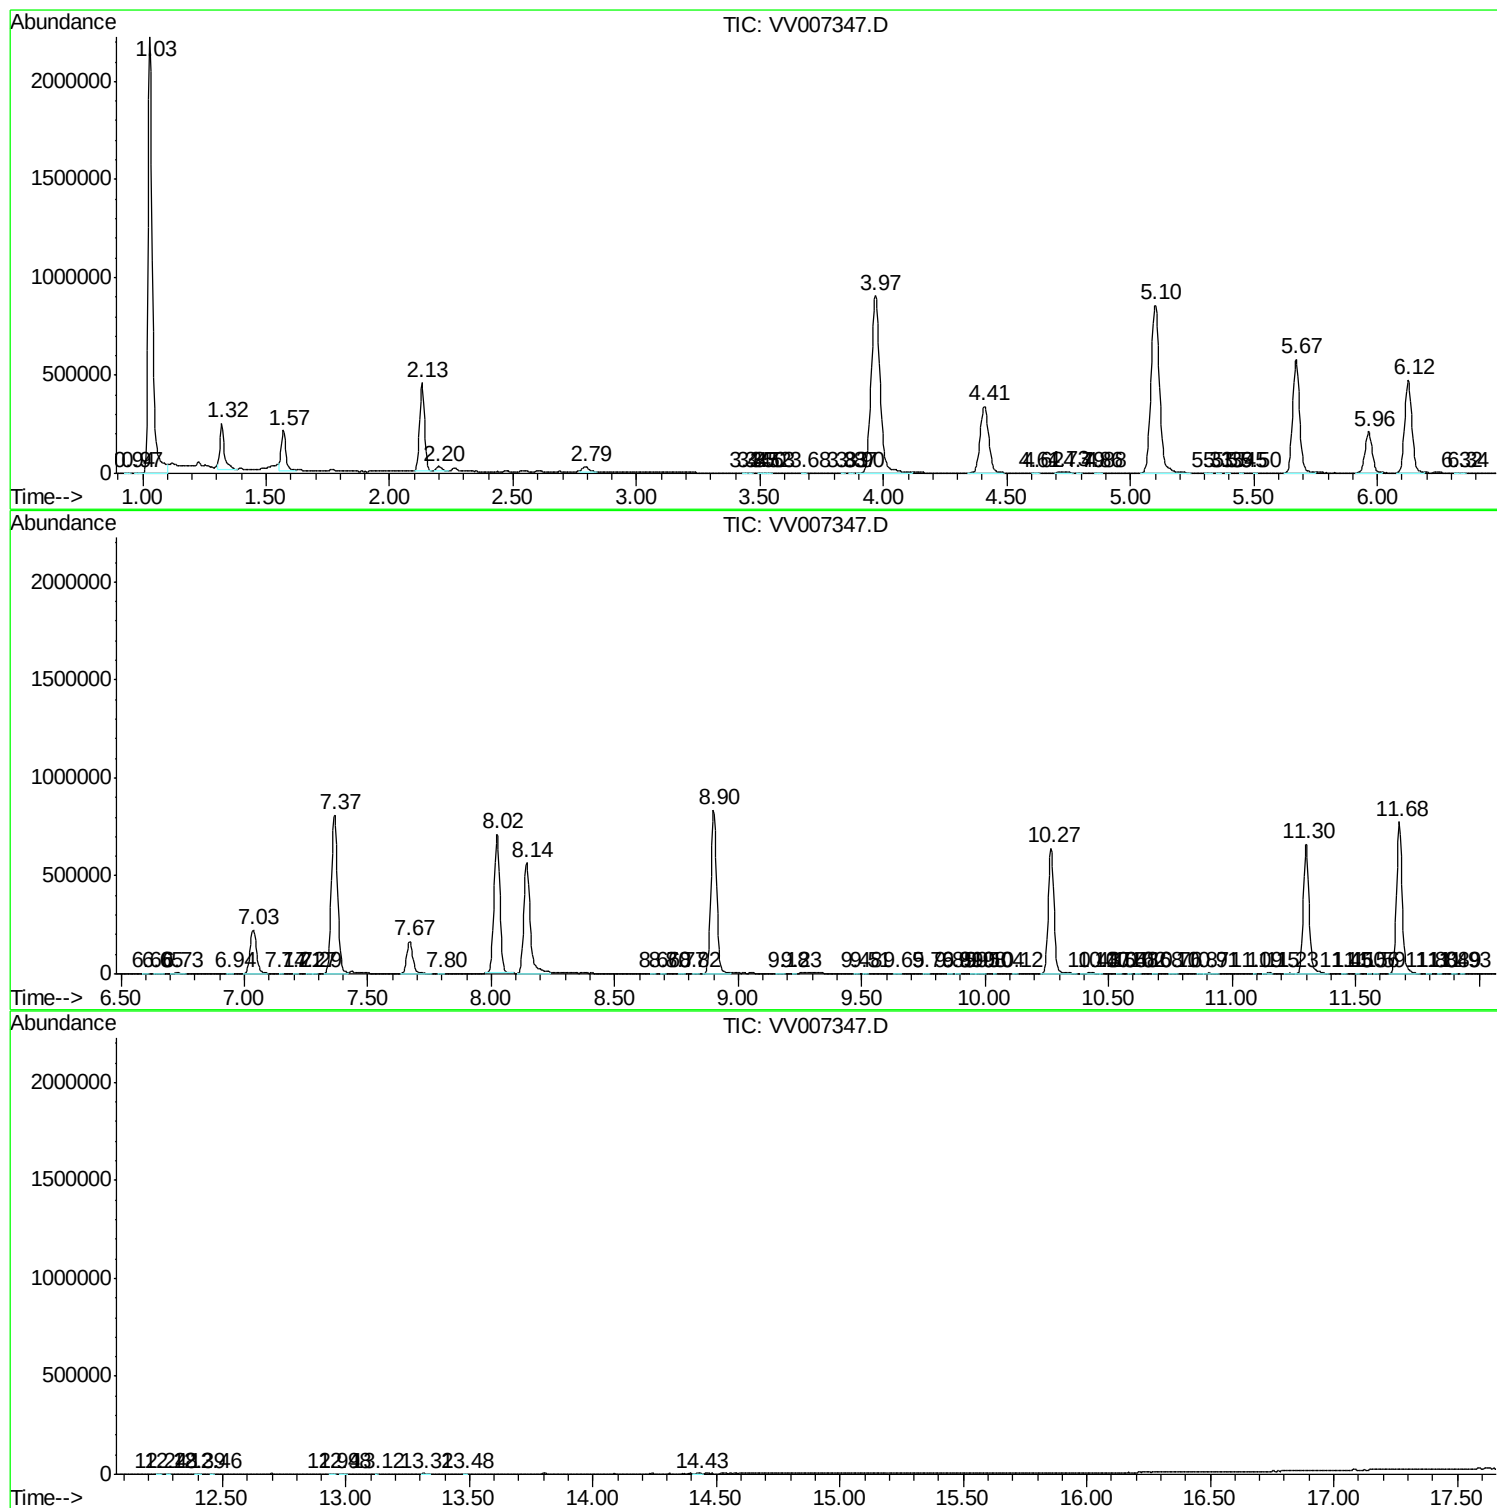

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007347.D
Acq On : 04 Sep 2018 23:41
Operator : SY/MD
Sample : J4695-02
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007347.D
Acq On : 04 Sep 2018 23:41
Operator : SY/MD
Sample : J4695-02
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE43

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc