

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007348.D
 Acq On : 05 Sep 2018 00:06
 Operator : SY/MD
 Sample : J4695-03
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.942	13	16	23	rVB3	537	512	0.02%	0.003%
2	0.980	23	28	30	rBV2	281	240	0.01%	0.001%
3	1.029	30	43	66	rBV	2425761	2960863	100.00%	15.717%
4	1.257	109	114	125	rVB	59306	76575	2.59%	0.406%
5	1.321	128	134	152	rVB	227659	271646	9.17%	1.442%
6	1.527	194	198	203	rBV	32385	35748	1.21%	0.190%
7	1.572	206	212	227	rVB	190639	229998	7.77%	1.221%
8	2.131	376	386	398	rBV	434149	609715	20.59%	3.237%
9	2.202	402	408	418	rVV	35148	56414	1.91%	0.299%
10	2.263	418	427	439	rVB	264245	383783	12.96%	2.037%
11	3.369	768	771	774	rBV4	487	423	0.01%	0.002%
12	3.440	790	793	797	rBV4	775	566	0.02%	0.003%
13	3.472	801	803	805	rBV2	476	285	0.01%	0.002%
14	3.581	832	837	840	rBV4	590	693	0.02%	0.004%
15	3.649	854	858	860	rBV3	366	287	0.01%	0.002%
16	3.672	863	865	868	rVV	700	330	0.01%	0.002%
17	3.700	868	874	875	rVV3	363	324	0.01%	0.002%
18	3.765	881	894	909	rBV6	2783	7266	0.25%	0.039%
19	3.964	934	956	981	rBV2	248917	690488	23.32%	3.665%
20	4.305	1058	1062	1065	rBV3	456	456	0.02%	0.002%
21	4.408	1074	1094	1129	rBV	330152	800413	27.03%	4.249%
22	4.610	1155	1157	1159	rBV2	569	341	0.01%	0.002%
23	4.636	1159	1165	1168	rVV2	358	352	0.01%	0.002%
24	4.655	1168	1171	1172	rBV3	723	361	0.01%	0.002%
25	4.729	1181	1194	1209	rBV9	5210	13554	0.46%	0.072%
26	4.909	1245	1250	1254	rBV4	562	523	0.02%	0.003%
27	4.990	1272	1275	1278	rBV2	382	342	0.01%	0.002%
28	5.025	1281	1286	1289	rVB2	447	340	0.01%	0.002%
29	5.102	1291	1310	1347	rBV2	813455	2000587	67.57%	10.620%
30	5.376	1386	1395	1397	rBV5	1719	2062	0.07%	0.011%
31	5.495	1429	1432	1435	rBV	501	337	0.01%	0.002%
32	5.559	1448	1452	1453	rBV	989	667	0.02%	0.004%
33	5.671	1472	1487	1511	rBV	575165	1138996	38.47%	6.046%
34	5.964	1565	1578	1595	rVB3	44445	95014	3.21%	0.504%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007348.D
 Acq On : 05 Sep 2018 00:06
 Operator : SY/MD
 Sample : J4695-03
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.054	1603	1606	1607	rBV3	829	445	0.02%	0.002%
36	6.125	1613	1628	1648	rBV	453318	906676	30.62%	4.813%
37	6.347	1685	1697	1708	rBV3	9120	19548	0.66%	0.104%
38	6.530	1751	1754	1756	rBV2	504	281	0.01%	0.001%
39	6.549	1756	1760	1761	rBV2	394	284	0.01%	0.002%
40	6.633	1784	1786	1788	rBV2	552	346	0.01%	0.002%
41	6.726	1808	1815	1827	rVV3	1959	4110	0.14%	0.022%
42	6.806	1837	1840	1842	rBV	434	279	0.01%	0.001%
43	6.925	1874	1877	1880	rBV2	998	697	0.02%	0.004%
44	7.035	1895	1911	1933	rBV	213537	383104	12.94%	2.034%
45	7.244	1974	1976	1979	rBV3	480	275	0.01%	0.001%
46	7.292	1979	1991	1999	rBV8	3111	5898	0.20%	0.031%
47	7.366	2000	2014	2031	rBV	785079	1364320	46.08%	7.242%
48	7.630	2093	2096	2097	rBV2	771	334	0.01%	0.002%
49	7.668	2097	2108	2130	rVV	153718	264663	8.94%	1.405%
50	7.890	2174	2177	2182	rBV6	1108	1063	0.04%	0.006%
51	8.022	2203	2218	2239	rVB	580778	981951	33.16%	5.213%
52	8.144	2244	2256	2283	rBV	504287	909701	30.72%	4.829%
53	8.292	2297	2302	2317	rVB4	13885	24826	0.84%	0.132%
54	8.472	2356	2358	2361	rBV2	525	378	0.01%	0.002%
55	8.520	2368	2373	2377	rBV6	511	591	0.02%	0.003%
56	8.630	2403	2407	2412	rBV5	668	698	0.02%	0.004%
57	8.774	2444	2452	2458	rVB5	2192	3133	0.11%	0.017%
58	8.832	2468	2470	2474	rBV2	480	324	0.01%	0.002%
59	8.900	2478	2491	2512	rBV	819908	1343625	45.38%	7.132%
60	9.228	2590	2593	2594	rBV2	586	314	0.01%	0.002%
61	9.247	2594	2599	2600	rBV4	2121	1607	0.05%	0.009%
62	9.501	2676	2678	2682	rVB2	585	288	0.01%	0.002%
63	9.607	2706	2711	2715	rVB5	1528	1470	0.05%	0.008%
64	9.646	2715	2723	2731	rBV5	1666	2223	0.08%	0.012%
65	9.720	2742	2746	2747	rVV3	466	276	0.01%	0.001%
66	9.755	2747	2757	2764	rVV5	3828	6401	0.22%	0.034%
67	9.784	2764	2766	2771	rVB4	736	601	0.02%	0.003%
68	9.858	2781	2789	2799	rBV5	7248	11442	0.39%	0.061%
69	9.967	2819	2823	2824	rBV	423	279	0.01%	0.001%
70	9.983	2826	2828	2833	rVB4	687	556	0.02%	0.003%
71	10.057	2847	2851	2855	rBV5	530	375	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007348.D
 Acq On : 05 Sep 2018 00:06
 Operator : SY/MD
 Sample : J4695-03
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE44

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.089	2857	2861	2864	rBV	333	296	0.01%	0.002%
73	10.137	2874	2876	2880	rBV2	355	257	0.01%	0.001%
74	10.266	2904	2916	2932	rBV	593960	932158	31.48%	4.948%
75	10.427	2956	2966	2973	rBV5	4331	8316	0.28%	0.044%
76	10.565	2999	3009	3015	rBV7	1504	2656	0.09%	0.014%
77	10.629	3026	3029	3037	rVB4	1485	1632	0.06%	0.009%
78	10.732	3052	3061	3070	rBV8	3271	5437	0.18%	0.029%
79	10.848	3095	3097	3100	rBV3	441	304	0.01%	0.002%
80	10.909	3109	3116	3124	rBV4	3573	5148	0.17%	0.027%
81	11.080	3167	3169	3170	rBV	566	247	0.01%	0.001%
82	11.160	3185	3194	3198	rBV8	3761	6086	0.21%	0.032%
83	11.298	3225	3237	3265	rBV	665987	1062974	35.90%	5.643%
84	11.588	3320	3327	3328	rBV7	2313	2580	0.09%	0.014%
85	11.678	3342	3355	3382	rVB	726031	1168969	39.48%	6.205%
86	11.880	3413	3418	3425	rBV6	3433	4517	0.15%	0.024%
87	11.954	3438	3441	3445	rBV2	687	466	0.02%	0.002%
88	12.018	3459	3461	3463	rBV	445	249	0.01%	0.001%
89	12.289	3541	3545	3546	rBV3	1073	818	0.03%	0.004%
90	12.398	3572	3579	3590	rBV8	3295	4935	0.17%	0.026%
91	12.662	3659	3661	3665	rBV2	561	288	0.01%	0.002%
92	12.793	3696	3702	3706	rBV2	789	906	0.03%	0.005%
93	12.813	3706	3708	3711	rBV3	632	335	0.01%	0.002%
94	12.935	3742	3746	3749	rBV2	1070	892	0.03%	0.005%
95	13.166	3816	3818	3820	rBV3	541	317	0.01%	0.002%
96	13.420	3894	3897	3898	rBV2	681	378	0.01%	0.002%
97	13.957	4062	4064	4067	rVB2	884	382	0.01%	0.002%
98	14.009	4075	4080	4086	rBV7	1048	1429	0.05%	0.008%
99	14.038	4086	4089	4092	rBV2	802	646	0.02%	0.003%
100	14.169	4128	4130	4134	rBV5	871	695	0.02%	0.004%


Sum of corrected areas: 18838196

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090418\
Data File : VV007348.D
Acq On : 05 Sep 2018 00:06
Operator : SY/MD
Sample : J4695-03
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

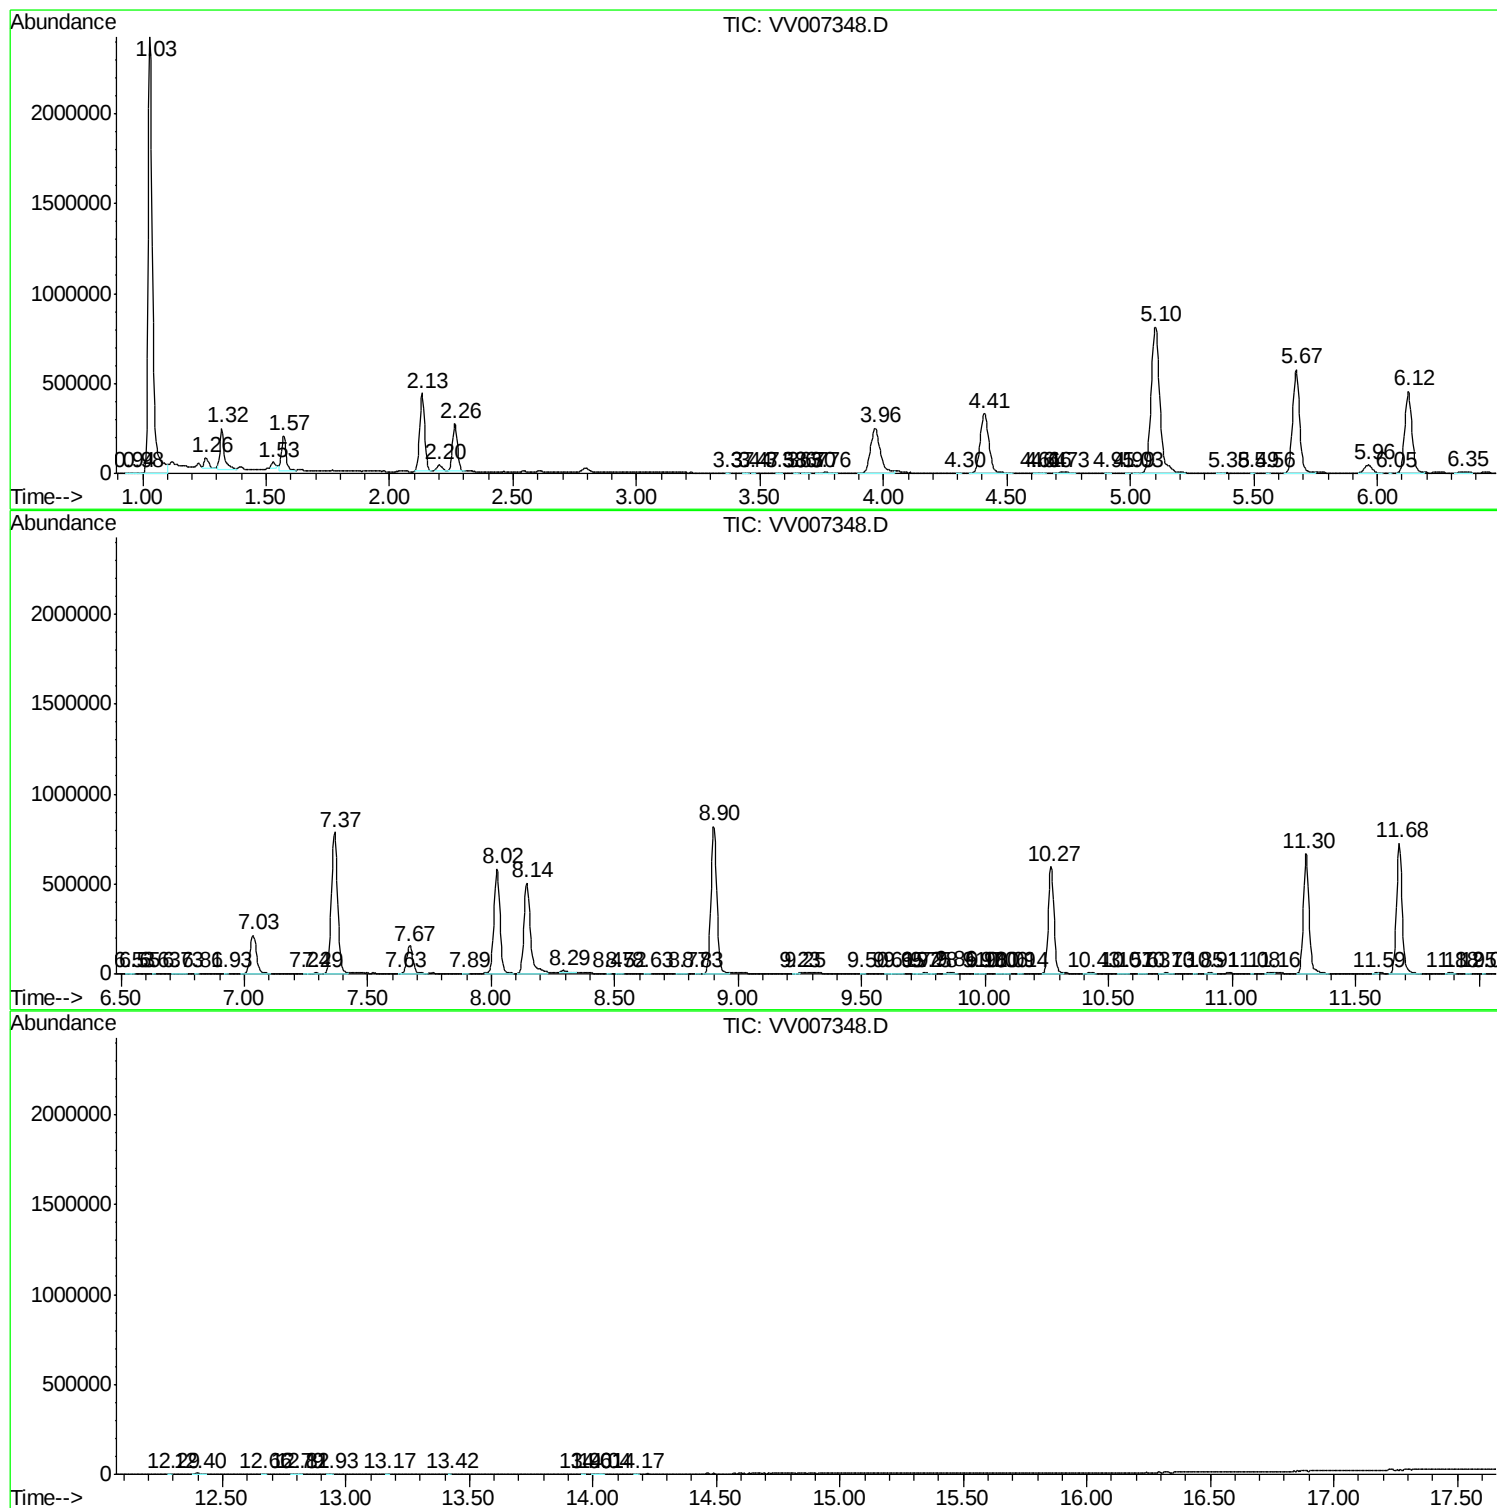

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007348.D
Acq On : 05 Sep 2018 00:06
Operator : SY/MD
Sample : J4695-03
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007348.D
Acq On : 05 Sep 2018 00:06
Operator : SY/MD
Sample : J4695-03
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE44

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc