

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007349.D
 Acq On : 05 Sep 2018 00:31
 Operator : SY/MD
 Sample : J4695-04
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.910	4	6	10	rVB2	562	417	0.02%	0.003%
2	0.942	10	16	19	rBV2	668	618	0.03%	0.004%
3	1.029	29	43	66	rBV	1200584	1441404	74.48%	8.729%
4	1.321	126	134	149	rVB	229173	289474	14.96%	1.753%
5	1.572	207	212	227	rVB	191999	220560	11.40%	1.336%
6	2.131	376	386	399	rBV	436859	612571	31.65%	3.710%
7	3.299	745	749	752	rBV4	718	678	0.04%	0.004%
8	3.485	803	807	810	rBV4	625	470	0.02%	0.003%
9	3.723	876	881	886	rBV3	511	485	0.03%	0.003%
10	3.758	886	892	895	rBV4	656	800	0.04%	0.005%
11	3.807	905	907	908	rBV	263	130	0.01%	0.001%
12	3.826	911	913	917	rVB2	579	336	0.02%	0.002%
13	3.871	923	927	928	rBV	347	259	0.01%	0.002%
14	3.967	939	957	994	rBV3	482863	1264702	65.35%	7.659%
15	4.408	1076	1094	1119	rBV	322170	764481	39.50%	4.630%
16	4.681	1176	1179	1181	rBV3	638	383	0.02%	0.002%
17	4.726	1181	1193	1207	rVV5	7091	17023	0.88%	0.103%
18	4.819	1219	1222	1223	rBV2	255	152	0.01%	0.001%
19	4.855	1231	1233	1236	rVV2	218	82	0.00%	0.000%
20	4.877	1238	1240	1244	rVB3	271	147	0.01%	0.001%
21	4.961	1264	1266	1268	rBV	280	143	0.01%	0.001%
22	4.974	1268	1270	1275	rVV3	305	210	0.01%	0.001%
23	5.012	1280	1282	1285	rVB2	325	150	0.01%	0.001%
24	5.099	1290	1309	1352	rBV2	807247	1935309	100.00%	11.720%
25	5.273	1359	1363	1366	rVB3	431	298	0.02%	0.002%
26	5.360	1388	1390	1391	rBV3	281	144	0.01%	0.001%
27	5.450	1412	1418	1431	rVB8	967	1738	0.09%	0.011%
28	5.549	1445	1449	1451	rBV2	310	189	0.01%	0.001%
29	5.565	1451	1454	1457	rBV2	433	247	0.01%	0.001%
30	5.591	1459	1462	1465	rVB3	550	289	0.01%	0.002%
31	5.614	1468	1469	1470	rBV3	171	65	0.00%	0.000%
32	5.672	1471	1487	1510	rBV	581912	1150139	59.43%	6.965%
33	5.964	1564	1578	1594	rBV2	110824	225021	11.63%	1.363%
34	6.125	1612	1628	1659	rBV	447213	900462	46.53%	5.453%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007349.D
 Acq On : 05 Sep 2018 00:31
 Operator : SY/MD
 Sample : J4695-04
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.363	1699	1702	1703	rBV2	471	317	0.02%	0.002%
36	6.588	1769	1772	1775	rBV2	430	375	0.02%	0.002%
37	6.607	1775	1778	1780	rBV4	517	390	0.02%	0.002%
38	6.646	1786	1790	1791	rBV2	475	370	0.02%	0.002%
39	6.700	1804	1807	1809	rBV2	399	251	0.01%	0.002%
40	6.729	1811	1816	1827	rVV6	1708	3227	0.17%	0.020%
41	6.823	1842	1845	1846	rBV2	420	199	0.01%	0.001%
42	6.861	1856	1857	1861	rVB2	379	179	0.01%	0.001%
43	6.890	1864	1866	1870	rVB3	677	405	0.02%	0.002%
44	6.932	1877	1879	1881	rBV	347	157	0.01%	0.001%
45	6.980	1893	1894	1896	rBV	266	134	0.01%	0.001%
46	7.035	1896	1911	1930	rVV	207427	375727	19.41%	2.275%
47	7.179	1954	1956	1958	rBV2	576	348	0.02%	0.002%
48	7.234	1968	1973	1979	rVB7	752	983	0.05%	0.006%
49	7.260	1979	1981	1983	rBV2	249	115	0.01%	0.001%
50	7.366	1999	2014	2031	rBV	811461	1399947	72.34%	8.478%
51	7.668	2097	2108	2126	rBV	151534	264561	13.67%	1.602%
52	8.022	2210	2218	2231	rVB2	34035	58136	3.00%	0.352%
53	8.144	2243	2256	2289	rBV	487348	901201	46.57%	5.457%
54	8.581	2390	2392	2393	rBV	287	82	0.00%	0.000%
55	8.671	2416	2420	2423	rBV2	744	596	0.03%	0.004%
56	8.707	2429	2431	2433	rVB2	383	150	0.01%	0.001%
57	8.729	2435	2438	2440	rBV3	673	430	0.02%	0.003%
58	8.771	2447	2451	2453	rBV2	436	396	0.02%	0.002%
59	8.900	2478	2491	2524	rBV	863822	1408412	72.77%	8.529%
60	9.183	2571	2579	2585	rBV5	1259	1760	0.09%	0.011%
61	9.279	2591	2609	2611	rBV4	5810	12561	0.65%	0.076%
62	9.491	2673	2675	2678	rVB3	410	197	0.01%	0.001%
63	9.578	2699	2702	2705	rBV4	600	535	0.03%	0.003%
64	9.655	2722	2726	2728	rBV	445	328	0.02%	0.002%
65	9.678	2731	2733	2740	rVB3	605	569	0.03%	0.003%
66	9.707	2740	2742	2745	rBV3	193	101	0.01%	0.001%
67	9.748	2753	2755	2760	rBV2	474	458	0.02%	0.003%
68	9.790	2766	2768	2769	rBV	235	107	0.01%	0.001%
69	9.861	2786	2790	2797	rVB4	503	586	0.03%	0.004%
70	9.999	2831	2833	2835	rBV2	376	207	0.01%	0.001%
71	10.019	2837	2839	2841	rVB	500	185	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007349.D
 Acq On : 05 Sep 2018 00:31
 Operator : SY/MD
 Sample : J4695-04
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE45

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.076	2854	2857	2859	rVB	278	137	0.01%	0.001%
73	10.093	2859	2862	2865	rBV2	517	312	0.02%	0.002%
74	10.138	2874	2876	2878	rBV	256	162	0.01%	0.001%
75	10.266	2903	2916	2951	rBV	604968	956755	49.44%	5.794%
76	10.427	2960	2966	2979	rVB3	5585	9597	0.50%	0.058%
77	10.507	2989	2991	2995	rVB3	512	271	0.01%	0.002%
78	10.530	2996	2998	3003	rVB3	467	316	0.02%	0.002%
79	10.777	3072	3075	3077	rBV	338	240	0.01%	0.001%
80	10.790	3077	3079	3082	rVB2	387	155	0.01%	0.001%
81	10.806	3082	3084	3088	rBV3	546	465	0.02%	0.003%
82	10.893	3110	3111	3112	rBV3	317	114	0.01%	0.001%
83	10.919	3117	3119	3124	rVB	634	348	0.02%	0.002%
84	10.945	3124	3127	3130	rVB3	592	352	0.02%	0.002%
85	10.977	3133	3137	3138	rBV2	485	321	0.02%	0.002%
86	11.060	3160	3163	3166	rBV2	398	271	0.01%	0.002%
87	11.083	3167	3170	3172	rBV2	408	260	0.01%	0.002%
88	11.144	3182	3189	3203	rBV2	4477	7314	0.38%	0.044%
89	11.298	3225	3237	3268	rBV	683915	1086543	56.14%	6.580%
90	11.485	3292	3295	3299	rBV3	657	456	0.02%	0.003%
91	11.678	3342	3355	3377	rBV	726779	1182790	61.12%	7.163%
92	12.157	3501	3504	3507	rBV2	596	361	0.02%	0.002%
93	12.826	3709	3712	3713	rBV	643	371	0.02%	0.002%
94	13.350	3873	3875	3878	rVB2	778	445	0.02%	0.003%
95	13.790	4010	4012	4015	rBV2	796	559	0.03%	0.003%


Sum of corrected areas: 16513173

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090418\
Data File : VV007349.D
Acq On : 05 Sep 2018 00:31
Operator : SY/MD
Sample : J4695-04
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

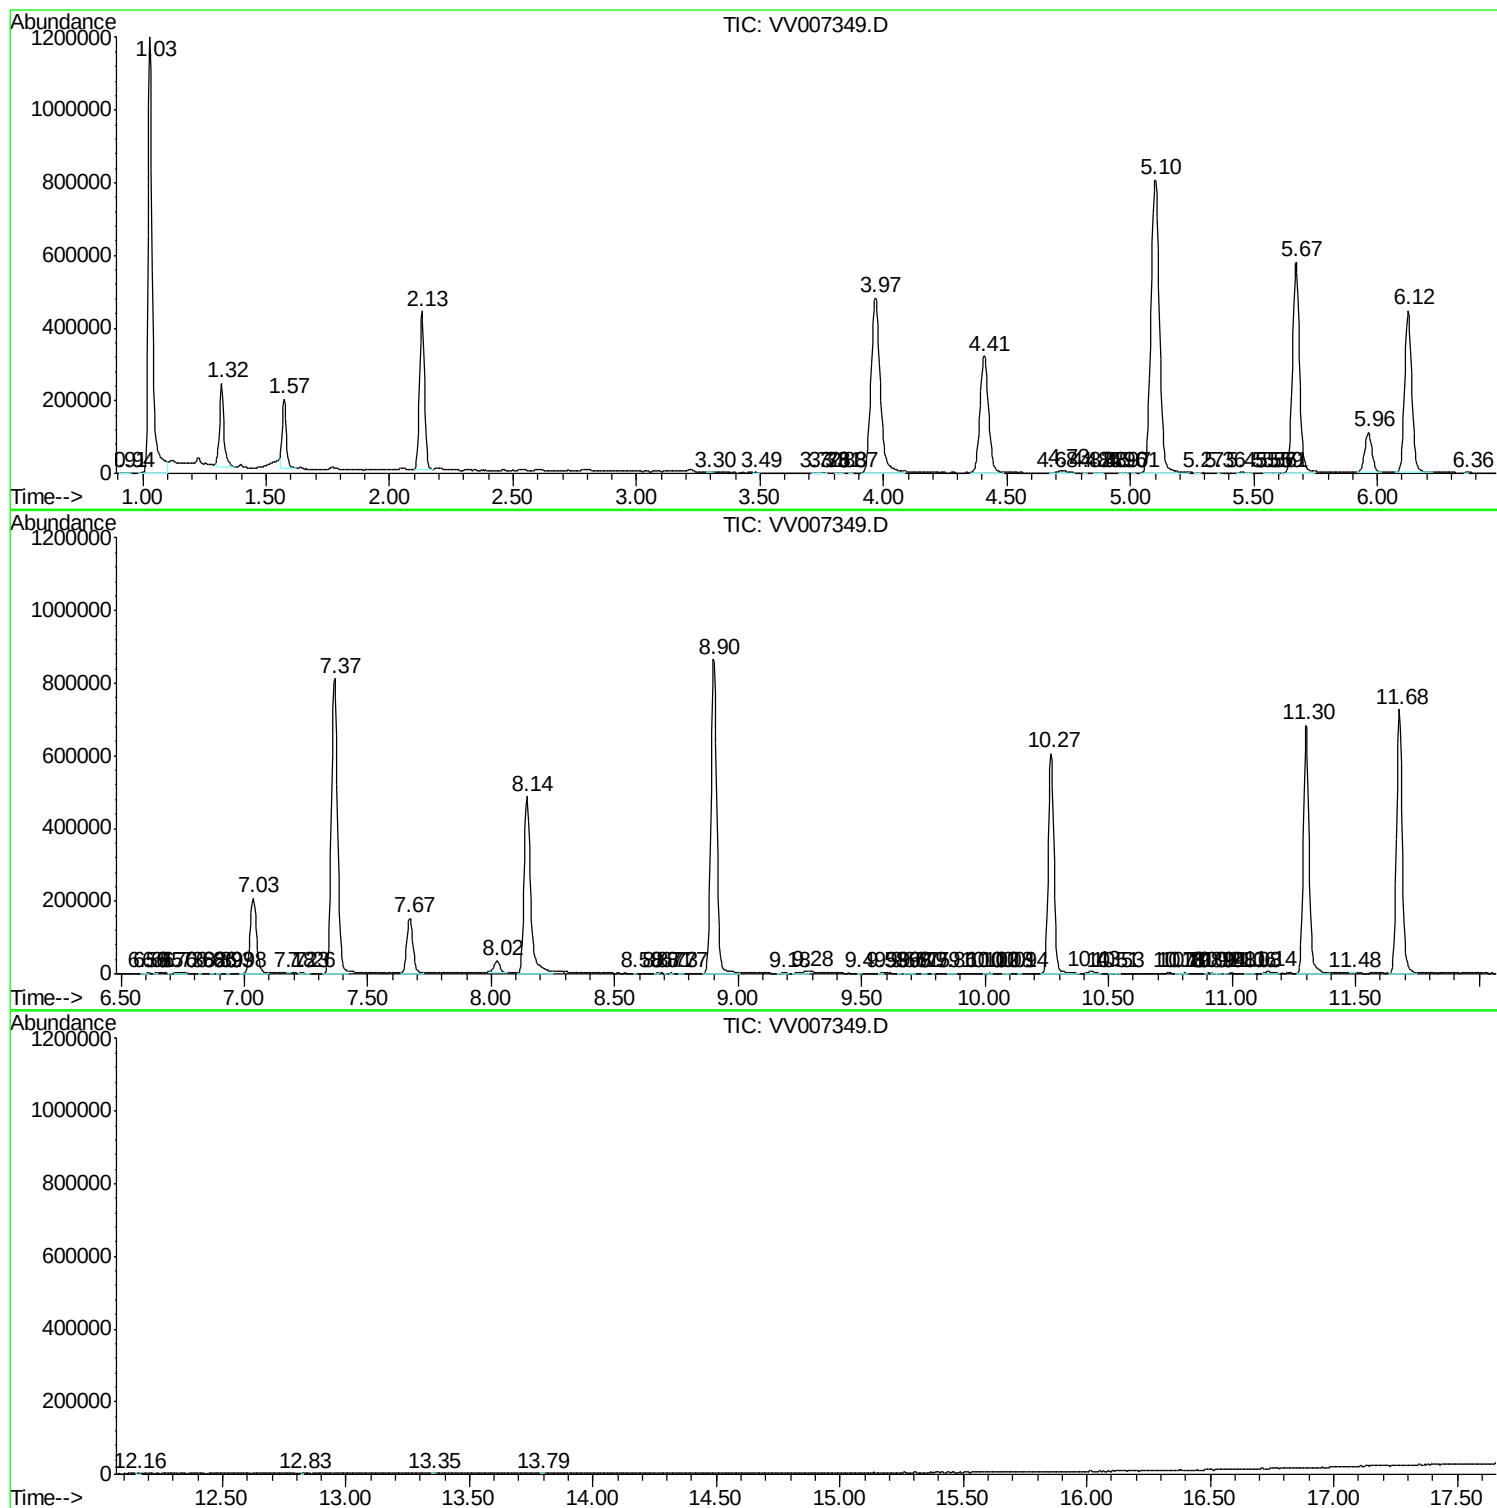

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007349.D
Acq On : 05 Sep 2018 00:31
Operator : SY/MD
Sample : J4695-04
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007349.D
Acq On : 05 Sep 2018 00:31
Operator : SY/MD
Sample : J4695-04
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE45

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc