

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007352.D
 Acq On : 05 Sep 2018 01:45
 Operator : SY/MD
 Sample : J4695-07
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.974	23	26	28	rBV2	538	353	0.002%	0.0002%
2	1.029	28	43	64	rBV	978610	1180205	58.77%	7.623%
3	1.321	127	134	151	rVB	235521	273177	13.60%	1.764%
4	1.569	206	211	228	rVB	197239	227670	11.34%	1.470%
5	2.132	376	386	397	rBV	457934	639066	31.82%	4.128%
6	3.318	753	755	759	rVB3	604	317	0.002%	0.0002%
7	3.418	782	786	789	rBV2	633	529	0.003%	0.0003%
8	3.752	887	890	894	rBV3	544	452	0.002%	0.0003%
9	3.791	900	902	905	rVB4	581	291	0.001%	0.0002%
10	3.897	930	935	938	rBV4	574	628	0.003%	0.0004%
11	3.961	939	955	1000	rVV	152157	451381	22.48%	2.915%
12	4.408	1075	1094	1118	rBV	340205	803525	40.01%	5.190%
13	4.553	1136	1139	1141	rBV3	462	354	0.002%	0.0002%
14	4.591	1148	1151	1153	rVB3	649	358	0.002%	0.0002%
15	4.607	1154	1156	1160	rVB3	392	235	0.001%	0.0002%
16	4.652	1167	1170	1177	rVB3	427	573	0.003%	0.0004%
17	4.688	1178	1181	1183	rBV2	727	390	0.002%	0.0003%
18	4.717	1183	1190	1191	rBV4	482	531	0.003%	0.0003%
19	4.810	1216	1219	1220	rBV	506	265	0.001%	0.0002%
20	4.871	1235	1238	1241	rBV3	624	488	0.002%	0.0003%
21	4.910	1245	1250	1253	rVB	293	246	0.001%	0.0002%
22	4.926	1253	1255	1259	rBV	322	251	0.001%	0.0002%
23	4.955	1262	1264	1267	rBV3	400	289	0.001%	0.0002%
24	5.099	1291	1309	1355	rBV2	845533	2008163	100.00%	12.970%
25	5.337	1380	1383	1387	rBV3	470	300	0.001%	0.0002%
26	5.450	1410	1418	1420	rBV5	1264	1464	0.007%	0.0009%
27	5.463	1420	1422	1426	rVB2	633	302	0.002%	0.0002%
28	5.517	1437	1439	1445	rVB3	434	450	0.002%	0.0003%
29	5.546	1445	1448	1453	rVB3	372	303	0.002%	0.0002%
30	5.572	1453	1456	1459	rBV2	553	345	0.002%	0.0002%
31	5.672	1471	1487	1514	rBV	602620	1192595	59.39%	7.703%
32	5.951	1564	1574	1588	rVB3	16812	37439	1.86%	0.242%
33	6.054	1602	1606	1612	rBV4	964	1294	0.006%	0.0008%
34	6.125	1613	1628	1654	rVV	463024	935353	46.58%	6.041%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007352.D
 Acq On : 05 Sep 2018 01:45
 Operator : SY/MD
 Sample : J4695-07
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.299	1679	1682	1683	rBV	480	268	0.01%	0.002%
36	6.324	1688	1690	1693	rVB2	627	295	0.01%	0.002%
37	6.469	1732	1735	1738	rVB4	458	333	0.02%	0.002%
38	6.537	1753	1756	1758	rBV2	626	425	0.02%	0.003%
39	6.562	1762	1764	1769	rVB3	918	641	0.03%	0.004%
40	6.591	1769	1773	1775	rBV3	749	572	0.03%	0.004%
41	6.604	1775	1777	1781	rVB3	540	361	0.02%	0.002%
42	6.649	1785	1791	1794	rBV4	1235	1274	0.06%	0.008%
43	6.726	1807	1815	1821	rBV5	3015	4862	0.24%	0.031%
44	6.774	1827	1830	1835	rBV3	608	533	0.03%	0.003%
45	6.816	1840	1843	1846	rBV2	358	326	0.02%	0.002%
46	6.910	1869	1872	1874	rBV	466	299	0.01%	0.002%
47	6.922	1874	1876	1881	rVB2	393	329	0.02%	0.002%
48	6.987	1892	1896	1898	rBV4	395	330	0.02%	0.002%
49	7.035	1898	1911	1933	rBV	213656	384525	19.15%	2.484%
50	7.167	1949	1952	1954	rBV3	692	507	0.03%	0.003%
51	7.237	1970	1974	1977	rBV4	561	534	0.03%	0.003%
52	7.366	2000	2014	2036	rBV	828630	1452592	72.33%	9.382%
53	7.668	2097	2108	2128	rBV	157112	265738	13.23%	1.716%
54	8.022	2212	2218	2229	rVB6	8781	14804	0.74%	0.096%
55	8.144	2243	2256	2286	rBV	510455	936846	46.65%	6.051%
56	8.495	2363	2365	2371	rVB5	801	577	0.03%	0.004%
57	8.646	2404	2412	2413	rBV6	461	582	0.03%	0.004%
58	8.694	2422	2427	2429	rBV2	584	544	0.03%	0.004%
59	8.762	2444	2448	2450	rBV	358	302	0.02%	0.002%
60	8.794	2455	2458	2462	rVB3	794	702	0.03%	0.005%
61	8.823	2462	2467	2470	rBV	528	586	0.03%	0.004%
62	8.900	2477	2491	2520	rBV	874733	1417917	70.61%	9.158%
63	9.157	2568	2571	2574	rBV2	369	261	0.01%	0.002%
64	9.176	2574	2577	2578	rBV	754	489	0.02%	0.003%
65	9.260	2589	2603	2605	rBV4	4090	6722	0.33%	0.043%
66	9.491	2671	2675	2678	rVV3	565	508	0.03%	0.003%
67	9.604	2708	2710	2714	rVV	646	317	0.02%	0.002%
68	9.626	2714	2717	2720	rVV2	415	253	0.01%	0.002%
69	9.704	2738	2741	2746	rBV4	472	448	0.02%	0.003%
70	9.729	2746	2749	2752	rVB2	575	386	0.02%	0.002%
71	9.758	2754	2758	2761	rBV2	433	333	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007352.D
 Acq On : 05 Sep 2018 01:45
 Operator : SY/MD
 Sample : J4695-07
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE50

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	9.823	2775	2778	2780	rBV	575	338	0.02%	0.002%
73	9.868	2790	2792	2797	rVB	610	389	0.02%	0.003%
74	9.909	2802	2805	2807	rBV3	399	263	0.01%	0.002%
75	9.954	2812	2819	2823	rVB3	413	547	0.03%	0.004%
76	9.977	2823	2826	2829	rBV2	401	362	0.02%	0.002%
77	10.022	2836	2840	2847	rBV3	286	347	0.02%	0.002%
78	10.070	2847	2855	2861	rBV4	1776	2969	0.15%	0.019%
79	10.266	2899	2916	2947	rBV	604858	955632	47.59%	6.172%
80	10.427	2957	2966	2977	rBV4	3138	5452	0.27%	0.035%
81	10.716	3052	3056	3057	rBV	660	453	0.02%	0.003%
82	10.810	3083	3085	3089	rVB2	463	313	0.02%	0.002%
83	10.829	3089	3091	3095	rBV3	284	270	0.01%	0.002%
84	10.948	3124	3128	3130	rBV2	473	349	0.02%	0.002%
85	10.964	3130	3133	3140	rVB4	579	647	0.03%	0.004%
86	10.996	3140	3143	3146	rBV2	454	350	0.02%	0.002%
87	11.099	3173	3175	3181	rVB3	468	434	0.02%	0.003%
88	11.154	3189	3192	3197	rBV2	420	434	0.02%	0.003%
89	11.186	3197	3202	3206	rVB3	442	388	0.02%	0.003%
90	11.231	3212	3216	3224	rBV5	794	1002	0.05%	0.006%
91	11.298	3224	3237	3264	rBV	659775	1064794	53.02%	6.877%
92	11.475	3289	3292	3295	rBV3	561	419	0.02%	0.003%
93	11.678	3341	3355	3377	rBV	737964	1186766	59.10%	7.665%
94	11.909	3425	3427	3429	rBV	422	233	0.01%	0.002%
95	11.941	3433	3437	3439	rBV2	711	578	0.03%	0.004%
96	12.080	3477	3480	3483	rVB4	503	300	0.01%	0.002%
97	12.440	3589	3592	3595	rBV2	473	449	0.02%	0.003%
98	12.945	3747	3749	3752	rVB3	868	461	0.02%	0.003%
99	13.803	4013	4016	4019	rBV4	823	564	0.03%	0.004%
100	14.215	4142	4144	4147	rBV3	863	455	0.02%	0.003%


Sum of corrected areas: 15482861

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090418\
Data File : VV007352.D
Acq On : 05 Sep 2018 01:45
Operator : SY/MD
Sample : J4695-07
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

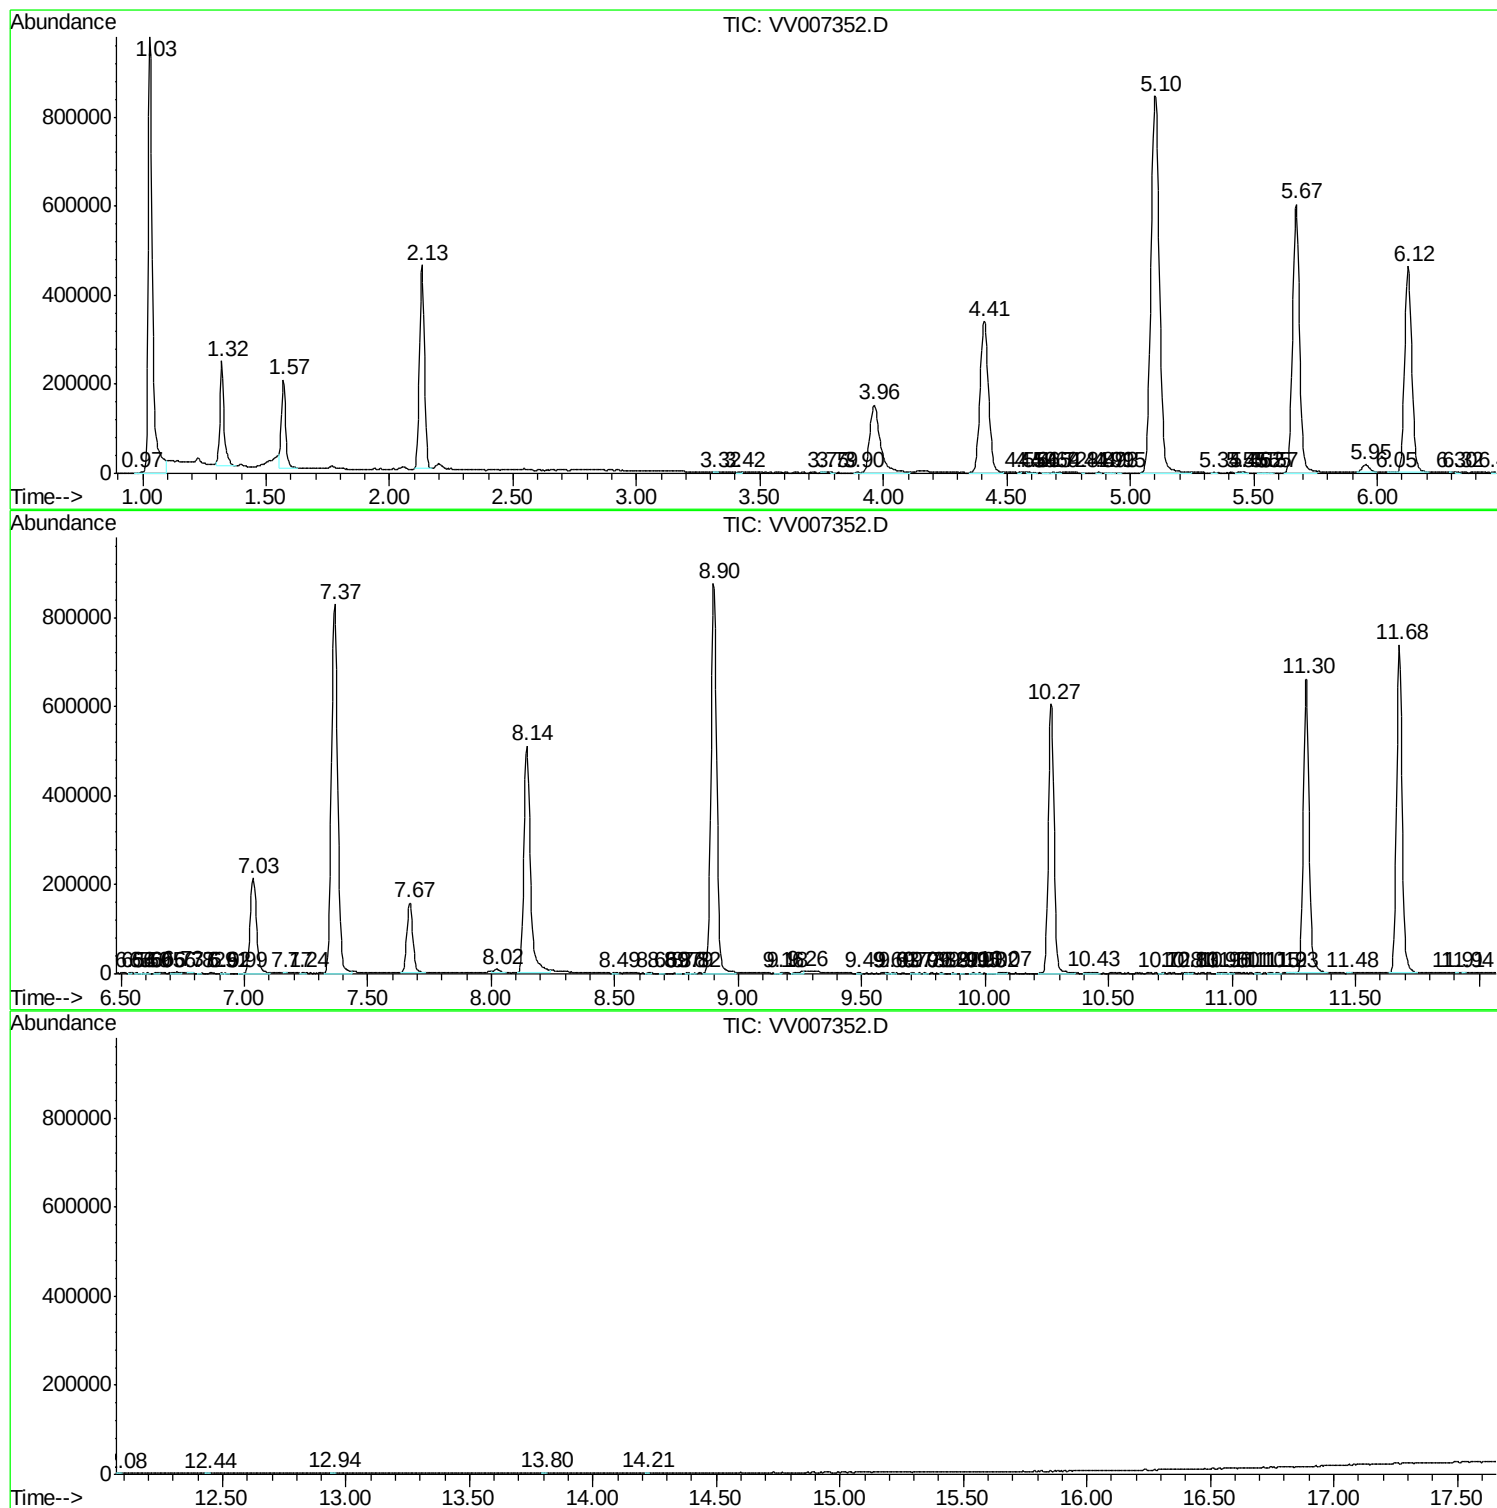

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007352.D
Acq On : 05 Sep 2018 01:45
Operator : SY/MD
Sample : J4695-07
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007352.D
Acq On : 05 Sep 2018 01:45
Operator : SY/MD
Sample : J4695-07
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE50

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc