

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007353.D
 Acq On : 05 Sep 2018 02:10
 Operator : SY/MD
 Sample : J4695-08
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.948	11	18	22	rBV3	612	805	0.002%	0.0004%
2	1.029	29	43	67	rBV	2642991	3221966	100.00%	17.989%
3	1.257	108	114	124	rVB	119018	135287	4.20%	0.755%
4	1.321	127	134	151	rVB	238358	283349	8.79%	1.582%
5	1.572	206	212	226	rVB	198661	234387	7.27%	1.309%
6	2.131	376	386	397	rBV	445537	621109	19.28%	3.468%
7	2.202	400	408	418	rVV	56339	93443	2.90%	0.522%
8	2.263	419	427	437	rVB	106634	155231	4.82%	0.867%
9	3.421	784	787	792	rBV5	542	542	0.002%	0.0003%
10	3.530	816	821	824	rBV3	497	500	0.002%	0.0003%
11	3.707	873	876	881	rBV3	352	260	0.001%	0.0001%
12	3.758	885	892	894	rBV5	1394	1752	0.005%	0.0010%
13	3.848	918	920	922	rBV	449	280	0.001%	0.0002%
14	3.881	928	930	934	rBV3	347	316	0.001%	0.0002%
15	3.961	939	955	977	rBV	149747	425757	13.21%	2.377%
16	4.244	1041	1043	1050	rVB5	815	608	0.002%	0.0003%
17	4.279	1052	1054	1057	rVV3	523	295	0.001%	0.0002%
18	4.308	1061	1063	1068	rVB3	913	770	0.002%	0.0004%
19	4.408	1075	1094	1119	rBV	341633	827533	25.68%	4.620%
20	4.572	1143	1145	1148	rVB3	565	319	0.001%	0.0002%
21	4.591	1148	1151	1154	rBV3	357	314	0.001%	0.0002%
22	4.662	1167	1173	1184	rBV7	1051	2063	0.006%	0.0012%
23	4.729	1184	1194	1205	rBV7	2880	6725	0.021%	0.0038%
24	4.929	1252	1256	1260	rBV2	569	532	0.002%	0.0003%
25	4.967	1263	1268	1276	rVB3	647	738	0.002%	0.0004%
26	5.102	1291	1310	1322	rBV2	835758	2001134	62.11%	11.173%
27	5.382	1390	1397	1411	rVB6	2878	6394	0.020%	0.0036%
28	5.434	1411	1413	1414	rBV2	544	295	0.001%	0.0002%
29	5.517	1432	1439	1440	rBV5	539	546	0.002%	0.0003%
30	5.559	1448	1452	1455	rBV3	1014	910	0.003%	0.0005%
31	5.671	1472	1487	1515	rBV	582968	1163013	36.10%	6.493%
32	5.951	1565	1574	1588	rVB5	10912	22605	0.070%	0.00126%
33	6.044	1601	1603	1606	rBV2	703	470	0.001%	0.0003%
34	6.125	1613	1628	1656	rBV	467111	936615	29.07%	5.229%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007353.D
 Acq On : 05 Sep 2018 02:10
 Operator : SY/MD
 Sample : J4695-08
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.353	1690	1699	1704	rVV8	1648	3005	0.09%	0.017%
36	6.453	1728	1730	1733	rBV2	332	234	0.01%	0.001%
37	6.498	1742	1744	1746	rBV	454	247	0.01%	0.001%
38	6.562	1760	1764	1767	rBV3	501	486	0.02%	0.003%
39	6.604	1771	1777	1780	rVB4	695	821	0.03%	0.005%
40	6.655	1780	1793	1796	rBV4	1419	2681	0.08%	0.015%
41	6.729	1807	1816	1825	rBV5	2611	4830	0.15%	0.027%
42	6.839	1845	1850	1856	rBV4	678	906	0.03%	0.005%
43	6.868	1856	1859	1864	rVB4	563	437	0.01%	0.002%
44	6.893	1864	1867	1870	rBV4	421	358	0.01%	0.002%
45	6.938	1876	1881	1882	rBV	447	342	0.01%	0.002%
46	7.035	1898	1911	1938	rBV	214509	384772	11.94%	2.148%
47	7.186	1956	1958	1960	rVB3	776	237	0.01%	0.001%
48	7.298	1984	1993	2000	rBV3	4503	8520	0.26%	0.048%
49	7.366	2001	2014	2033	rBV	817950	1421422	44.12%	7.936%
50	7.668	2094	2108	2125	rBV	159108	270040	8.38%	1.508%
51	7.758	2133	2136	2140	rBV4	967	686	0.02%	0.004%
52	7.983	2202	2206	2210	rBV4	2937	3441	0.11%	0.019%
53	8.022	2211	2218	2228	rVB3	15124	24234	0.75%	0.135%
54	8.144	2243	2256	2282	rBV	501517	921362	28.60%	5.144%
55	8.559	2381	2385	2389	rVB5	786	806	0.03%	0.005%
56	8.581	2389	2392	2396	rBV3	703	690	0.02%	0.004%
57	8.610	2399	2401	2404	rVB2	524	285	0.01%	0.002%
58	8.630	2404	2407	2409	rBV3	514	259	0.01%	0.001%
59	8.723	2434	2436	2439	rBV2	555	306	0.01%	0.002%
60	8.806	2459	2462	2464	rBV2	419	241	0.01%	0.001%
61	8.832	2465	2470	2474	rVB4	612	608	0.02%	0.003%
62	8.900	2477	2491	2515	rBV	863495	1398847	43.42%	7.810%
63	9.276	2590	2608	2612	rBV8	6216	14918	0.46%	0.083%
64	9.430	2654	2656	2661	rVB4	1139	948	0.03%	0.005%
65	9.494	2670	2676	2678	rVB4	467	415	0.01%	0.002%
66	9.591	2703	2706	2707	rBV2	669	336	0.01%	0.002%
67	9.649	2716	2724	2732	rVV5	3870	5960	0.18%	0.033%
68	9.681	2732	2734	2737	rVB3	951	557	0.02%	0.003%
69	9.758	2750	2758	2766	rVB5	2577	3992	0.12%	0.022%
70	9.816	2771	2776	2778	rBV3	405	328	0.01%	0.002%
71	9.832	2778	2781	2783	rBV2	509	282	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007353.D
 Acq On : 05 Sep 2018 02:10
 Operator : SY/MD
 Sample : J4695-08
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE51

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	9.957	2815	2820	2821	rBV2	317	278	0.01%	0.002%
73	10.067	2853	2854	2863	rVB2	553	447	0.01%	0.002%
74	10.112	2866	2868	2874	rBV3	503	371	0.01%	0.002%
75	10.266	2903	2916	2933	rBV	609594	959678	29.79%	5.358%
76	10.404	2957	2959	2960	rBV2	730	344	0.01%	0.002%
77	10.427	2961	2966	2976	rVB3	3972	5194	0.16%	0.029%
78	10.584	3013	3015	3019	rVB2	511	374	0.01%	0.002%
79	10.806	3081	3084	3086	rVB	623	405	0.01%	0.002%
80	10.909	3105	3116	3130	rBV4	5746	12822	0.40%	0.072%
81	10.990	3135	3141	3144	rBV7	2139	2308	0.07%	0.013%
82	11.089	3169	3172	3178	rVB3	814	828	0.03%	0.005%
83	11.150	3182	3191	3203	rBV9	5660	12366	0.38%	0.069%
84	11.228	3212	3215	3217	rBV4	746	492	0.02%	0.003%
85	11.298	3225	3237	3267	rBV	662317	1082155	33.59%	6.042%
86	11.482	3292	3294	3296	rBV3	927	476	0.01%	0.003%
87	11.517	3303	3305	3311	rVB4	1046	741	0.02%	0.004%
88	11.543	3311	3313	3314	rBV	526	239	0.01%	0.001%
89	11.578	3321	3324	3326	rBV4	850	627	0.02%	0.004%
90	11.678	3343	3355	3383	rVB	747717	1198758	37.21%	6.693%
91	11.838	3403	3405	3409	rVB4	737	368	0.01%	0.002%
92	11.977	3443	3448	3450	rBV2	750	708	0.02%	0.004%
93	12.076	3476	3479	3481	rBV4	503	350	0.01%	0.002%
94	12.089	3481	3483	3488	rVB5	972	820	0.03%	0.005%
95	12.186	3509	3513	3516	rBV3	546	485	0.02%	0.003%
96	12.292	3543	3546	3548	rBV3	1058	711	0.02%	0.004%
97	12.366	3567	3569	3573	rBV2	508	261	0.01%	0.001%
98	12.433	3587	3590	3591	rBV2	604	366	0.01%	0.002%
99	12.700	3667	3673	3680	rBV6	953	1649	0.05%	0.009%
100	13.211	3829	3832	3836	rBV3	741	708	0.02%	0.004%


Sum of corrected areas: 17911031

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090418\
Data File : VV007353.D
Acq On : 05 Sep 2018 02:10
Operator : SY/MD
Sample : J4695-08
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

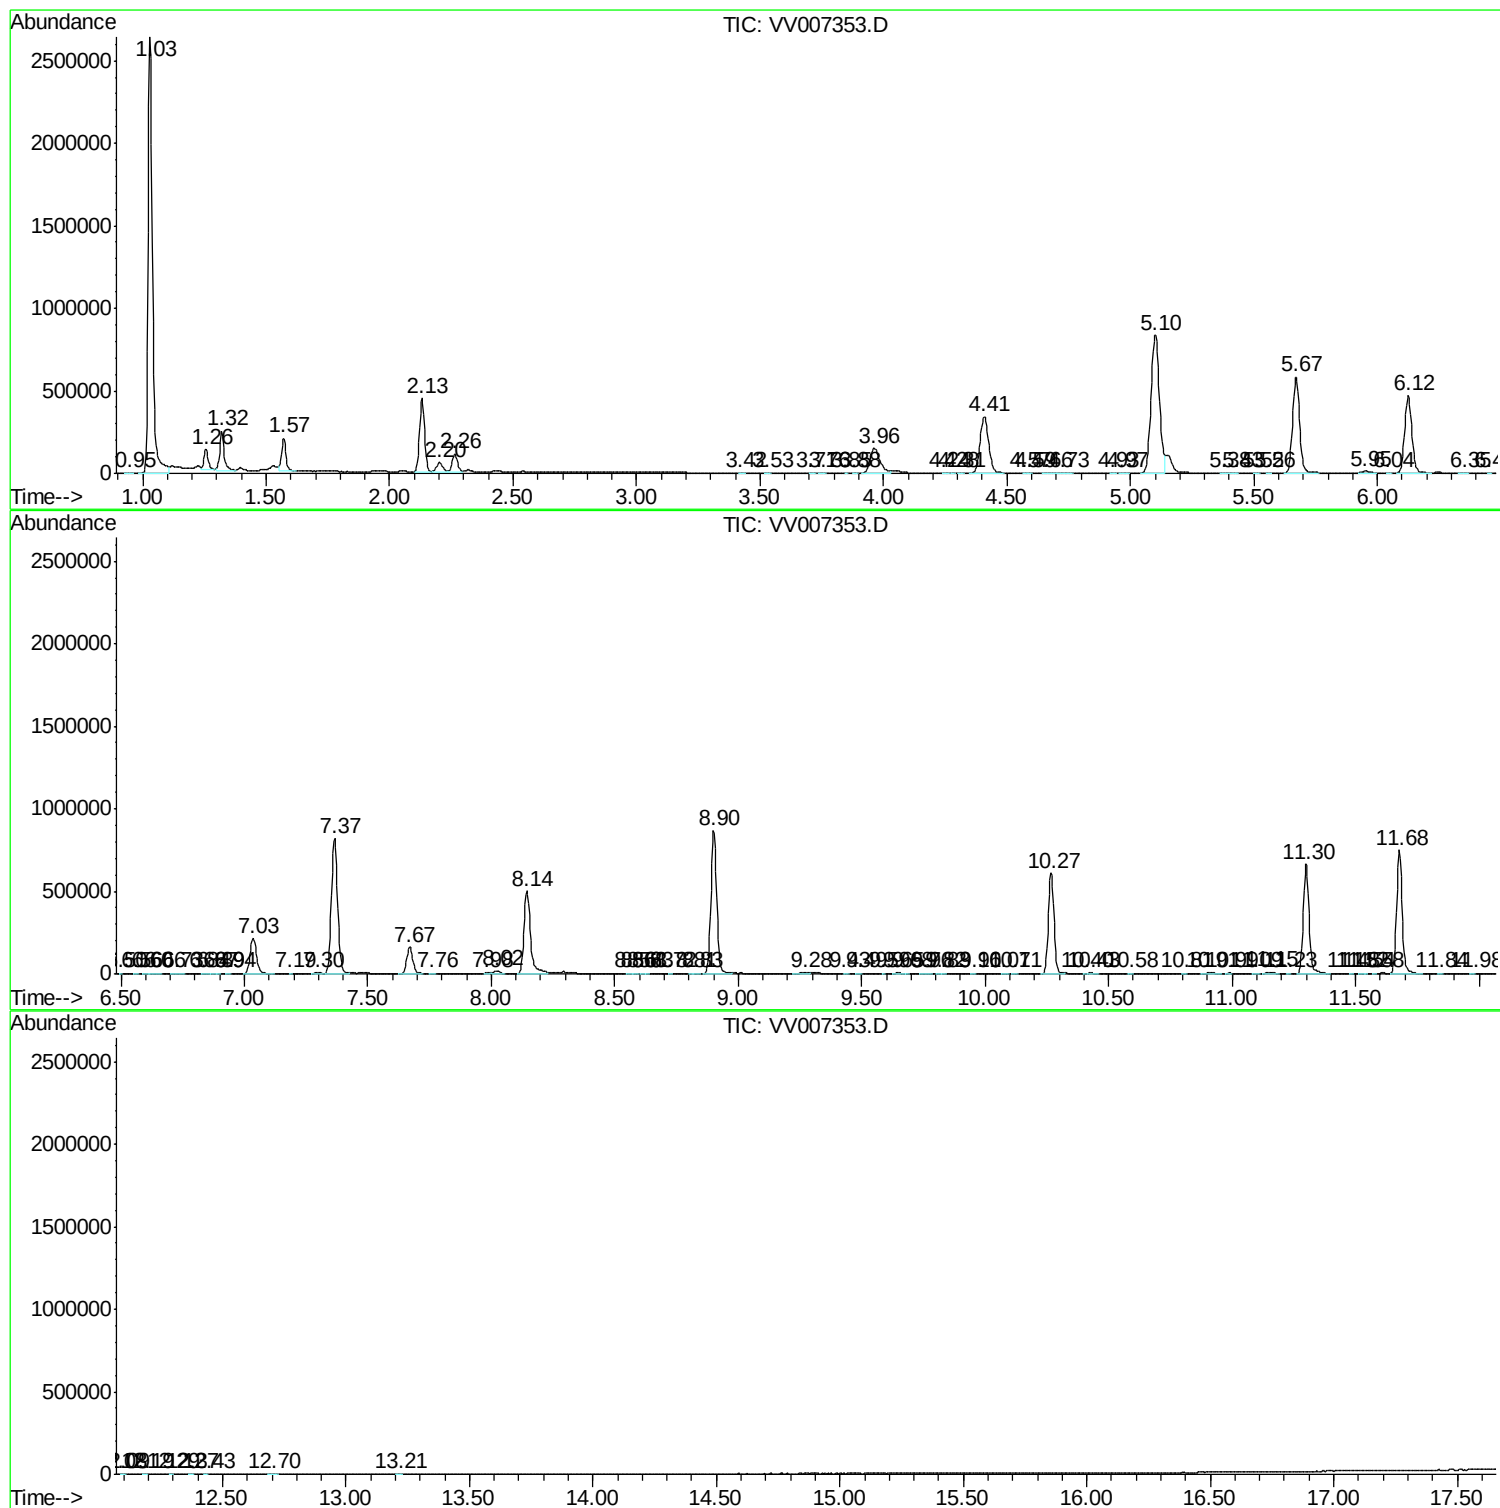

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007353.D
Acq On : 05 Sep 2018 02:10
Operator : SY/MD
Sample : J4695-08
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007353.D
Acq On : 05 Sep 2018 02:10
Operator : SY/MD
Sample : J4695-08
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE51

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc