

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007354.D
 Acq On : 05 Sep 2018 02:35
 Operator : SY/MD
 Sample : J4695-11
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.945	12	17	21	rBV3	623	568	0.003%	0.0003%
2	1.028	31	43	67	rBV	1314512	1622216	79.43%	9.946%
3	1.321	127	134	153	rVB	239613	285255	13.97%	1.749%
4	1.572	206	212	224	rVB	194554	224042	10.97%	1.374%
5	2.131	376	386	398	rBV	465352	651414	31.89%	3.994%
6	2.202	400	408	423	rVB	54552	92837	4.55%	0.569%
7	3.376	771	773	777	rBV2	662	356	0.002%	0.0002%
8	3.536	820	823	827	rVV	508	284	0.001%	0.0002%
9	3.639	853	855	859	rVB2	400	247	0.001%	0.0002%
10	3.671	862	865	868	rBV	526	366	0.002%	0.0002%
11	3.768	887	895	897	rVV3	655	659	0.003%	0.0004%
12	3.784	897	900	904	rVB	433	317	0.002%	0.0002%
13	3.835	913	916	920	rBV3	381	362	0.002%	0.0002%
14	3.877	925	929	933	rBV3	543	480	0.002%	0.0003%
15	3.961	937	955	997	rBV	154139	464596	22.75%	2.849%
16	4.244	1041	1043	1048	rVB3	828	517	0.003%	0.0003%
17	4.321	1066	1067	1071	rVB	622	275	0.001%	0.0002%
18	4.408	1074	1094	1121	rBV	345802	833957	40.83%	5.113%
19	4.597	1150	1153	1159	rVB3	643	612	0.003%	0.0004%
20	4.726	1182	1193	1207	rBV8	6192	14316	0.70%	0.0088%
21	4.778	1207	1209	1214	rVB3	720	425	0.002%	0.0003%
22	4.816	1218	1221	1224	rVV3	426	284	0.001%	0.0002%
23	4.887	1238	1243	1246	rBV2	490	506	0.002%	0.0003%
24	4.903	1246	1248	1252	rVB	390	230	0.001%	0.0001%
25	4.922	1252	1254	1260	rBV3	357	298	0.001%	0.0002%
26	4.967	1265	1268	1270	rBV2	387	226	0.001%	0.0001%
27	5.025	1284	1286	1289	rVB	514	259	0.001%	0.0002%
28	5.099	1289	1309	1334	rBV2	861009	2042390	100.00%	12.523%
29	5.263	1356	1360	1362	rBV3	889	545	0.003%	0.0003%
30	5.305	1370	1373	1377	rVB4	346	272	0.001%	0.0002%
31	5.456	1416	1420	1423	rVV4	515	385	0.002%	0.0002%
32	5.472	1423	1425	1431	rVB3	615	570	0.003%	0.0003%
33	5.511	1431	1437	1439	rBV3	565	544	0.003%	0.0003%
34	5.549	1447	1449	1453	rVB2	472	266	0.001%	0.0002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007354.D
 Acq On : 05 Sep 2018 02:35
 Operator : SY/MD
 Sample : J4695-11
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	5.572	1453	1456	1459	rBV2	649	458	0.02%	0.003%
36	5.671	1471	1487	1506	rBV	606918	1196394	58.58%	7.336%
37	5.951	1564	1574	1591	rVB5	14914	30706	1.50%	0.188%
38	6.125	1612	1628	1657	rBV	475868	962873	47.14%	5.904%
39	6.314	1686	1687	1692	rVB2	673	371	0.02%	0.002%
40	6.414	1715	1718	1722	rBV3	402	342	0.02%	0.002%
41	6.440	1722	1726	1732	rBV4	442	500	0.02%	0.003%
42	6.485	1738	1740	1743	rBV	326	245	0.01%	0.002%
43	6.588	1770	1772	1775	rVB	470	301	0.01%	0.002%
44	6.658	1785	1794	1802	rBV7	1473	2854	0.14%	0.017%
45	6.726	1807	1815	1826	rBV3	2687	5518	0.27%	0.034%
46	6.797	1834	1837	1840	rBV3	544	381	0.02%	0.002%
47	6.816	1840	1843	1846	rVV3	408	279	0.01%	0.002%
48	6.867	1854	1859	1864	rBV3	681	550	0.03%	0.003%
49	7.035	1897	1911	1927	rBV	214388	386236	18.91%	2.368%
50	7.279	1983	1987	1991	rVB5	557	513	0.03%	0.003%
51	7.305	1991	1995	2000	rBV4	383	485	0.02%	0.003%
52	7.366	2000	2014	2032	rBV	848889	1479534	72.44%	9.072%
53	7.668	2096	2108	2124	rBV	157077	270948	13.27%	1.661%
54	7.835	2157	2160	2162	rBV2	674	509	0.02%	0.003%
55	7.986	2202	2207	2214	rBV3	2250	3482	0.17%	0.021%
56	8.144	2243	2256	2291	rBV	501949	929980	45.53%	5.702%
57	8.498	2363	2366	2369	rBB3	586	354	0.02%	0.002%
58	8.520	2369	2373	2375	rBV3	539	374	0.02%	0.002%
59	8.646	2409	2412	2413	rBV2	425	265	0.01%	0.002%
60	8.781	2451	2454	2458	rVV4	432	329	0.02%	0.002%
61	8.900	2478	2491	2516	rBV	873431	1439896	70.50%	8.829%
62	9.189	2577	2581	2588	rVB4	1279	1380	0.07%	0.008%
63	9.279	2588	2609	2635	rBV3	9954	49266	2.41%	0.302%
64	9.565	2693	2698	2702	rBV3	361	375	0.02%	0.002%
65	9.588	2702	2705	2708	rBV4	619	460	0.02%	0.003%
66	9.652	2723	2725	2731	rVB3	615	441	0.02%	0.003%
67	9.681	2731	2734	2737	rBV3	588	377	0.02%	0.002%
68	9.739	2748	2752	2754	rBV3	398	264	0.01%	0.002%
69	9.777	2760	2764	2768	rBV4	365	346	0.02%	0.002%
70	9.813	2772	2775	2779	rBV3	363	266	0.01%	0.002%
71	9.867	2786	2792	2797	rBV4	515	738	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007354.D
 Acq On : 05 Sep 2018 02:35
 Operator : SY/MD
 Sample : J4695-11
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEE53

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	9.980	2824	2827	2831	rVV2	989	759	0.04%	0.005%
73	10.006	2832	2835	2840	rVV2	485	406	0.02%	0.002%
74	10.089	2858	2861	2866	rBV5	451	431	0.02%	0.003%
75	10.121	2867	2871	2873	rBV2	381	246	0.01%	0.002%
76	10.189	2887	2892	2895	rBV2	709	570	0.03%	0.003%
77	10.266	2904	2916	2932	rBV	617322	973776	47.68%	5.971%
78	10.388	2951	2954	2957	rVB3	591	393	0.02%	0.002%
79	10.427	2957	2966	2976	rVV2	5251	8693	0.43%	0.053%
80	10.568	3006	3010	3013	rBV3	559	383	0.02%	0.002%
81	10.588	3013	3016	3019	rBV2	326	262	0.01%	0.002%
82	10.800	3076	3082	3086	rBV3	647	695	0.03%	0.004%
83	10.829	3086	3091	3096	rVB3	731	871	0.04%	0.005%
84	10.903	3110	3114	3117	rBV3	647	556	0.03%	0.003%
85	11.105	3174	3177	3180	rBV4	358	321	0.02%	0.002%
86	11.163	3193	3195	3199	rVB3	466	246	0.01%	0.002%
87	11.237	3213	3218	3225	rVB5	848	916	0.04%	0.006%
88	11.301	3225	3238	3262	rBV	676670	1090190	53.38%	6.684%
89	11.507	3299	3302	3306	rVB2	726	540	0.03%	0.003%
90	11.526	3306	3308	3310	rBV2	536	257	0.01%	0.002%
91	11.613	3333	3335	3340	rVB4	695	481	0.02%	0.003%
92	11.678	3342	3355	3380	rBV	745171	1215374	59.51%	7.452%
93	12.137	3495	3498	3500	rBV3	531	351	0.02%	0.002%
94	12.182	3510	3512	3514	rVB	526	219	0.01%	0.001%
95	12.266	3536	3538	3540	rBV3	494	293	0.01%	0.002%
96	13.012	3766	3770	3774	rBV3	865	652	0.03%	0.004%
97	13.314	3861	3864	3866	rBV2	655	508	0.02%	0.003%
98	13.346	3872	3874	3876	rBV2	875	405	0.02%	0.002%
99	13.555	3937	3939	3942	rBV2	1308	778	0.04%	0.005%
100	13.706	3983	3986	3989	rBV3	805	554	0.03%	0.003%


Sum of corrected areas: 16309592

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090418\
Data File : VV007354.D
Acq On : 05 Sep 2018 02:35
Operator : SY/MD
Sample : J4695-11
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE53

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

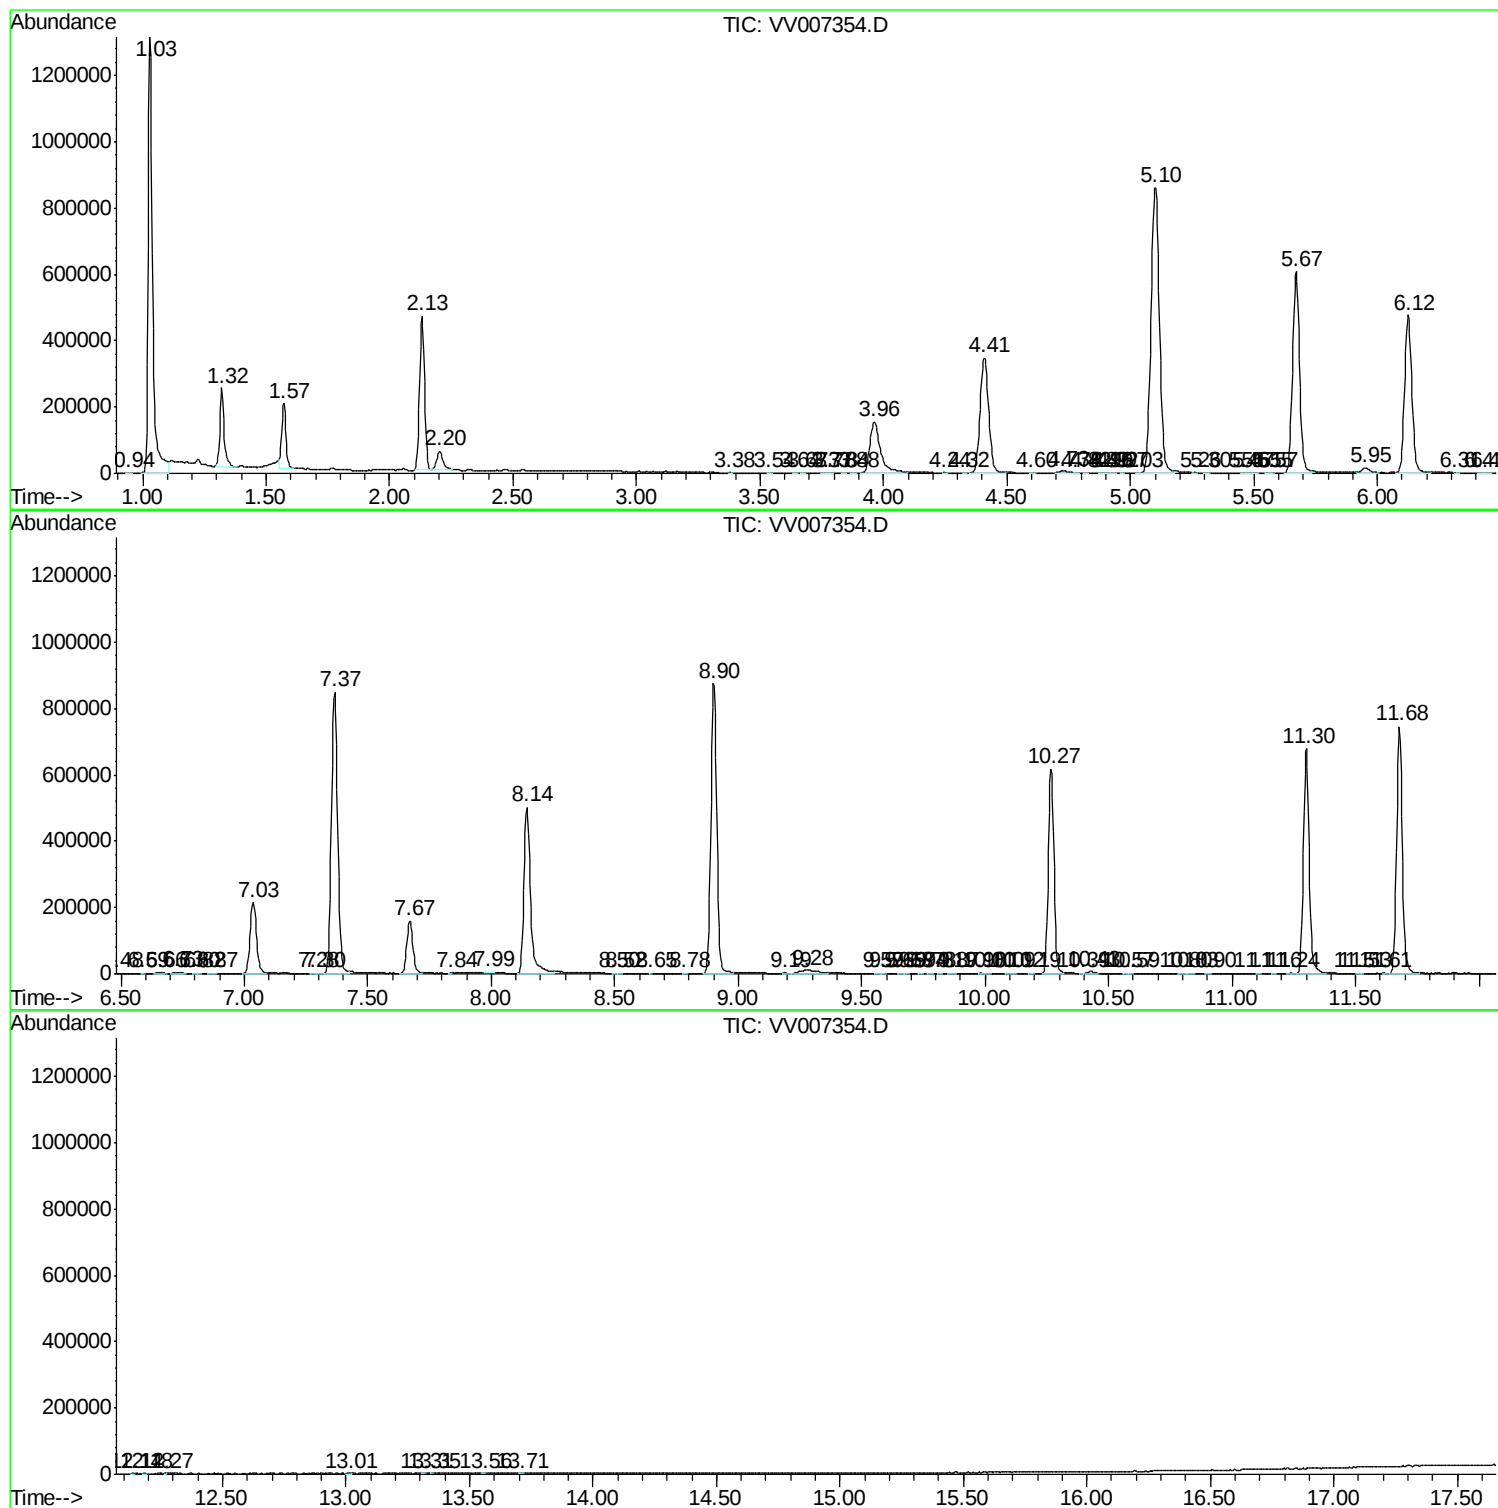

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007354.D
Acq On : 05 Sep 2018 02:35
Operator : SY/MD
Sample : J4695-11
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE53

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007354.D
Acq On : 05 Sep 2018 02:35
Operator : SY/MD
Sample : J4695-11
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEE53

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc