

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007365.D
 Acq On : 05 Sep 2018 07:06
 Operator : SY/MD
 Sample : J4695-20
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.945	13	17	22	rVB2	540	584	0.03%	0.004%
2	1.032	30	44	66	rBV	667307	850237	41.61%	5.168%
3	1.321	127	134	153	rVB	237494	276432	13.53%	1.680%
4	1.575	207	213	226	rVB	205589	236752	11.59%	1.439%
5	2.131	376	386	399	rBV	455568	652855	31.95%	3.968%
6	3.292	745	747	750	rBV2	686	405	0.02%	0.002%
7	3.411	780	784	786	rBV3	780	471	0.02%	0.003%
8	3.594	838	841	844	rBV2	545	347	0.02%	0.002%
9	3.964	937	956	1004	rBV	155085	484600	23.72%	2.946%
10	4.408	1076	1094	1121	rBV	345777	826581	40.45%	5.024%
11	4.527	1129	1131	1136	rVB4	464	307	0.02%	0.002%
12	4.559	1138	1141	1146	rVV4	650	553	0.03%	0.003%
13	4.598	1150	1153	1156	rBV2	544	382	0.02%	0.002%
14	4.671	1172	1176	1179	rBV3	439	334	0.02%	0.002%
15	4.733	1182	1195	1206	rBV10	4077	10044	0.49%	0.061%
16	4.839	1224	1228	1232	rBV4	485	521	0.03%	0.003%
17	4.890	1240	1244	1246	rBV3	303	296	0.01%	0.002%
18	4.903	1246	1248	1251	rVB2	566	260	0.01%	0.002%
19	4.919	1251	1253	1256	rVB2	511	250	0.01%	0.002%
20	4.942	1256	1260	1263	rBV3	430	463	0.02%	0.003%
21	5.102	1290	1310	1333	rBV2	858480	2043243	100.00%	12.420%
22	5.379	1393	1396	1399	rBV4	562	370	0.02%	0.002%
23	5.433	1409	1413	1414	rBV3	567	253	0.01%	0.002%
24	5.459	1414	1421	1424	rVB4	938	1107	0.05%	0.007%
25	5.511	1433	1437	1439	rBV2	455	360	0.02%	0.002%
26	5.533	1442	1444	1448	rVB2	521	287	0.01%	0.002%
27	5.607	1463	1467	1468	rBV3	497	334	0.02%	0.002%
28	5.671	1471	1487	1510	rBV	667958	1326284	64.91%	8.062%
29	5.864	1543	1547	1551	rBV5	875	996	0.05%	0.006%
30	5.964	1564	1578	1594	rBV4	148208	302988	14.83%	1.842%
31	6.125	1613	1628	1657	rBV	476161	966955	47.32%	5.878%
32	6.472	1734	1736	1741	rVB3	619	486	0.02%	0.003%
33	6.507	1744	1747	1752	rBV4	374	307	0.02%	0.002%
34	6.533	1752	1755	1759	rVB4	630	391	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007365.D
 Acq On : 05 Sep 2018 07:06
 Operator : SY/MD
 Sample : J4695-20
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.552	1759	1761	1764	rVB2	440	263	0.01%	0.002%
36	6.575	1764	1768	1772	rBV4	889	746	0.04%	0.005%
37	6.597	1772	1775	1778	rBV2	422	265	0.01%	0.002%
38	6.642	1782	1789	1791	rBV5	1361	1388	0.07%	0.008%
39	6.694	1803	1805	1808	rBV	652	393	0.02%	0.002%
40	6.729	1808	1816	1826	rVV3	1994	4132	0.20%	0.025%
41	6.768	1826	1828	1834	rVV2	821	667	0.03%	0.004%
42	6.848	1851	1853	1862	rVB4	559	580	0.03%	0.004%
43	6.890	1862	1866	1867	rBV2	336	252	0.01%	0.002%
44	6.961	1886	1888	1892	rBV3	460	362	0.02%	0.002%
45	7.035	1898	1911	1934	rBV	211376	383198	18.75%	2.329%
46	7.366	1999	2014	2043	rBV	859167	1496204	73.23%	9.095%
47	7.668	2096	2108	2134	rBV	157299	268528	13.14%	1.632%
48	7.803	2148	2150	2151	rBV	634	270	0.01%	0.002%
49	8.022	2205	2218	2233	rVB	211121	358080	17.53%	2.177%
50	8.102	2240	2243	2244	rBV2	669	419	0.02%	0.003%
51	8.144	2244	2256	2288	rVV2	490538	923319	45.19%	5.613%
52	8.501	2363	2367	2374	rBV4	563	688	0.03%	0.004%
53	8.533	2374	2377	2381	rVB3	455	320	0.02%	0.002%
54	8.568	2385	2388	2394	rBV5	464	402	0.02%	0.002%
55	8.629	2404	2407	2410	rBV3	331	306	0.01%	0.002%
56	8.829	2463	2469	2472	rBV4	674	689	0.03%	0.004%
57	8.845	2472	2474	2477	rBV2	454	256	0.01%	0.002%
58	8.900	2477	2491	2516	rBV	974342	1590383	77.84%	9.667%
59	9.163	2571	2573	2576	rBV	424	248	0.01%	0.002%
60	9.186	2576	2580	2583	rBV2	791	640	0.03%	0.004%
61	9.282	2589	2610	2636	rBV6	10621	48321	2.36%	0.294%
62	9.514	2680	2682	2685	rVB2	530	279	0.01%	0.002%
63	9.581	2700	2703	2705	rBV	717	542	0.03%	0.003%
64	9.684	2731	2735	2737	rBV3	459	369	0.02%	0.002%
65	9.842	2778	2784	2789	rBV2	266	370	0.02%	0.002%
66	9.893	2797	2800	2802	rBV3	424	308	0.02%	0.002%
67	9.925	2807	2810	2813	rBV2	427	270	0.01%	0.002%
68	9.970	2821	2824	2830	rBV3	532	415	0.02%	0.003%
69	10.099	2859	2864	2866	rBV2	299	279	0.01%	0.002%
70	10.118	2867	2870	2873	rVB2	534	352	0.02%	0.002%
71	10.192	2891	2893	2895	rBV2	510	288	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007365.D
 Acq On : 05 Sep 2018 07:06
 Operator : SY/MD
 Sample : J4695-20
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGB5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.266	2903	2916	2948	rBV	601290	956459	46.81%	5.814%
73	10.375	2948	2950	2952	rVV2	601	333	0.02%	0.002%
74	10.427	2956	2966	2977	rVB4	2986	4891	0.24%	0.030%
75	10.520	2988	2995	2998	rBV3	292	331	0.02%	0.002%
76	10.543	2998	3002	3003	rBV2	449	296	0.01%	0.002%
77	10.552	3003	3005	3010	rVB	428	254	0.01%	0.002%
78	11.153	3189	3192	3194	rVB	490	281	0.01%	0.002%
79	11.211	3208	3210	3212	rBV	388	271	0.01%	0.002%
80	11.301	3225	3238	3265	rBV	733450	1186679	58.08%	7.213%
81	11.559	3313	3318	3319	rBV3	420	350	0.02%	0.002%
82	11.581	3319	3325	3329	rBV6	1980	2532	0.12%	0.015%
83	11.678	3342	3355	3376	rBV	740296	1215538	59.49%	7.389%
84	12.292	3542	3546	3547	rBV2	584	388	0.02%	0.002%
85	12.305	3547	3550	3553	rVV2	917	800	0.04%	0.005%
86	12.334	3556	3559	3562	rBV2	556	345	0.02%	0.002%
87	12.404	3579	3581	3588	rVB3	629	548	0.03%	0.003%
88	12.481	3602	3605	3607	rBV	664	386	0.02%	0.002%
89	12.661	3656	3661	3663	rBV4	522	528	0.03%	0.003%
90	12.745	3684	3687	3689	rBV2	804	542	0.03%	0.003%
91	12.825	3710	3712	3716	rBV3	392	276	0.01%	0.002%
92	12.880	3726	3729	3731	rBV2	676	484	0.02%	0.003%
93	12.935	3744	3746	3750	rVB3	687	423	0.02%	0.003%
94	13.321	3862	3866	3872	rBV5	1376	1364	0.07%	0.008%
95	13.440	3901	3903	3912	rBV4	807	1111	0.05%	0.007%
96	13.652	3967	3969	3975	rVB3	696	566	0.03%	0.003%
97	13.697	3977	3983	3987	rBV4	749	982	0.05%	0.006%
98	14.002	4075	4078	4083	rBV4	968	972	0.05%	0.006%
99	14.301	4169	4171	4176	rBV2	734	762	0.04%	0.005%
100	14.478	4224	4226	4229	rVB4	1122	514	0.03%	0.003%


Sum of corrected areas: 16451032

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090418\
Data File : VV007365.D
Acq On : 05 Sep 2018 07:06
Operator : SY/MD
Sample : J4695-20
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGB5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

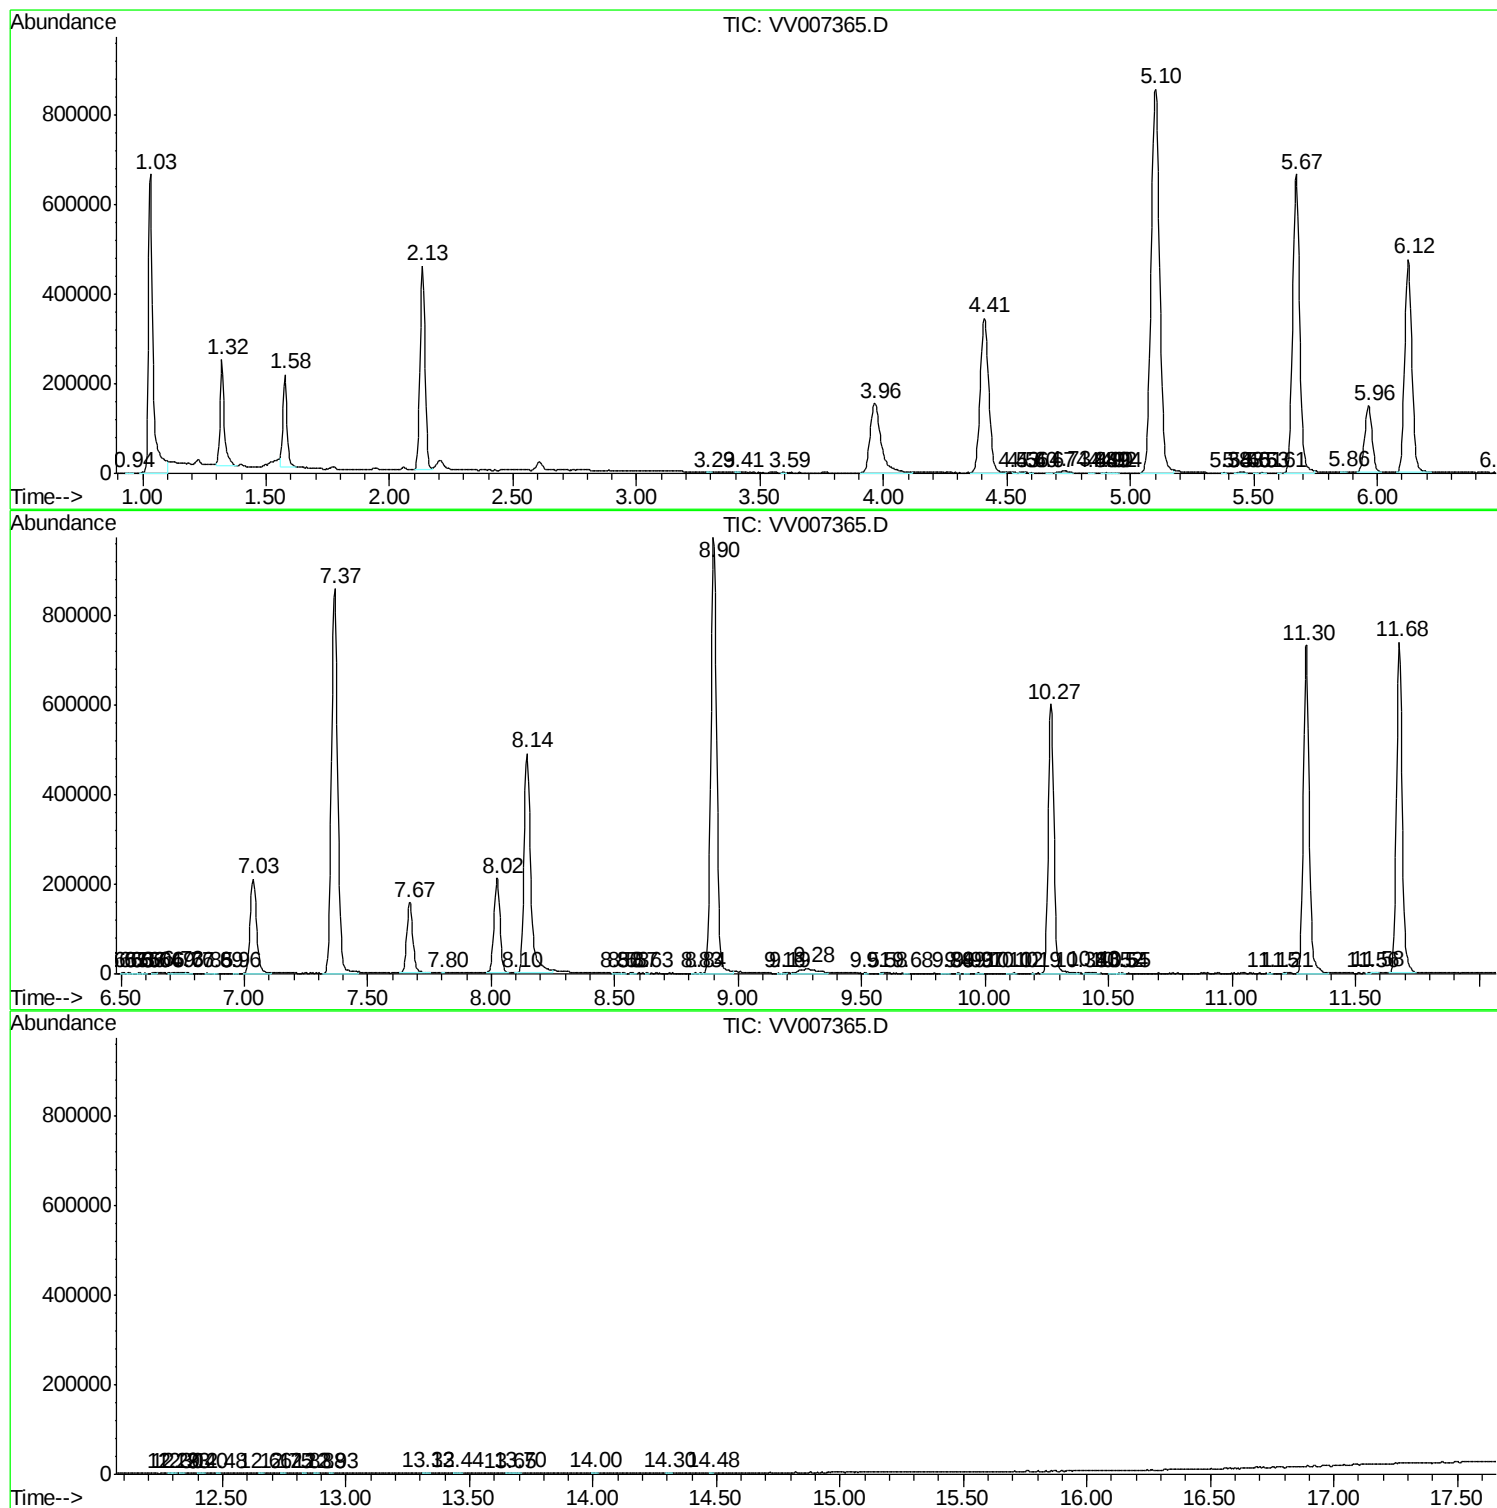

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007365.D
Acq On : 05 Sep 2018 07:06
Operator : SY/MD
Sample : J4695-20
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGB5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007365.D
Acq On : 05 Sep 2018 07:06
Operator : SY/MD
Sample : J4695-20
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGB5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc