

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007375.D
 Acq On : 05 Sep 2018 11:13
 Operator : SY/MD
 Sample : J4665-19DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.951	14	19	22	rBV3	412	381	0.002%	0.0002%
2	1.028	28	43	64	rBV	1611741	1862206	93.35%	10.385%
3	1.321	128	134	164	rVB	218167	280662	14.07%	1.565%
4	1.569	206	211	227	rVB	189525	226819	11.37%	1.265%
5	2.131	376	386	398	rVB	448723	624493	31.31%	3.483%
6	3.308	749	752	754	rBV	607	397	0.002%	0.0002%
7	3.366	767	770	775	rVB4	703	498	0.002%	0.0003%
8	3.517	815	817	820	rBV3	456	273	0.001%	0.0002%
9	3.533	820	822	826	rVB	548	279	0.001%	0.0002%
10	3.556	826	829	833	rBV3	407	299	0.001%	0.0002%
11	3.662	859	862	866	rVB2	368	259	0.001%	0.0001%
12	3.694	866	872	875	rVB3	577	571	0.003%	0.0003%
13	3.713	875	878	880	rBV2	319	251	0.001%	0.0001%
14	3.736	882	885	890	rVB	592	469	0.002%	0.0003%
15	3.771	890	896	899	rBV4	598	548	0.003%	0.0003%
16	3.835	911	916	919	rBV2	303	248	0.001%	0.0001%
17	3.967	938	957	1005	rBV2	473790	1292979	64.82%	7.211%
18	4.292	1055	1058	1060	rBV3	506	332	0.002%	0.0002%
19	4.308	1060	1063	1068	rVB4	797	601	0.003%	0.0003%
20	4.408	1071	1094	1121	rBV	338455	811124	40.66%	4.523%
21	4.649	1167	1169	1173	rVB2	470	358	0.002%	0.0002%
22	4.694	1177	1183	1186	rVB4	670	629	0.003%	0.0004%
23	4.716	1186	1190	1193	rBV3	649	551	0.003%	0.0003%
24	4.781	1205	1210	1216	rVB6	799	855	0.004%	0.0005%
25	4.861	1232	1235	1237	rBV	403	281	0.001%	0.0002%
26	4.987	1272	1274	1277	rVB2	373	229	0.001%	0.0001%
27	5.102	1288	1310	1335	rBV2	839364	1994862	100.00%	11.125%
28	5.269	1360	1362	1369	rVB5	486	403	0.002%	0.0002%
29	5.327	1375	1380	1384	rVB5	796	817	0.004%	0.0005%
30	5.350	1384	1387	1392	rBV4	732	825	0.004%	0.0005%
31	5.433	1407	1413	1414	rBV3	673	626	0.003%	0.0003%
32	5.453	1416	1419	1432	rVB6	1376	2289	0.11%	0.0013%
33	5.504	1432	1435	1436	rBV2	529	261	0.001%	0.0001%
34	5.575	1450	1457	1463	rBV3	409	580	0.003%	0.0003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007375.D
 Acq On : 05 Sep 2018 11:13
 Operator : SY/MD
 Sample : J4665-19DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	5.671	1467	1487	1520	rBV	585888	1168053	58.55%	6.514%
36	5.964	1559	1578	1605	rBV2	353271	701456	35.16%	3.912%
37	6.125	1613	1628	1652	rBV	466660	941208	47.18%	5.249%
38	6.247	1662	1666	1667	rBV4	1165	765	0.04%	0.004%
39	6.298	1680	1682	1685	rVB3	575	276	0.01%	0.002%
40	6.597	1771	1775	1778	rBV3	402	397	0.02%	0.002%
41	6.617	1778	1781	1784	rVB2	399	244	0.01%	0.001%
42	6.633	1784	1786	1788	rBV3	416	272	0.01%	0.002%
43	6.652	1788	1792	1794	rBV4	1118	784	0.04%	0.004%
44	6.684	1800	1802	1806	rVB2	441	246	0.01%	0.001%
45	6.726	1806	1815	1823	rBV4	2335	4450	0.22%	0.025%
46	6.774	1827	1830	1832	rBV	452	258	0.01%	0.001%
47	6.829	1844	1847	1854	rVB4	636	625	0.03%	0.003%
48	6.864	1854	1858	1860	rBV3	643	420	0.02%	0.002%
49	7.035	1898	1911	1931	rBV	222439	396150	19.86%	2.209%
50	7.366	1999	2014	2036	rBV	841818	1451930	72.78%	8.097%
51	7.668	2095	2108	2127	rBV	165435	275436	13.81%	1.536%
52	7.806	2147	2151	2154	rBV3	825	652	0.03%	0.004%
53	7.896	2177	2179	2181	rBV	665	373	0.02%	0.002%
54	8.022	2203	2218	2236	rVB	195132	328196	16.45%	1.830%
55	8.144	2243	2256	2283	rBV	514218	949554	47.60%	5.295%
56	8.549	2380	2382	2389	rVB5	469	512	0.03%	0.003%
57	8.597	2394	2397	2400	rVB3	409	280	0.01%	0.002%
58	8.758	2445	2447	2450	rBV2	393	262	0.01%	0.001%
59	8.826	2466	2468	2472	rVB4	615	320	0.02%	0.002%
60	8.900	2478	2491	2514	rBV	840091	1377287	69.04%	7.681%
61	9.279	2607	2609	2614	rVB3	772	500	0.03%	0.003%
62	9.308	2614	2618	2621	rBV2	397	286	0.01%	0.002%
63	9.340	2625	2628	2630	rBV2	415	259	0.01%	0.001%
64	9.420	2649	2653	2656	rBV2	403	366	0.02%	0.002%
65	9.498	2673	2677	2680	rBV2	393	296	0.01%	0.002%
66	9.530	2684	2687	2689	rBV3	373	223	0.01%	0.001%
67	9.707	2738	2742	2746	rBV3	720	707	0.04%	0.004%
68	9.790	2765	2768	2771	rVB4	416	277	0.01%	0.002%
69	9.816	2771	2776	2778	rBV2	418	355	0.02%	0.002%
70	9.851	2783	2787	2790	rBV3	421	277	0.01%	0.002%
71	9.935	2811	2813	2817	rBV3	397	232	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007375.D
 Acq On : 05 Sep 2018 11:13
 Operator : SY/MD
 Sample : J4665-19DL 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 E0AB8DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.035	2839	2844	2846	rBV2	535	474	0.02%	0.003%
73	10.128	2871	2873	2876	rVB2	643	336	0.02%	0.002%
74	10.144	2876	2878	2882	rBV	400	243	0.01%	0.001%
75	10.199	2892	2895	2902	rVB3	477	369	0.02%	0.002%
76	10.266	2903	2916	2944	rBV	605149	964552	48.35%	5.379%
77	10.427	2958	2966	2970	rBV3	921	1286	0.06%	0.007%
78	10.507	2987	2991	2994	rBV2	299	221	0.01%	0.001%
79	10.626	3023	3028	3029	rBV2	699	548	0.03%	0.003%
80	10.652	3034	3036	3041	rVB3	520	446	0.02%	0.002%
81	10.690	3045	3048	3051	rBV3	420	277	0.01%	0.002%
82	10.813	3083	3086	3089	rBV3	492	311	0.02%	0.002%
83	10.899	3111	3113	3117	rBV3	526	451	0.02%	0.003%
84	10.993	3136	3142	3146	rBV2	535	644	0.03%	0.004%
85	11.076	3164	3168	3170	rBV	379	247	0.01%	0.001%
86	11.121	3178	3182	3183	rBV2	545	354	0.02%	0.002%
87	11.179	3195	3200	3202	rBV2	514	476	0.02%	0.003%
88	11.301	3221	3238	3262	rBV	651161	1042441	52.26%	5.813%
89	11.578	3319	3324	3325	rBV3	1106	882	0.04%	0.005%
90	11.678	3342	3355	3380	rBV	737779	1201867	60.25%	6.702%
91	12.060	3472	3474	3476	rBV2	439	279	0.01%	0.002%
92	12.073	3476	3478	3482	rVB2	776	497	0.02%	0.003%
93	12.276	3539	3541	3544	rBV2	401	272	0.01%	0.002%
94	12.880	3726	3729	3732	rBV4	689	505	0.03%	0.003%
95	13.022	3770	3773	3775	rBV2	556	364	0.02%	0.002%
96	13.137	3805	3809	3814	rVB2	626	574	0.03%	0.003%
97	13.205	3826	3830	3833	rBV3	547	413	0.02%	0.002%
98	13.504	3921	3923	3925	rBV	601	293	0.01%	0.002%
99	13.623	3957	3960	3963	rBV2	665	441	0.02%	0.002%
100	14.153	4122	4125	4126	rBV2	723	362	0.02%	0.002%


Sum of corrected areas: 17931864

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090418\
Data File : VV007375.D
Acq On : 05 Sep 2018 11:13
Operator : SY/MD
Sample : J4665-19DL 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

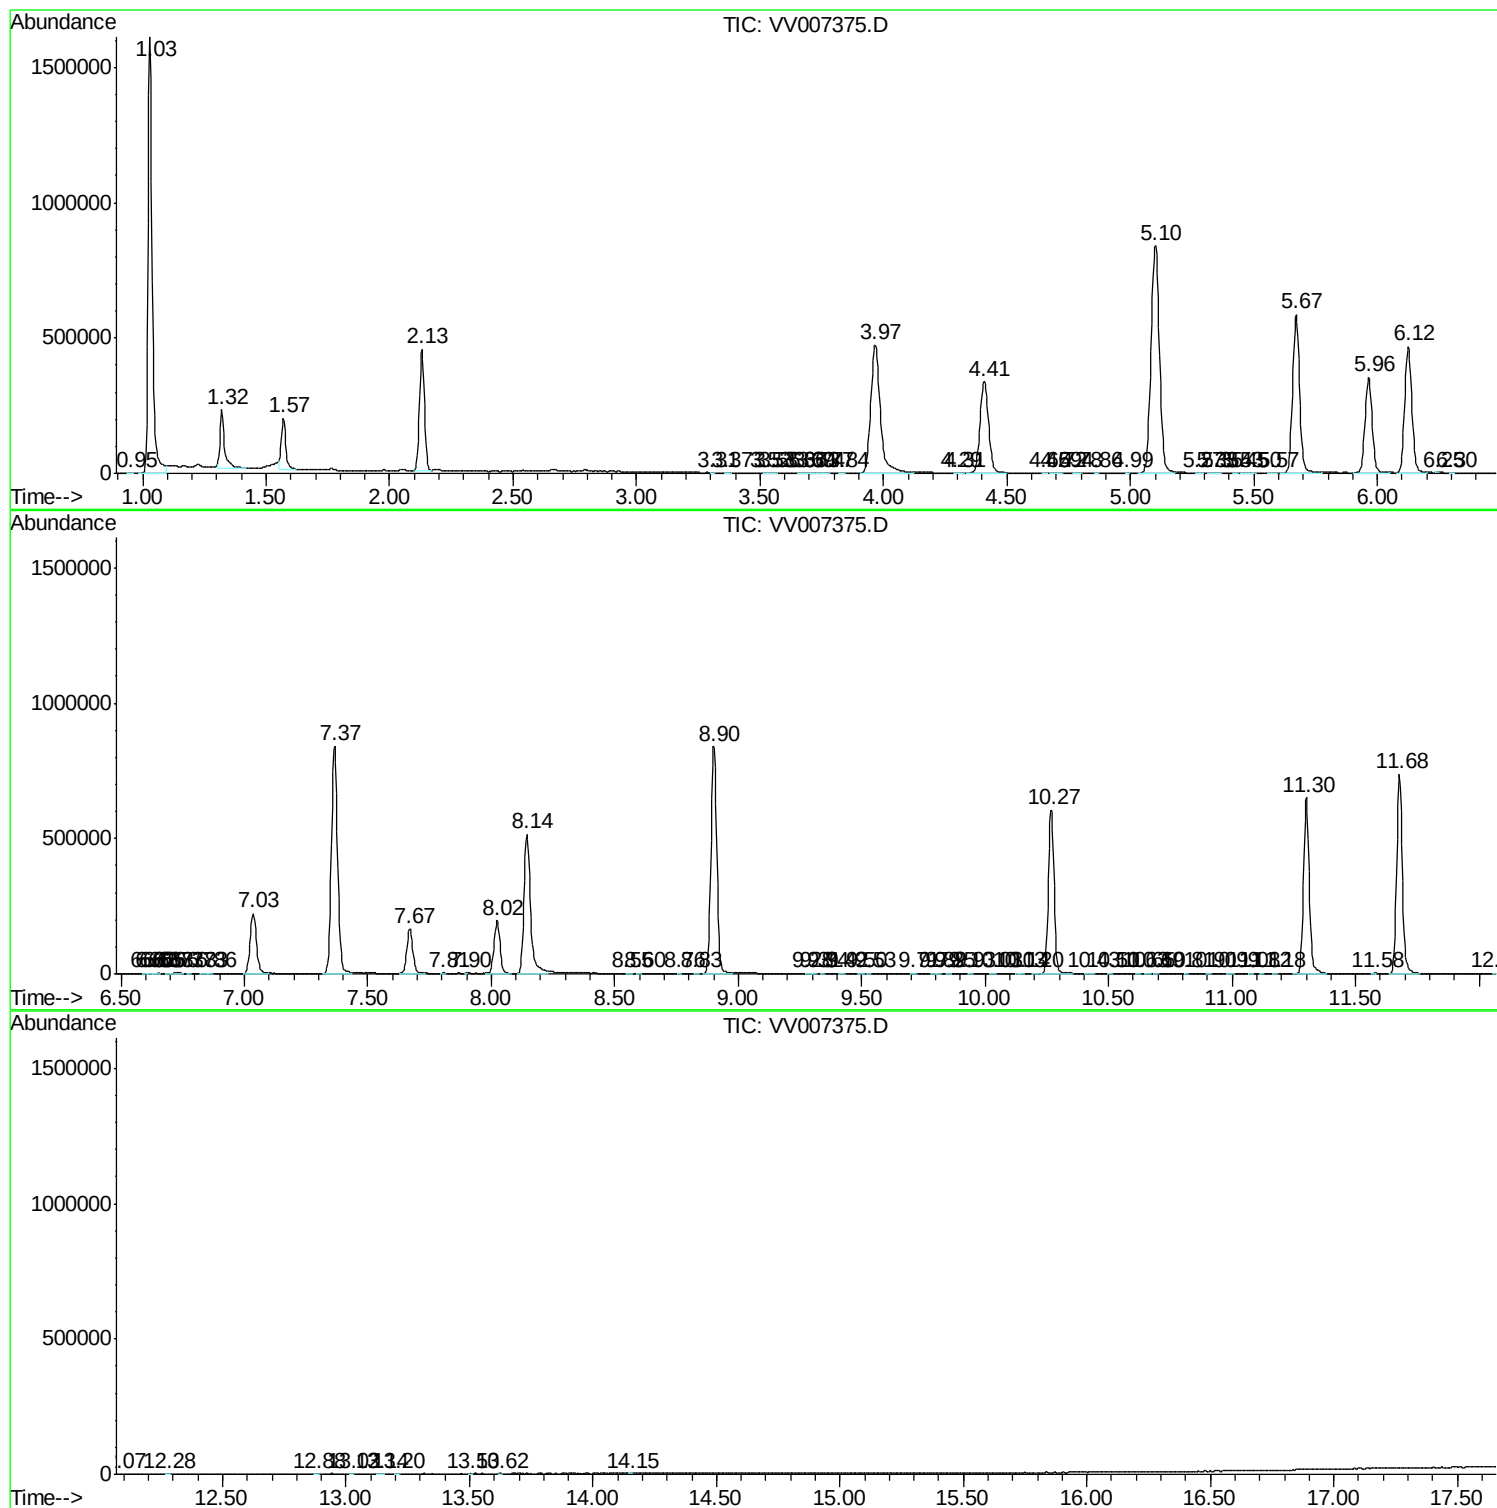

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090418\
Data File : VV007375.D
Acq On : 05 Sep 2018 11:13
Operator : SY/MD
Sample : J4665-19DL 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
E0AB8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV090418\
Data File : VV007375.D
Acq On : 05 Sep 2018 11:13
Operator : SY/MD
Sample : J4665-19DL 50X
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
E0AB8DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc