


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090418\
 Data File : VV007336.D
 Acq On : 04 Sep 2018 18:08
 Operator : SY/MD
 Sample : BFB71
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB71

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis
 Last Update : Thu Sep 06 02:12:11 2018

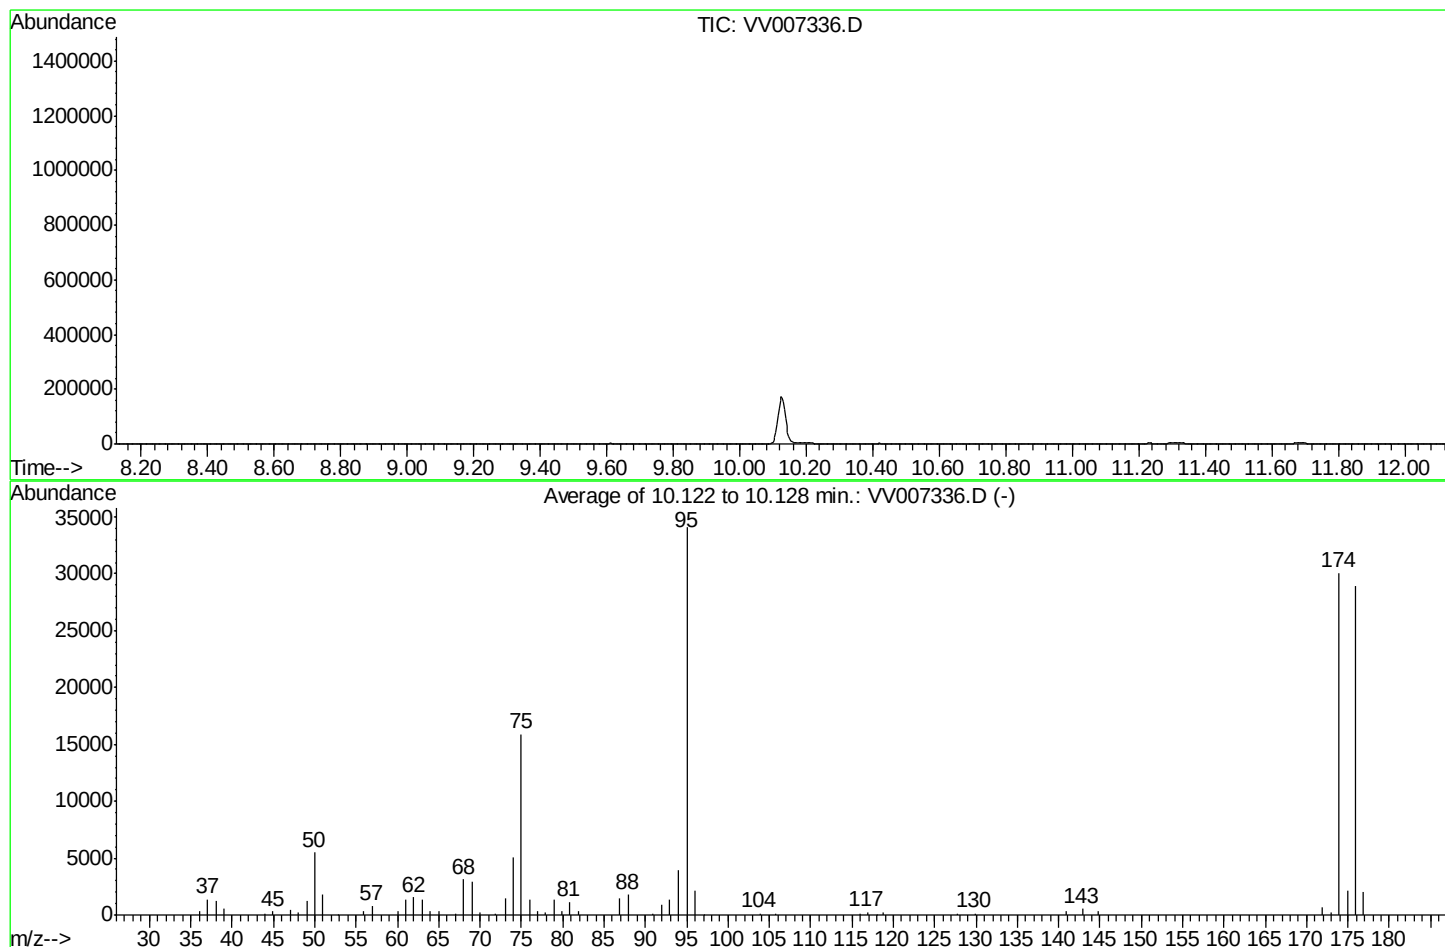

AutoFind: Scans 2871, 2872, 2873; Background Corrected with Scan 2860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	5487	PASS
75	95	30	80	46.7	15928	PASS
95	95	100	100	100.0	34088	PASS
96	95	5	9	6.3	2139	PASS
173	174	0.00	2	0.8	235	PASS
174	95	50	120	88.2	30056	PASS
175	174	5	9	6.9	2087	PASS
176	174	95	101	96.3	28936	PASS
177	176	5	9	7.1	2046	PASS

Scan 2860 (10.086 min): VV007336.D
BFB71

m/z	Abundance
39.90	292.0
43.90	964.0
206.90	119.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	299.0
37.00	1380.0
38.00	1131.0
39.00	630.0
39.90	315.0
44.00	1195.0
45.00	283.0
47.00	447.0
48.00	258.0
49.00	1131.0
50.00	5651.0
51.00	1763.0
55.90	392.0
56.90	749.0
60.10	279.0
61.00	1508.0
62.00	1552.0
63.00	1270.0
64.00	303.0
65.00	310.0
67.10	108.0
68.00	3020.0
69.00	2762.0
70.00	199.0
71.80	151.0
73.00	1378.0
74.00	5239.0
75.00	15395.0
76.00	1306.0
76.90	352.0
77.80	256.0
78.90	1391.0
79.90	297.0
80.80	1140.0
82.00	331.0
86.90	1414.0
87.90	1592.0
90.90	109.0
91.90	842.0
92.90	1378.0
94.00	3617.0
95.00	32568.0
96.00	2153.0
103.80	127.0
105.80	116.0
115.90	130.0
116.90	238.0
118.80	229.0
127.80	104.0
129.90	149.0
140.80	267.0
142.90	545.0
144.80	330.0
171.90	647.0
173.90	27544.0
174.90	2042.0
175.90	26960.0
176.90	1882.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	323.0
37.00	1475.0
38.00	1239.0
39.00	642.0
39.90	265.0
44.00	1121.0
44.90	299.0
47.10	485.0
48.00	223.0
49.00	1259.0
50.00	5603.0
51.00	1860.0
52.80	103.0
55.90	402.0
56.90	879.0
60.00	330.0
61.00	1399.0
62.00	1590.0
63.00	1342.0
64.00	296.0
65.00	357.0
67.10	121.0
68.00	3198.0
69.00	2988.0
69.90	239.0
71.80	178.0
73.00	1513.0
74.00	5220.0
75.00	16345.0
76.00	1370.0
76.90	367.0
77.80	272.0
78.90	1431.0
79.90	301.0
80.80	1159.0
81.90	365.0
86.90	1526.0
87.90	1842.0
90.90	144.0
92.00	900.0
93.00	1418.0
94.00	4048.0
95.00	35200.0
96.00	2213.0
97.00	104.0
103.90	127.0
105.80	117.0
115.90	127.0
116.90	268.0
118.80	257.0
127.80	126.0
129.90	144.0
140.80	301.0
142.90	566.0
144.80	321.0
171.90	669.0
173.00	338.0
173.90	30968.0
174.90	2151.0
175.90	29880.0
176.90	2111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71

m/z	Abundance
36.00	283.0
37.00	1348.0
38.00	1205.0
39.00	582.0
40.00	229.0
44.00	1097.0
44.90	284.0
47.10	421.0
47.90	178.0
49.00	1281.0
50.00	5209.0
51.00	1861.0
55.90	387.0
56.90	882.0
60.00	393.0
61.00	1284.0
62.00	1430.0
63.00	1282.0
64.00	291.0
64.90	369.0
68.00	3096.0
69.00	3086.0
70.00	265.0
71.80	183.0
73.00	1603.0
74.00	4845.0
75.00	16046.0
76.00	1342.0
76.90	366.0
77.80	215.0
78.90	1286.0
79.90	299.0
80.80	1113.0
81.90	341.0
86.90	1526.0
87.90	1828.0
90.90	178.0
92.00	891.0
93.00	1405.0
94.00	4129.0
95.00	34496.0
96.00	2051.0
103.90	131.0
105.80	119.0
115.90	117.0
116.90	280.0
118.00	108.0
118.80	259.0
127.80	123.0
129.90	122.0
140.90	324.0
142.90	490.0
144.80	241.0
171.90	656.0
172.90	367.0
173.90	31656.0
174.90	2068.0
175.90	29968.0
176.90	2147.0
207.00	117.0

Instrument :
MSVOA_V
ClientSampleId :
BFB71