

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090419\
 Data File : VV012559.D
 Acq On : 04 Sep 2019 11:20
 Operator : SY/MD
 Sample : K4605-02
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0AA1

Quant Time: Sep 05 01:58:00 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 05 01:26:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	134383	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	133934	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	46851	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	58032	4.45	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.00%
7) Chloroethane-d5	1.58	69	63402	4.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.20%
11) 1,1-Dichloroethene-d2	2.13	63	99974	3.14	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.80%
20) 2-Butanone-d5	3.96	46	124623	50.11	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	100.22%
24) Chloroform-d	4.40	84	98112	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
26) 1,2-Dichloroethane-d4	5.08	65	52644	5.06	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.20%
32) Benzene-d6	5.10	84	176195	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.40%
36) 1,2-Dichloropropane-d6	6.12	67	58028	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	7.36	98	138814	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.40%
43) trans-1,3-Dichloropropene-	7.67	79	18558	4.28	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	85.60%
46) 2-Hexanone-d5	8.14	63	66488	40.99	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.98%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	38916	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	45559	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds					Ovalue
13) Acetone	2.22	43	27768	7.868 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090419\
Data File : VV012559.D
Acq On : 04 Sep 2019 11:20
Operator : SY/MD
Sample : K4605-02
Misc : 25mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0AA1

Quant Time: Sep 05 01:58:00 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 05 01:26:42 2019
Response via : Initial Calibration

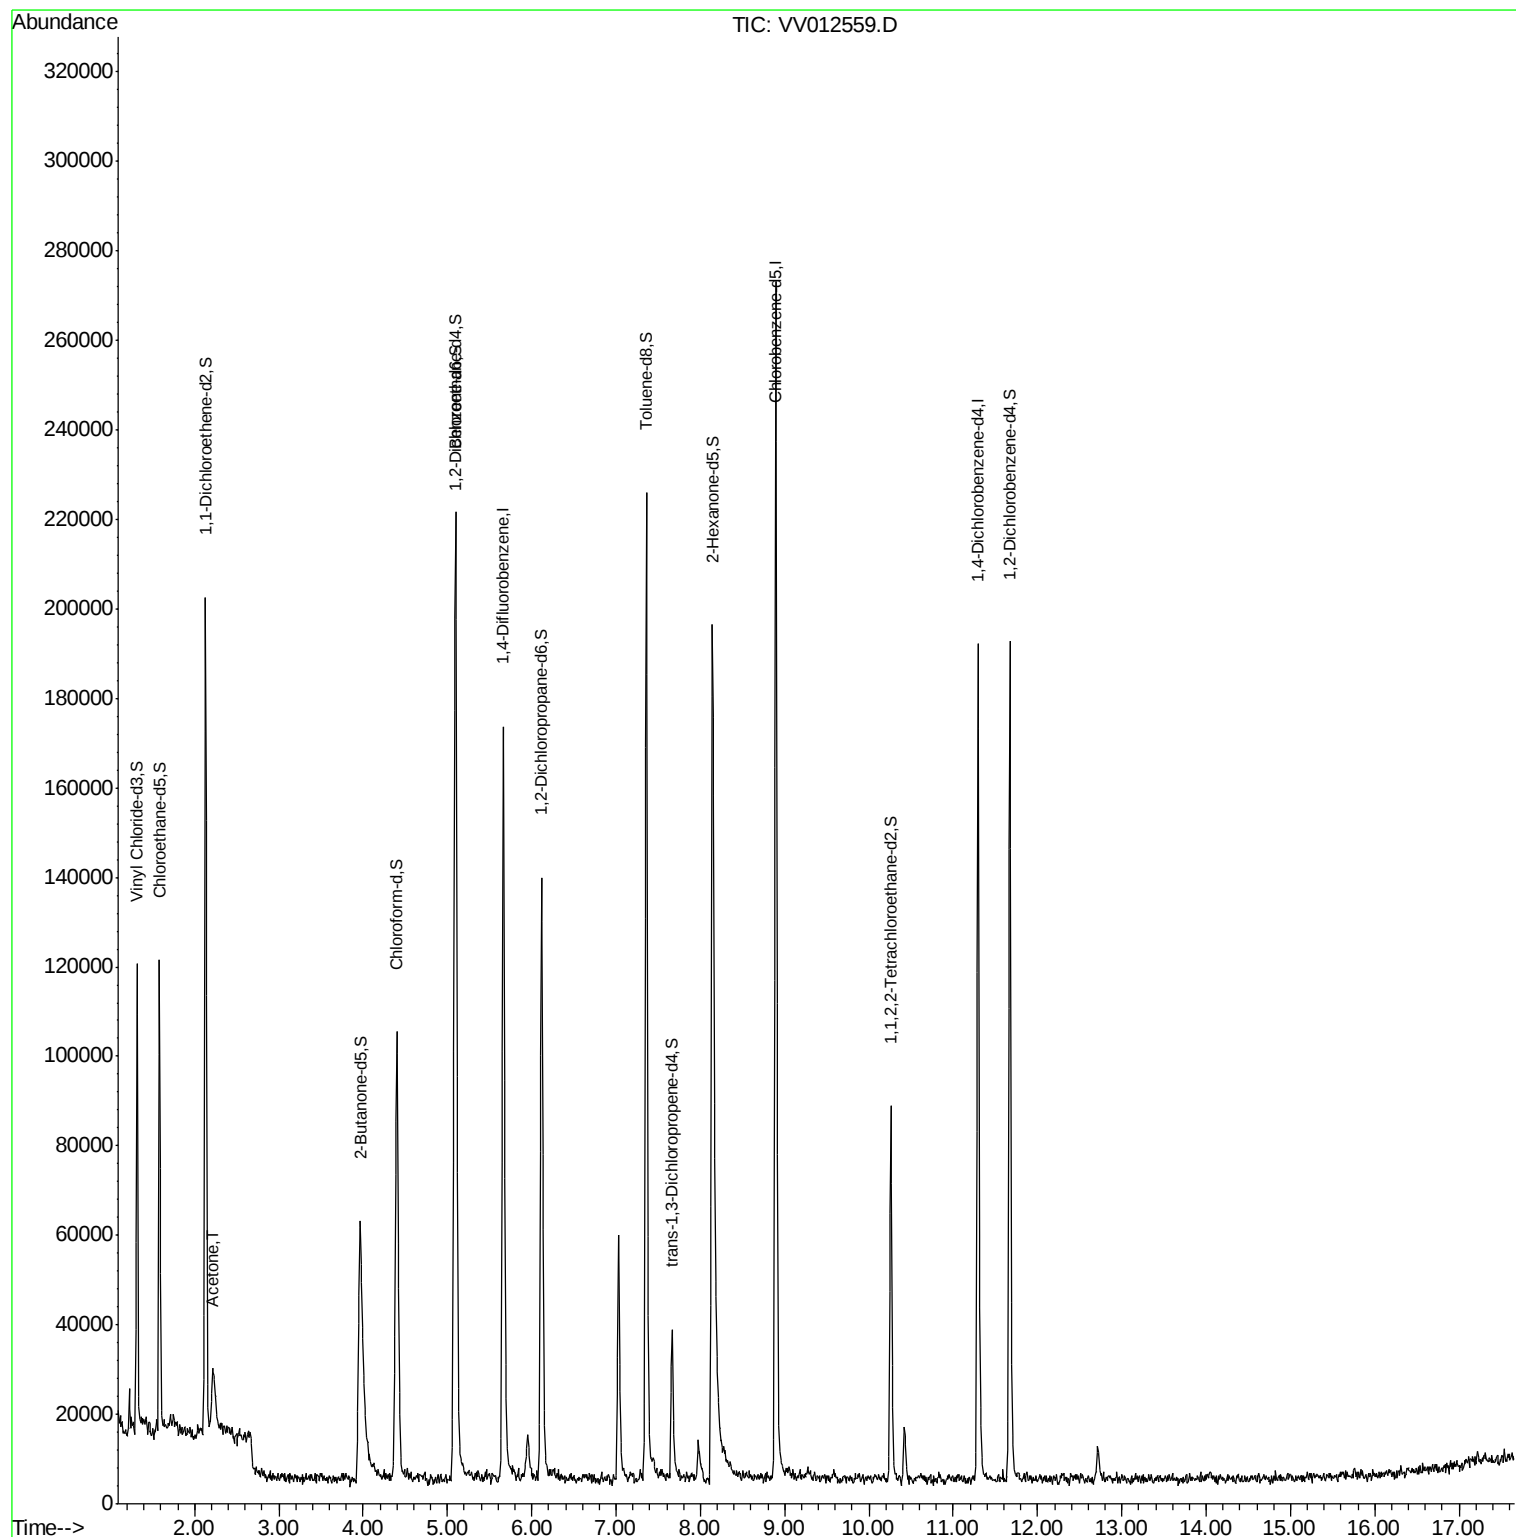

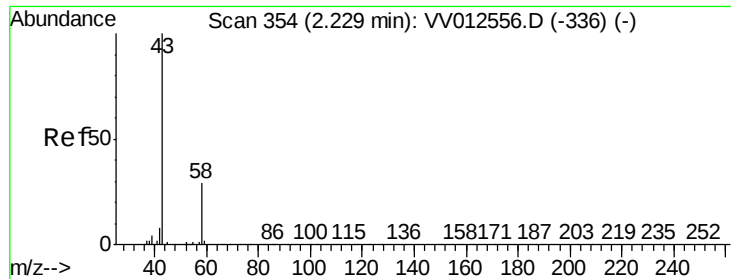

#13
Acetone
Concen: 7.868 ug/L
RT: 2.22 min Scan# 350
Delta R.T. -0.01 min
Lab File: VV012559.D
Acq: 04 Sep 2019 11:20

Instrument :
MSVOA_V
ClientSampleId :
C0AA1

Tot Ion: 43 Resp: 27768
Ion Ratio Lower Upper
43 100
58 34.9 0.0 58.2

