

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090419\
 Data File : VV012570.D
 Acq On : 04 Sep 2019 16:12
 Operator : SY/MD
 Sample : K4685-05
 Misc : 25mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFD74

Quant Time: Sep 05 02:34:38 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Sep 05 01:26:42 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	129287	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	134316	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	45660	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	52908	4.21	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	84.20%
7) Chloroethane-d5	1.59	69	59101	4.76	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	95.20%
11) 1,1-Dichloroethene-d2	2.13	63	93721	3.06	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	61.20%
20) 2-Butanone-d5	3.96	46	142796	59.68	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	119.36%
24) Chloroform-d	4.40	84	96929	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
26) 1,2-Dichloroethane-d4	5.08	65	54890	5.48	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.60%
32) Benzene-d6	5.10	84	171720	4.54	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.80%
36) 1,2-Dichloropropane-d6	6.12	67	59463	5.00	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.00%
41) Toluene-d8	7.36	98	133900	3.91	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	78.20%
43) trans-1,3-Dichloropropene-	7.67	79	18874	4.34	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	86.80%
46) 2-Hexanone-d5	8.14	63	78112	48.02	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.04%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	42087	5.01	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	100.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	44626	5.32	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.40%


Target Compounds					Ovalue
13) Acetone	2.22	43	13473	3.968 ug/L	98
34) Trichloroethene	5.96	95	195000	12.761 ug/L	99
47) Tetrachloroethene	8.02	164	4875	0.442 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090419\
Data File : VV012570.D
Acq On : 04 Sep 2019 16:12
Operator : SY/MD
Sample : K4685-05
Misc : 25mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFD74

Quant Time: Sep 05 02:34:38 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Sep 05 01:26:42 2019
Response via : Initial Calibration

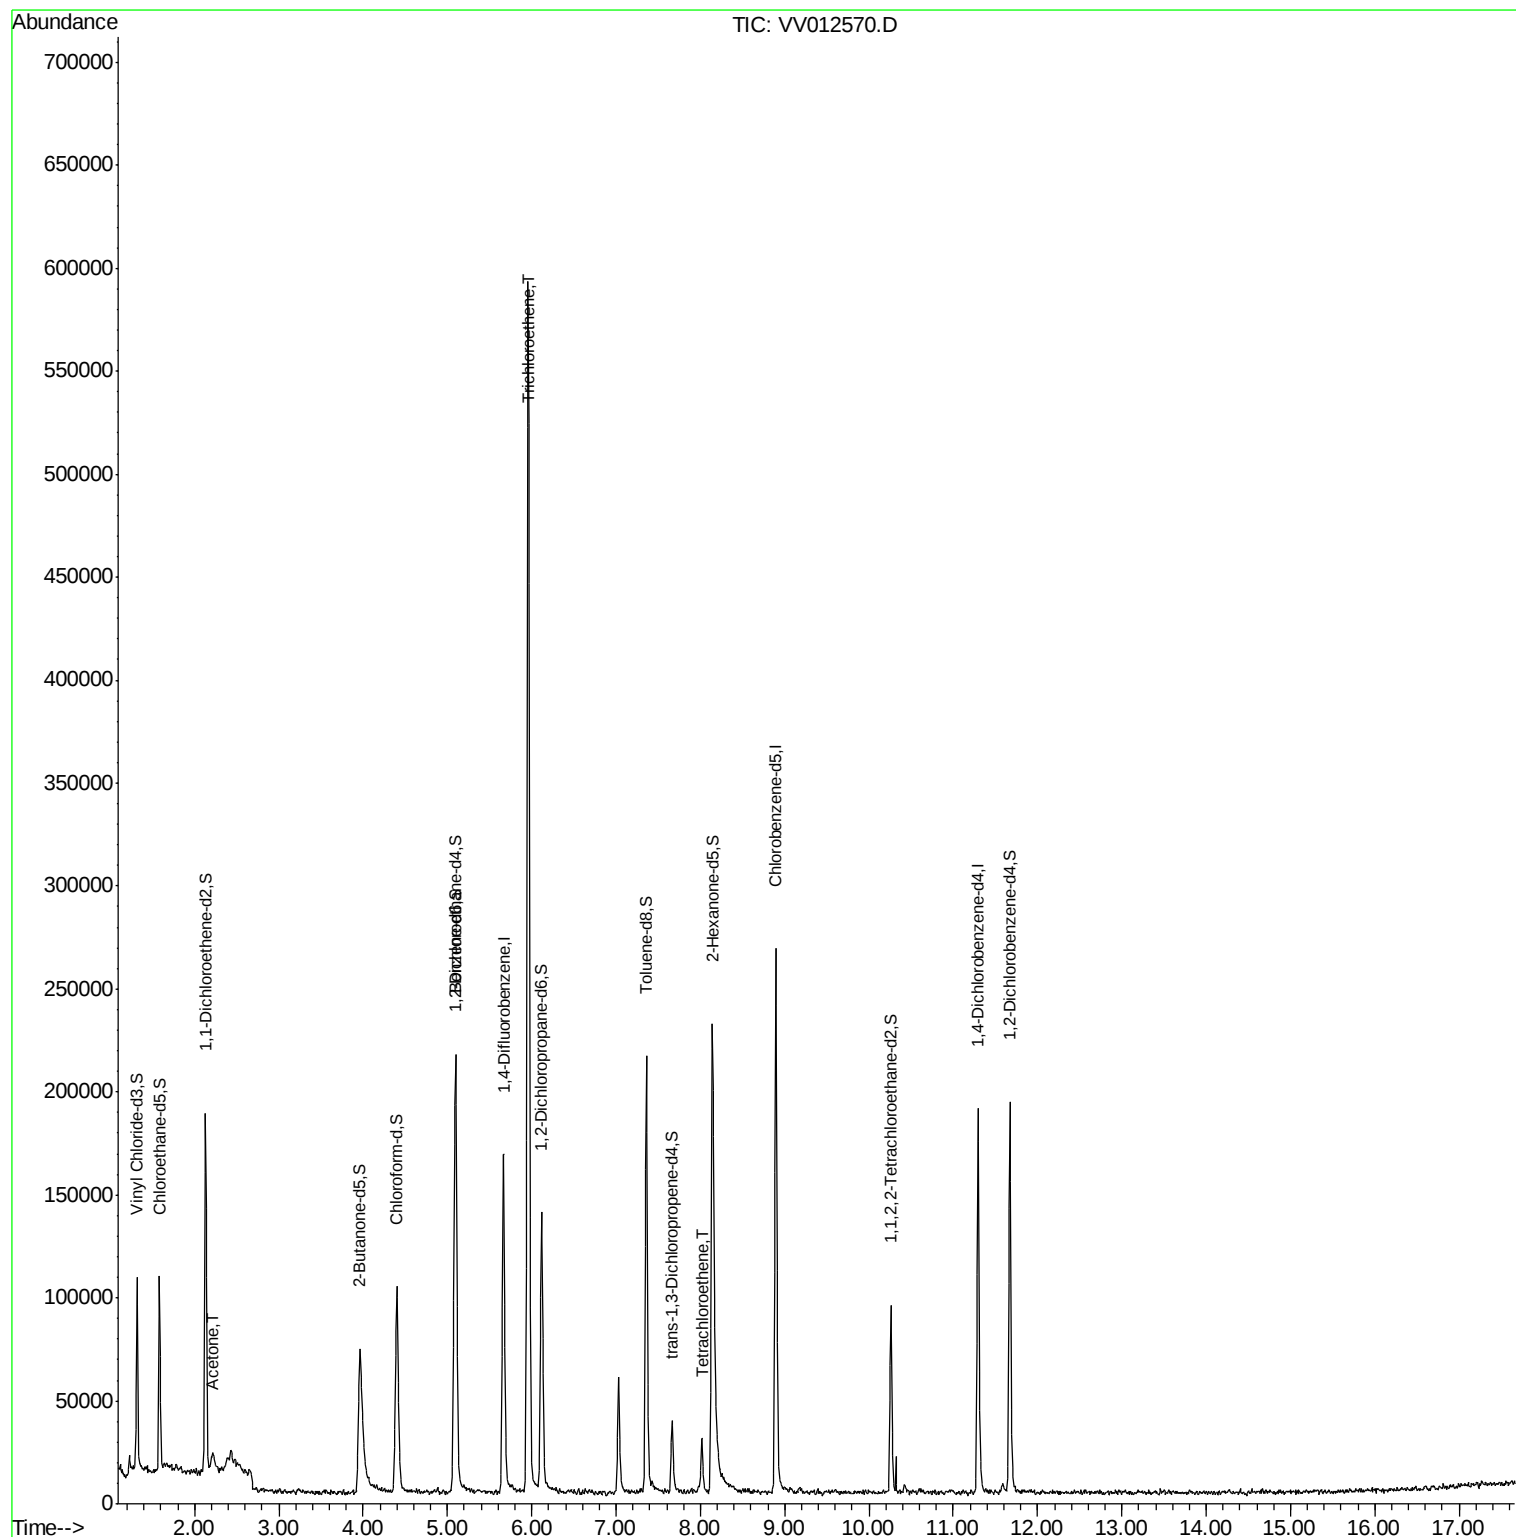

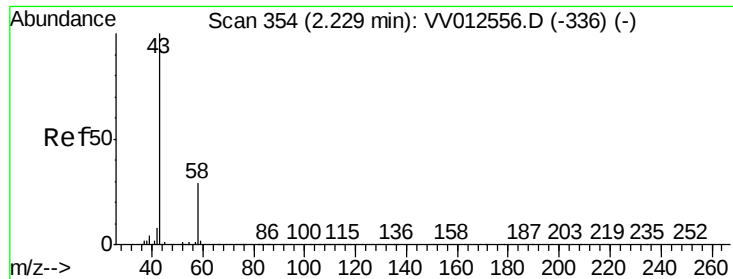

#13

Acetone

Concen: 3.968 ug/L

RT: 2.22 min Scan# 352

Delta R.T. -0.01 min

Lab File: VV012570.D

Acq: 04 Sep 2019 16:12

Instrument :

MSVOA_V

ClientSampled :


BFD74

Tot Ion: 43 Resp: 13473

Ion Ratio Lower Upper

43 100

58 28.2 0.0 58.2

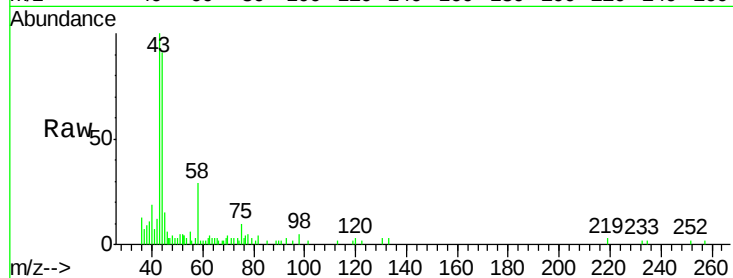

Abundance Ion 43.05 (42.75 to 43.75): VV012556.D (-336) (-)

Ion 58.05 (57.75 to 58.75): VV012556.D (-336) (-)

2.22

5000

4000

3000



2000

1000

0

Time-->

2.15 2.20 2.25 2.30

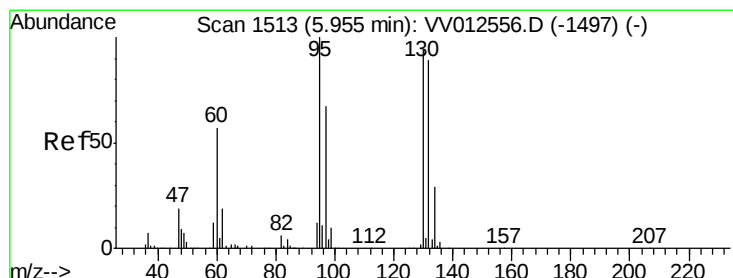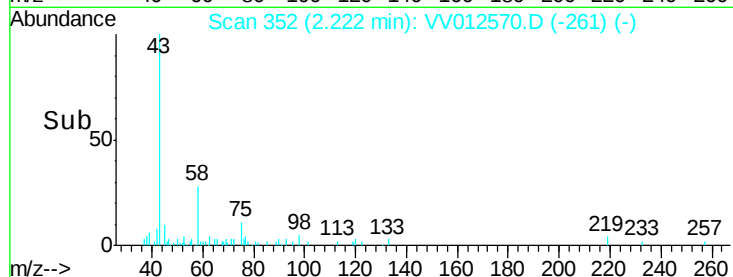

#34

Trichloroethene

Concen: 12.761 ug/L

RT: 5.96 min Scan# 1514

Delta R.T. 0.00 min

Lab File: VV012570.D

Acq: 04 Sep 2019 16:12

Tgt Ion: 95 Resp: 195000


Ion Ratio Lower Upper

95 100

97 65.0 44.7 83.1

132 91.7 63.8 118.4

130 96.9 66.6 123.6

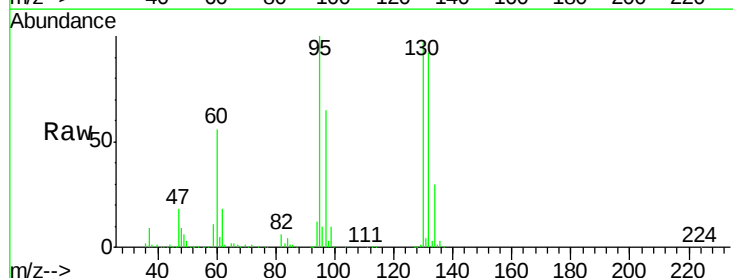

Abundance Ion 95.00 (94.70 to 95.70): VV012556.D (-1497) (-)

Ion 96.95 (96.65 to 97.65): VV012556.D (-1497) (-)

Ion 131.95 (131.65 to 132.65): VV012556.D (-1497) (-)

Ion 129.95 (129.65 to 130.65): VV012556.D (-1497) (-)

150000


100000


50000

0

Time-->

5.85 5.90 5.95 6.00 6.05

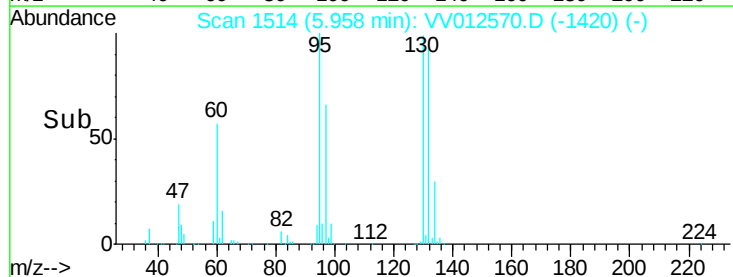

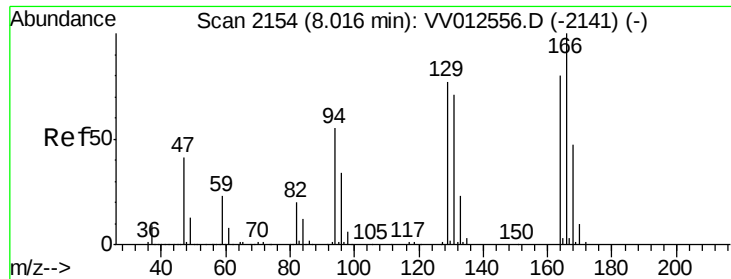

#47

Tetrachloroethene

Concen: 0.442 ug/L


RT: 8.02 min Scan# 2155

Delta R.T. 0.00 min

Lab File: VV012570.D

Acq: 04 Sep 2019 16:12

Instrument :
MSVOA_V
ClientSampleId :
BFD74

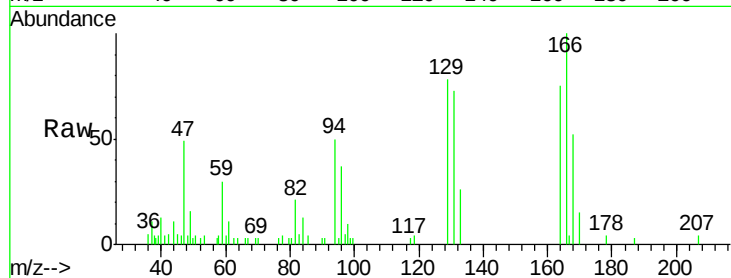

Tot Ion:164 Resp: 4875

Ion Ratio Lower Upper

164 100

129 103.5 64.5 119.9

131 97.1 62.3 115.7

166 132.9 86.5 160.6

Abundance Ion 163.90 (163.60 to 164.60): V

Ion 128.95 (128.65 to 129.65): V

Ion 130.95 (130.65 to 131.65): V

Ion 165.90 (165.60 to 166.60): V

