


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV090419\
Data File : VV012555.D
Acq On : 04 Sep 2019 08:34
Operator : SY/MD
Sample : BFB60
Misc : 25mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB60

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR090219WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Sep 05 01:26:42 2019

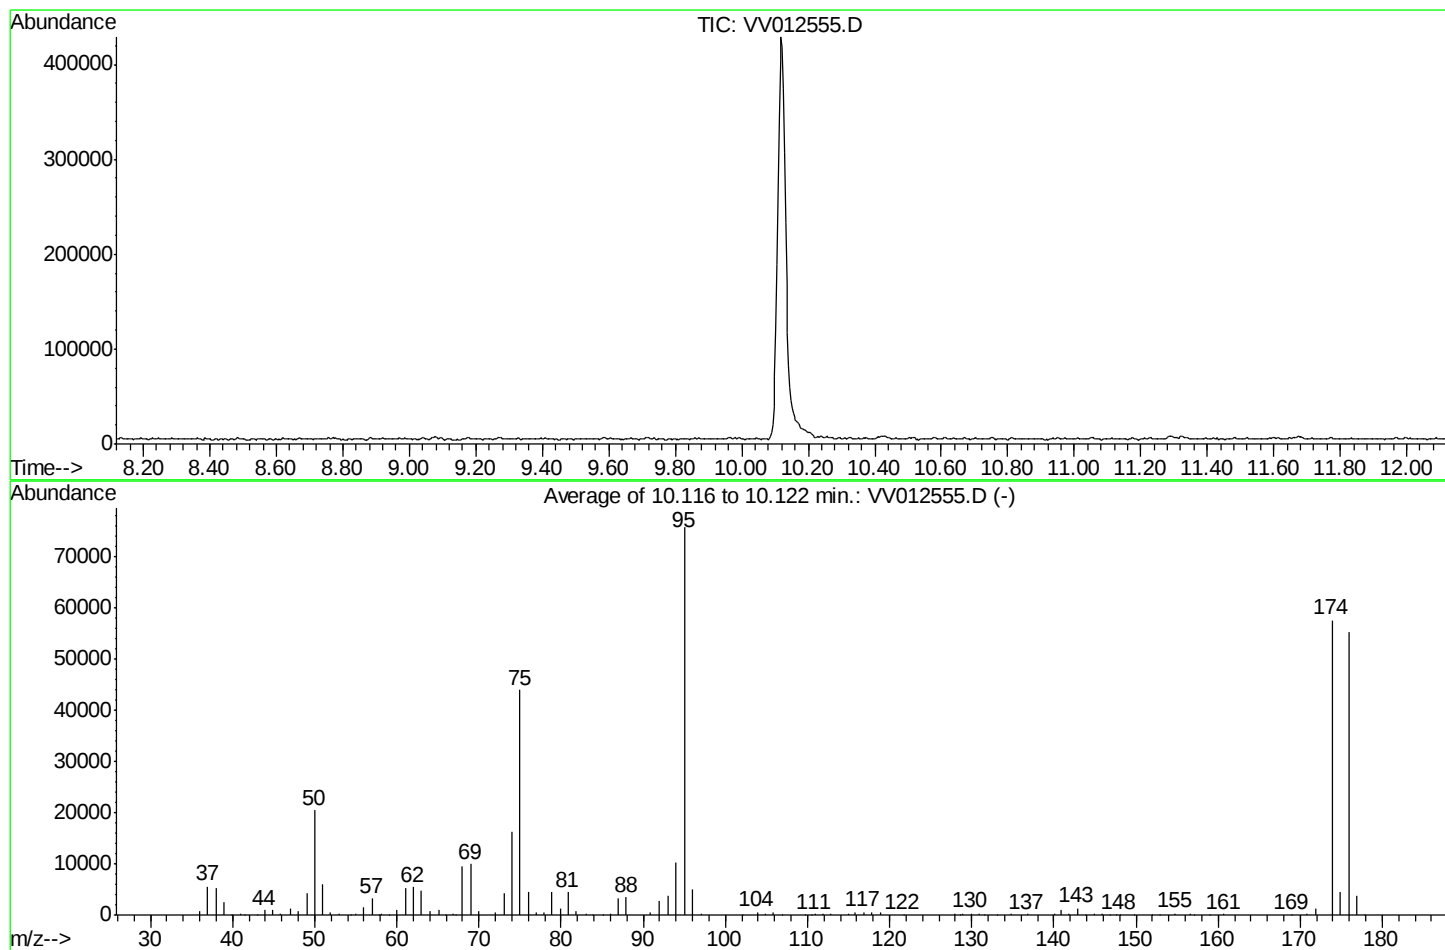

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	26.9	20392	PASS
75	95	30	80	58.1	43978	PASS
95	95	100	100	100.0	75701	PASS
96	95	5	9	6.6	5021	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.1	57608	PASS
175	174	5	9	8.0	4619	PASS
176	174	95	101	95.9	55224	PASS
177	176	5	9	6.7	3717	PASS

m/z	Abundance
35.90	1013.0
37.00	5624.0
38.00	5229.0
39.00	2452.0
40.00	658.0
41.00	143.0
41.40	119.0
42.80	190.0
43.90	1326.0
44.90	980.0
45.90	248.0
47.00	1206.0
47.90	730.0
49.00	4191.0
50.00	20016.0
51.00	5978.0
51.90	392.0
52.90	227.0
53.40	165.0
54.30	118.0
55.00	351.0
55.90	1716.0
57.00	3142.0
58.10	221.0
59.90	1046.0
61.00	5156.0
62.00	5339.0
63.00	4723.0
64.10	726.0
65.00	946.0
65.90	145.0
66.90	278.0
67.10	278.0
68.00	9255.0
69.00	9812.0
70.00	972.0
72.00	503.0
73.00	4096.0
74.00	15614.0
75.00	43264.0
76.00	4267.0
77.10	461.0
77.90	430.0
78.90	4274.0
79.90	1259.0
80.90	4527.0
81.90	798.0
83.00	188.0
83.90	101.0
85.10	110.0
85.90	227.0
86.90	3202.0
87.90	3424.0
90.80	324.0
92.00	2605.0
92.90	3547.0
94.00	9915.0
95.00	73928.0
96.00	4828.0
97.10	181.0
102.10	108.0
103.90	628.0
104.90	172.0
105.80	459.0
106.90	118.0
109.70	114.0
110.50	131.0
110.90	156.0
111.90	154.0
112.90	188.0
115.00	147.0
115.90	399.0
116.80	592.0
117.80	420.0
118.90	483.0
121.70	130.0
127.90	228.0
128.60	159.0
129.00	181.0
129.90	373.0
130.90	197.0
131.60	104.0
133.10	103.0
134.80	167.0
136.70	178.0
140.10	202.0
140.90	1016.0
141.80	203.0
142.90	1275.0
143.90	134.0
145.00	382.0
145.90	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

146.80	122.0
148.00	226.0
149.80	129.0
152.00	143.0
152.90	104.0
154.80	274.0
156.60	160.0
157.20	134.0
158.90	105.0
160.80	182.0
169.00	107.0
170.80	258.0
171.90	1161.0
173.90	54560.0
174.90	4409.0
175.90	51672.0
176.90	3736.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.90	1039.0
37.00	5903.0
38.00	5597.0
39.00	2605.0
39.90	598.0
40.90	150.0
41.50	119.0
43.00	199.0
43.90	1400.0
44.90	1095.0
45.90	255.0
47.00	1428.0
47.90	734.0
49.00	4350.0
50.00	21096.0
51.00	6279.0
51.90	427.0
52.90	223.0
53.20	183.0
53.90	121.0
55.00	392.0
55.90	1634.0
57.00	3309.0
58.10	197.0
60.00	1067.0
61.00	5270.0
61.90	5683.0
63.00	4885.0
64.00	739.0
65.10	986.0
65.90	153.0
66.90	272.0
68.00	9970.0
69.00	10189.0
70.00	1004.0
72.00	557.0
73.00	4562.0
74.00	16736.0
75.00	45264.0
76.00	4686.0
76.90	476.0
77.90	510.0
78.90	4522.0
79.90	1255.0
80.90	4744.0
81.80	868.0
83.00	164.0
86.00	289.0
86.90	3260.0
87.90	3556.0
90.90	392.0
92.00	2730.0
93.00	3729.0
94.00	10509.0
95.00	77664.0
96.00	5254.0
97.10	197.0
102.10	103.0
103.90	638.0
104.90	205.0
105.90	534.0
106.90	104.0
109.70	139.0
110.90	173.0
111.90	166.0
112.80	238.0
114.90	180.0
115.90	436.0
116.80	607.0
117.90	456.0
118.90	578.0
121.70	134.0
128.00	309.0
128.90	223.0
129.90	385.0
130.90	173.0
131.60	125.0
134.90	168.0
136.80	183.0
140.10	207.0
140.90	1123.0
141.80	226.0
142.90	1322.0
143.90	123.0
144.90	404.0
145.90	155.0
146.80	135.0
148.00	181.0
149.80	105.0
152.00	138.0
152.90	129.0
154.80	262.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

156.60	178.0
157.10	125.0
158.90	109.0
160.70	202.0
170.80	268.0
171.90	1362.0
173.90	59088.0
174.90	4742.0
175.90	56696.0
176.90	3821.0
177.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.90	909.0
37.00	5622.0
38.00	5401.0
39.00	2485.0
39.90	587.0
41.00	145.0
41.40	120.0
43.10	202.0
43.90	1361.0
45.00	1146.0
45.80	295.0
47.00	1313.0
48.00	718.0
49.00	4179.0
50.00	20064.0
51.00	5900.0
52.00	379.0
53.00	226.0
53.80	147.0
55.00	368.0
55.90	1464.0
57.00	3096.0
57.80	145.0
58.20	137.0
59.10	114.0
60.00	1137.0
61.00	5011.0
61.90	5317.0
63.00	4536.0
63.90	750.0
65.10	891.0
65.90	136.0
66.90	276.0
68.00	9615.0
69.00	9775.0
70.00	933.0
72.00	579.0
73.00	4450.0
74.00	16237.0
75.00	43408.0
76.00	4462.0
77.00	465.0
78.00	560.0
78.90	4388.0
79.90	1195.0
80.90	4379.0
81.80	897.0
83.00	147.0
86.10	339.0
86.90	3370.0
87.90	3459.0
90.90	453.0
91.90	2689.0
93.00	3769.0
94.00	10303.0
95.00	75512.0
96.00	4982.0
97.00	191.0
103.90	578.0
104.90	237.0
105.90	563.0
109.70	137.0
110.90	162.0
111.80	130.0
112.80	213.0
114.90	181.0
115.80	410.0
116.80	614.0
117.90	491.0
118.80	645.0
121.70	110.0
127.90	402.0
128.90	214.0
129.90	343.0
130.90	152.0
134.90	198.0
136.80	190.0
140.00	161.0
140.90	1037.0
141.80	196.0
142.90	1252.0
143.90	138.0
144.90	354.0
145.90	113.0
146.90	114.0
147.60	186.0
152.00	118.0
152.90	126.0
154.80	244.0
156.70	156.0
158.90	130.0
160.70	187.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

170.90	267.0
171.90	1382.0
173.90	59176.0
174.90	4708.0
175.90	57304.0
176.90	3596.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60

m/z	Abundance
35.20	144.0
35.90	189.0
36.90	130.0
37.90	160.0
38.70	138.0
39.90	571.0
42.30	112.0
42.80	101.0
43.90	410.0
44.80	154.0
45.50	133.0
46.30	141.0
47.40	151.0
49.50	109.0
51.40	119.0
52.30	179.0
53.30	158.0
53.90	119.0
54.70	105.0
55.40	111.0
58.40	163.0
61.50	100.0
64.30	118.0
66.00	104.0
69.80	116.0
71.90	149.0
73.70	124.0
74.60	117.0
80.80	154.0
89.80	102.0
100.30	104.0
106.10	121.0
124.80	102.0
150.10	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB60