


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090420\
 Data File : VV018153.D
 Acq On : 04 Sep 2020 11:16
 Operator : SY/MD
 Sample : BFB86
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB86

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM081120WMA.M
 Title : VOC Analysis
 Last Update : Mon Sep 07 03:40:15 2020

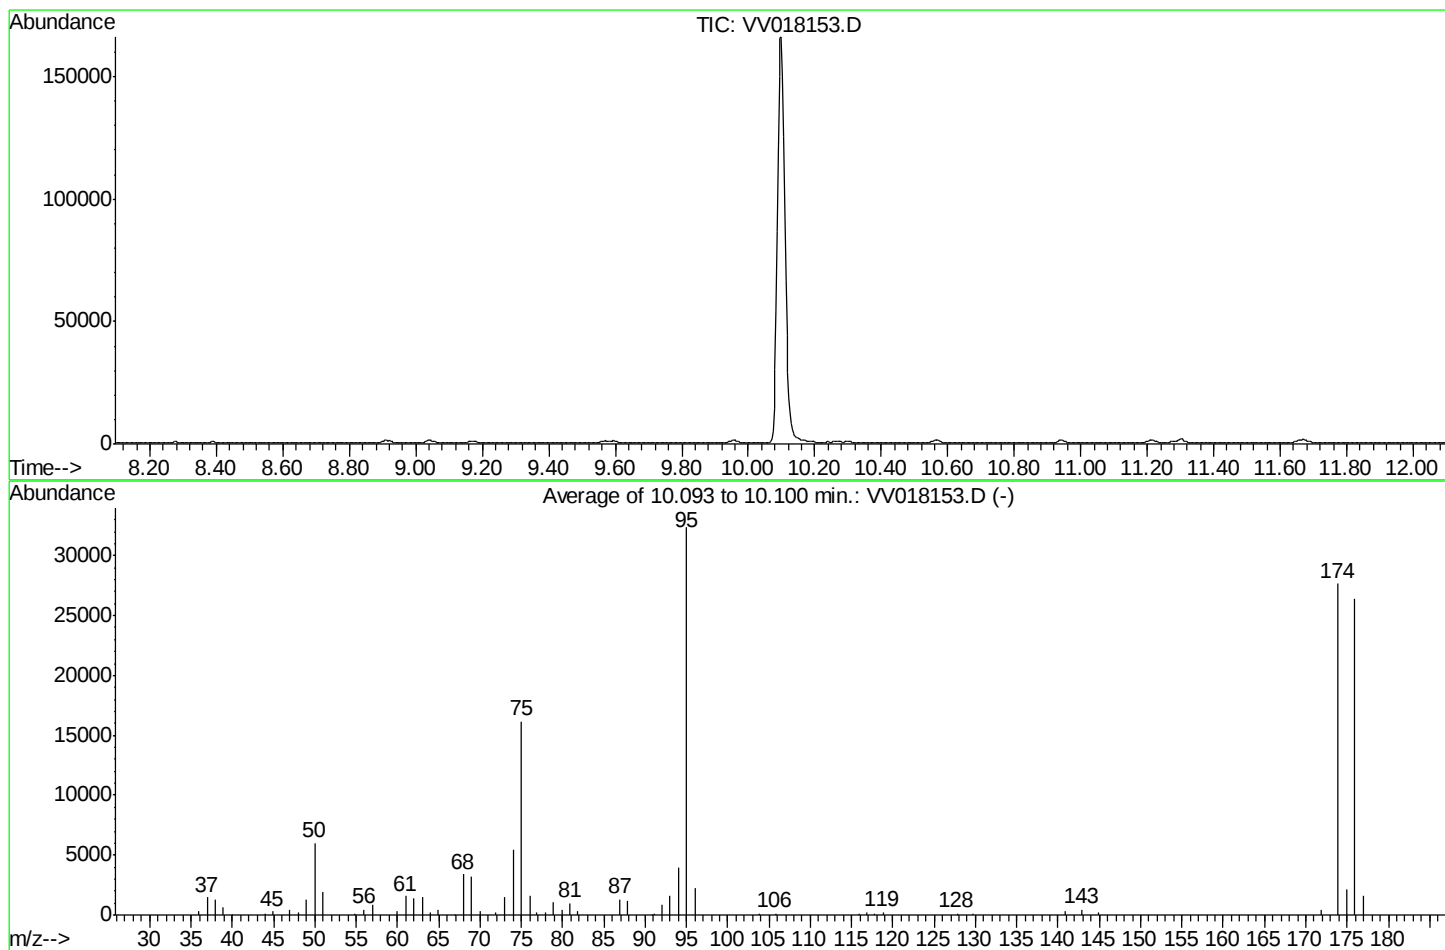

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	5988	PASS
75	95	30	80	50.0	16177	PASS
95	95	100	100	100.0	32362	PASS
96	95	5	9	6.9	2243	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.5	27656	PASS
175	174	5	9	7.9	2191	PASS
176	174	95	101	95.6	26442	PASS
177	176	5	9	6.0	1577	PASS

Scan 2790 (10.061 min): VV018153.D
BFB86

m/z	Abundance
40.00	196.0
44.00	425.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
35.90	284.0
37.00	1470.0
38.00	1233.0
38.90	629.0
39.90	208.0
44.00	554.0
44.90	321.0
47.00	422.0
48.00	196.0
49.00	1249.0
50.00	5706.0
51.00	1871.0
54.90	170.0
56.00	466.0
57.00	721.0
59.90	336.0
61.00	1515.0
62.00	1416.0
63.00	1334.0
63.90	228.0
64.90	392.0
68.00	3089.0
69.00	3041.0
70.00	334.0
72.00	199.0
73.00	1386.0
74.00	5111.0
75.00	15363.0
76.00	1446.0
76.90	190.0
78.00	186.0
78.90	952.0
79.90	351.0
80.90	1032.0
81.80	259.0
86.90	1276.0
87.90	1182.0
91.10	113.0
92.00	830.0
93.00	1493.0
94.00	3814.0
95.00	30256.0
96.00	2177.0
103.80	133.0
105.80	141.0
115.90	111.0
116.90	221.0
117.90	115.0
118.80	224.0
127.80	131.0
129.70	124.0
140.80	281.0
143.00	429.0
144.90	174.0
171.90	398.0
173.90	25216.0
174.90	2137.0
175.90	23904.0
176.90	1455.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
35.90	304.0
37.00	1501.0
38.00	1290.0
38.90	674.0
39.90	222.0
44.00	569.0
44.90	332.0
47.00	447.0
48.10	175.0
49.00	1347.0
50.00	6203.0
51.00	2026.0
54.90	158.0
55.90	482.0
57.00	851.0
59.90	342.0
61.00	1621.0
62.00	1446.0
63.00	1541.0
63.90	231.0
65.00	416.0
68.00	3483.0
69.00	3311.0
70.00	334.0
71.90	198.0
73.00	1524.0
74.00	5668.0
75.00	16696.0
76.00	1634.0
76.90	205.0
78.00	228.0
78.90	1095.0
79.90	405.0
80.90	1005.0
81.80	303.0
86.90	1333.0
87.90	1247.0
91.00	131.0
92.00	920.0
93.00	1673.0
94.00	4140.0
95.00	33448.0
96.00	2349.0
103.80	142.0
105.80	147.0
115.90	115.0
116.80	239.0
117.80	116.0
118.80	254.0
127.80	154.0
129.70	130.0
140.80	358.0
143.00	496.0
144.90	174.0
171.90	448.0
173.90	28520.0
174.90	2252.0
175.90	27280.0
176.90	1633.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86

m/z	Abundance
35.90	306.0
37.00	1393.0
38.00	1229.0
38.90	639.0
39.90	225.0
43.90	561.0
44.90	292.0
47.00	431.0
48.10	147.0
49.00	1342.0
50.00	6056.0
51.00	2003.0
54.90	125.0
55.90	464.0
57.00	907.0
60.00	328.0
61.00	1592.0
62.00	1414.0
63.00	1516.0
63.90	212.0
64.90	405.0
66.90	104.0
68.00	3543.0
69.00	3270.0
69.90	299.0
71.90	180.0
72.90	1453.0
74.00	5635.0
75.00	16472.0
76.00	1607.0
76.90	222.0
78.00	219.0
78.90	1107.0
79.90	424.0
80.90	963.0
81.80	319.0
87.00	1353.0
87.90	1236.0
90.80	146.0
92.00	951.0
93.00	1638.0
94.00	4056.0
95.00	33384.0
96.00	2204.0
103.80	141.0
105.80	145.0
116.80	249.0
117.70	123.0
118.80	252.0
127.80	155.0
129.80	121.0
140.80	389.0
142.90	491.0
144.90	149.0
171.90	421.0
173.90	29232.0
175.00	2185.0
175.90	28144.0
176.90	1644.0

Instrument :
MSVOA_V
ClientSampleId :
BFB86