

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
 Data File : VV007392.D
 Acq On : 05 Sep 2018 19:08
 Operator : SY/MD
 Sample : J4719-05 50X
 Misc : 5.0 mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE1

Quant Time: Sep 06 01:46:07 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Sep 06 01:44:11 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	513951	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	510350	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	183953	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	159811	43.53	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	87.06%
7) Chloroethane-d5	1.56	69	129886	54.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	108.02%
11) 1,1-Dichloroethene-d2	2.13	63	216909	33.54	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	67.08%
21) 2-Butanone-d5	3.96	46	235263	78.79	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	78.79%
24) Chloroform-d	4.41	84	347336	45.74	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.48%
26) 1,2-Dichloroethane-d4	5.09	65	221984	48.46	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.92%
32) Benzene-d6	5.10	84	674465	43.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	87.70%
36) 1,2-Dichloropropane-d6	6.12	67	233259	45.25	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	90.50%
41) Toluene-d8	7.36	98	542063	40.94	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	81.88%
43) trans-1,3-Dichloropropene-	7.67	79	91895	41.85	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	83.70%
47) 2-Hexanone-d5	8.14	63	161478	79.91	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	79.91%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	321356	45.64	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	91.28%
64) 1,2-Dichlorobenzene-d4	11.68	152	203905	51.58	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.16%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
59) 1,2,3-Trichloropropane	11.30	75	21257	3.984	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007392.D
Acq On : 05 Sep 2018 19:08
Operator : SY/MD
Sample : J4719-05 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE1

Quant Time: Sep 06 01:46:07 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Sep 06 01:44:11 2018
Response via : Initial Calibration

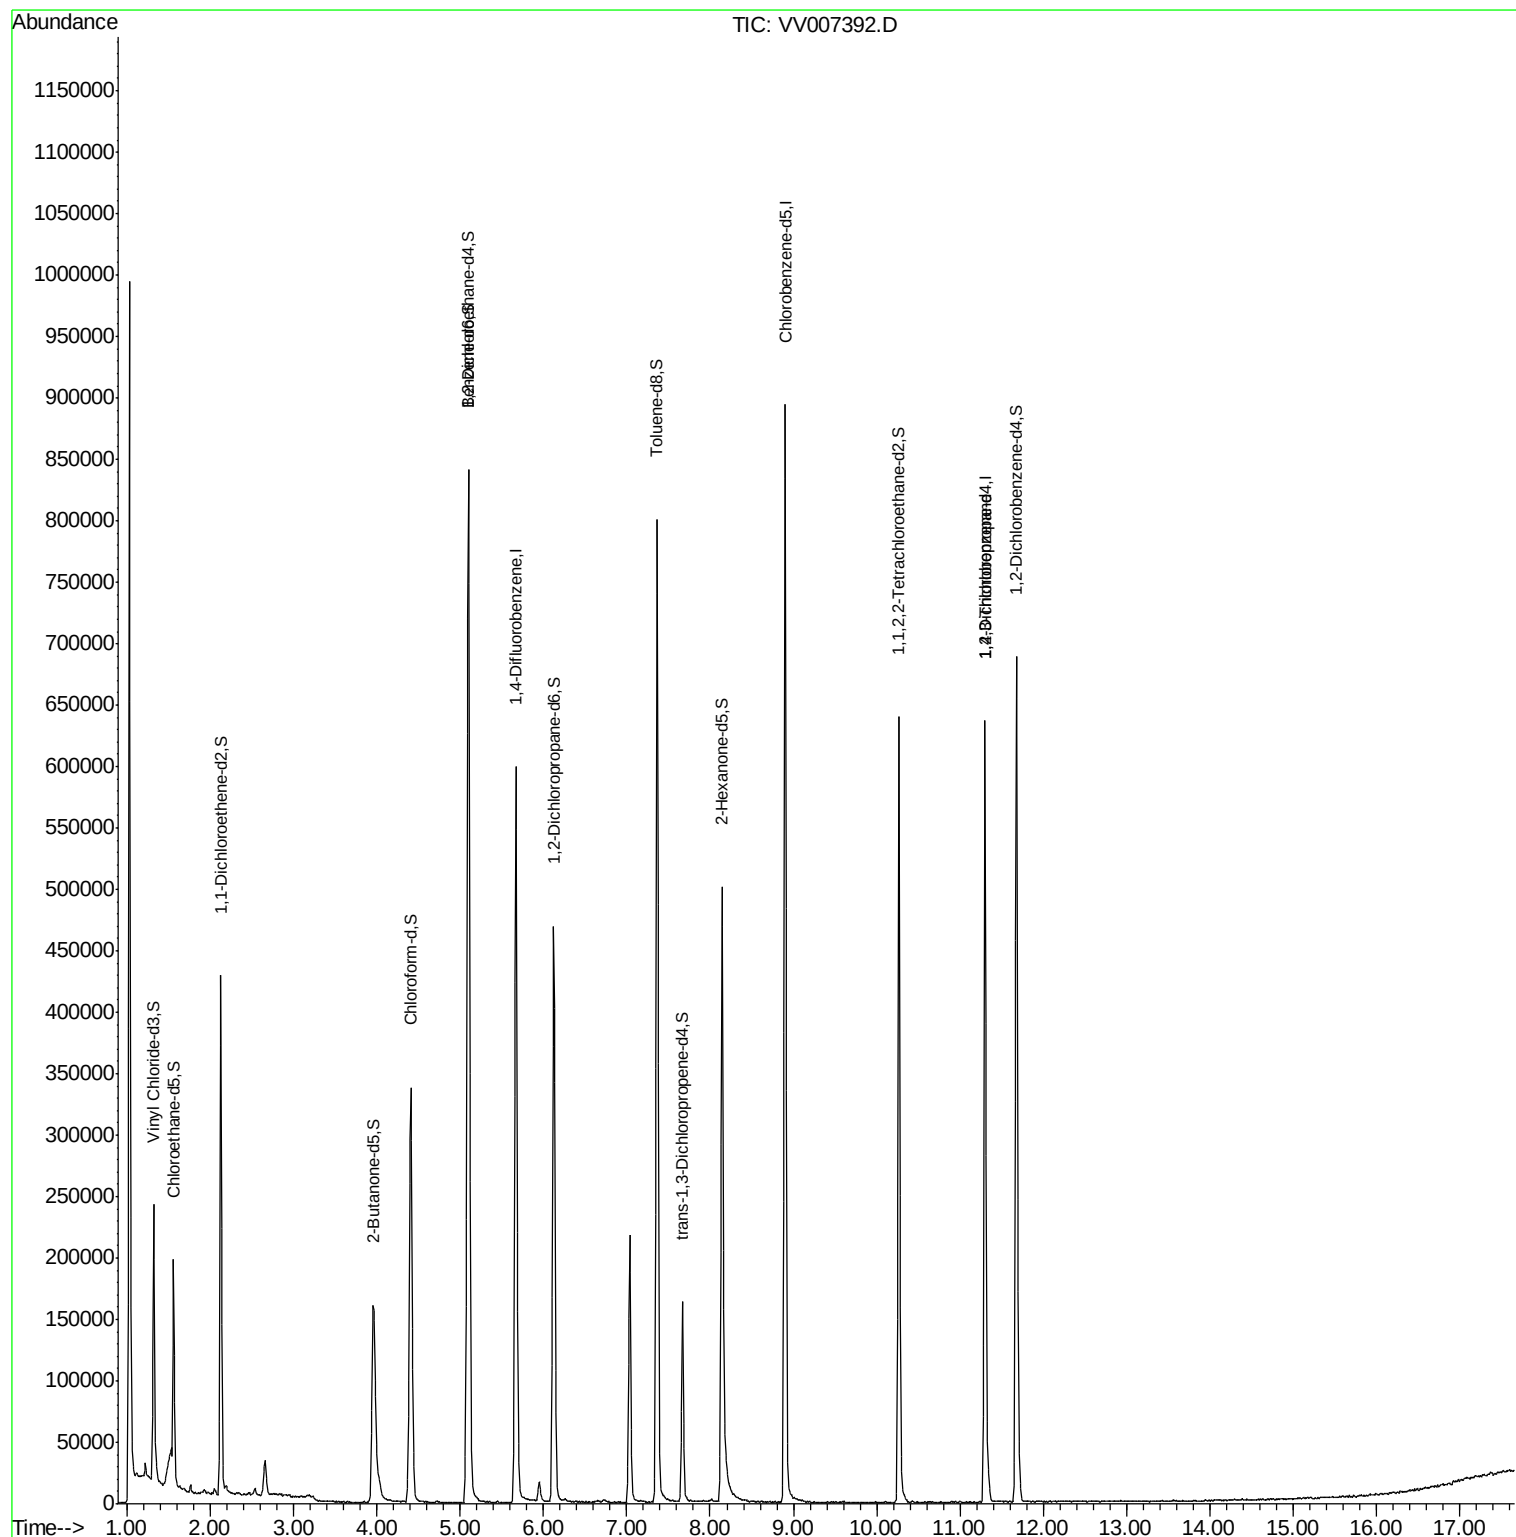

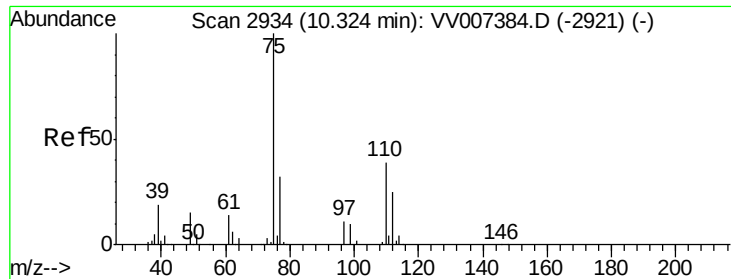

#59

1,2,3-Trichloropropane

Concen: 3.984 ug/L

RT: 11.30 min Scan# 3237

Delta R.T. 0.97 min

Lab File: VV007392.D

Acq: 05 Sep 2018 19:08

Instrument :

MSVOA_V

ClientSampleId :

BEGE1

Tgt Ion: 75 Resp: 21257

Ion Ratio Lower Upper

75 100

77 35.0 25.5 38.3

