

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007388.D
 Acq On : 05 Sep 2018 17:28
 Operator : SY/MD
 Sample : J4719-01 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.913	5	7	11	rVB	443	274	0.01%	0.002%
2	0.945	11	17	20	rBV3	613	718	0.04%	0.004%
3	1.029	28	43	66	rBV	996650	1297293	65.27%	8.091%
4	1.321	126	134	154	rVB	215002	274652	13.82%	1.713%
5	1.559	203	208	224	rVB	185283	233052	11.73%	1.453%
6	2.128	375	385	396	rBV	425430	599335	30.16%	3.738%
7	2.656	542	549	564	rVB	25210	47991	2.41%	0.299%
8	3.569	830	833	836	rBV3	661	410	0.02%	0.003%
9	3.717	876	879	883	rBV3	383	287	0.01%	0.002%
10	3.865	922	925	928	rBV2	496	393	0.02%	0.002%
11	3.961	937	955	997	rBV2	160576	517790	26.05%	3.229%
12	4.234	1037	1040	1043	rBV3	698	439	0.02%	0.003%
13	4.344	1068	1074	1075	rBV2	394	417	0.02%	0.003%
14	4.405	1075	1093	1121	rVV2	336304	804555	40.48%	5.018%
15	4.565	1140	1143	1146	rBV2	386	298	0.01%	0.002%
16	4.617	1157	1159	1162	rVB3	638	283	0.01%	0.002%
17	4.649	1165	1169	1174	rVB3	395	479	0.02%	0.003%
18	4.704	1183	1186	1188	rBV3	619	434	0.02%	0.003%
19	4.726	1188	1193	1196	rVV4	909	1126	0.06%	0.007%
20	4.742	1196	1198	1204	rVB4	997	861	0.04%	0.005%
21	4.797	1213	1215	1219	rBV3	484	291	0.01%	0.002%
22	4.881	1239	1241	1245	rVB2	567	391	0.02%	0.002%
23	4.916	1245	1252	1253	rBV2	328	306	0.02%	0.002%
24	4.961	1263	1266	1271	rVB3	379	327	0.02%	0.002%
25	5.099	1290	1309	1341	rBV2	842380	1987507	100.00%	12.395%
26	5.324	1375	1379	1382	rVB4	450	359	0.02%	0.002%
27	5.382	1392	1397	1401	rBV3	580	727	0.04%	0.005%
28	5.450	1416	1418	1422	rVB2	605	400	0.02%	0.002%
29	5.559	1447	1452	1456	rVB3	362	358	0.02%	0.002%
30	5.668	1469	1486	1524	rVV	618322	1233095	62.04%	7.690%
31	5.951	1565	1574	1593	rVB2	18059	35815	1.80%	0.223%
32	6.125	1611	1628	1653	rBV	465631	946535	47.62%	5.903%
33	6.289	1677	1679	1688	rVB9	1193	1272	0.06%	0.008%
34	6.598	1772	1775	1778	rBV4	549	471	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007388.D
 Acq On : 05 Sep 2018 17:28
 Operator : SY/MD
 Sample : J4719-01 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.726	1808	1815	1825	rVB4	2937	4390	0.22%	0.027%
36	6.832	1842	1848	1849	rBV2	506	392	0.02%	0.002%
37	6.900	1864	1869	1871	rBV3	392	309	0.02%	0.002%
38	6.935	1876	1880	1882	rVB4	428	291	0.01%	0.002%
39	7.035	1898	1911	1933	rBV	220956	396557	19.95%	2.473%
40	7.167	1948	1952	1956	rBV5	938	833	0.04%	0.005%
41	7.218	1964	1968	1971	rBV4	607	572	0.03%	0.004%
42	7.253	1976	1979	1981	rBV2	591	359	0.02%	0.002%
43	7.282	1984	1988	1994	rVB3	761	529	0.03%	0.003%
44	7.311	1994	1997	1999	rBV4	597	382	0.02%	0.002%
45	7.366	1999	2014	2031	rBV	819113	1415179	71.20%	8.826%
46	7.668	2096	2108	2130	rBV	168642	283907	14.28%	1.771%
47	7.864	2165	2169	2173	rBV4	800	883	0.04%	0.006%
48	8.144	2242	2256	2295	rBV2	498150	1029864	51.82%	6.423%
49	8.533	2374	2377	2380	rBV2	468	349	0.02%	0.002%
50	8.636	2406	2409	2411	rBV3	523	354	0.02%	0.002%
51	8.700	2425	2429	2433	rBV3	743	618	0.03%	0.004%
52	8.758	2441	2447	2450	rBV3	322	354	0.02%	0.002%
53	8.900	2478	2491	2522	rBV	918125	1506500	75.80%	9.395%
54	9.173	2573	2576	2578	rVB2	495	266	0.01%	0.002%
55	9.192	2578	2582	2586	rBV2	888	733	0.04%	0.005%
56	9.221	2589	2591	2595	rVB2	677	421	0.02%	0.003%
57	9.244	2595	2598	2599	rBV	748	369	0.02%	0.002%
58	9.282	2607	2610	2613	rVB2	501	309	0.02%	0.002%
59	9.305	2614	2617	2622	rVB2	394	328	0.02%	0.002%
60	9.334	2622	2626	2630	rVB2	797	479	0.02%	0.003%
61	9.372	2633	2638	2641	rBV3	420	404	0.02%	0.003%
62	9.427	2652	2655	2660	rVB3	415	379	0.02%	0.002%
63	9.456	2660	2664	2667	rVB3	313	274	0.01%	0.002%
64	9.488	2669	2674	2678	rBV2	449	468	0.02%	0.003%
65	9.597	2705	2708	2712	rBV3	631	572	0.03%	0.004%
66	9.716	2740	2745	2747	rBV3	688	637	0.03%	0.004%
67	9.829	2777	2780	2784	rBV4	439	383	0.02%	0.002%
68	9.919	2805	2808	2811	rVB2	456	278	0.01%	0.002%
69	9.986	2824	2829	2833	rVB2	457	546	0.03%	0.003%
70	10.041	2843	2846	2849	rBV2	454	333	0.02%	0.002%
71	10.105	2862	2866	2872	rVB3	641	635	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007388.D
 Acq On : 05 Sep 2018 17:28
 Operator : SY/MD
 Sample : J4719-01 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.138	2872	2876	2878	rBV2	339	304	0.02%	0.002%
73	10.266	2903	2916	2949	rVV	633491	1043020	52.48%	6.505%
74	10.392	2952	2955	2961	rVB3	647	517	0.03%	0.003%
75	10.427	2962	2966	2973	rVB4	1070	1482	0.07%	0.009%
76	10.462	2973	2977	2984	rVB2	757	715	0.04%	0.004%
77	10.494	2984	2987	2990	rBV2	383	376	0.02%	0.002%
78	10.514	2990	2993	3002	rVB3	490	484	0.02%	0.003%
79	10.594	3015	3018	3020	rBV2	435	307	0.02%	0.002%
80	10.748	3062	3066	3067	rBV2	390	269	0.01%	0.002%
81	10.903	3110	3114	3117	rBV3	864	628	0.03%	0.004%
82	10.929	3120	3122	3126	rVB2	581	337	0.02%	0.002%
83	10.951	3126	3129	3132	rBV2	360	358	0.02%	0.002%
84	11.048	3153	3159	3162	rBV3	412	386	0.02%	0.002%
85	11.134	3183	3186	3191	rBV3	393	367	0.02%	0.002%
86	11.231	3214	3216	3222	rVB5	1463	1164	0.06%	0.007%
87	11.302	3225	3238	3266	rVV	666991	1128014	56.76%	7.035%
88	11.678	3342	3355	3377	rBV	711622	1210282	60.89%	7.548%
89	11.858	3407	3411	3415	rBV3	560	501	0.03%	0.003%
90	11.906	3423	3426	3429	rBV3	502	426	0.02%	0.003%
91	11.951	3438	3440	3444	rBV2	544	352	0.02%	0.002%
92	12.031	3463	3465	3473	rVB5	646	481	0.02%	0.003%
93	12.260	3533	3536	3538	rBV2	524	280	0.01%	0.002%
94	12.356	3563	3566	3571	rBV4	471	465	0.02%	0.003%
95	12.411	3581	3583	3588	rVV4	520	457	0.02%	0.003%
96	12.633	3650	3652	3656	rBV2	405	339	0.02%	0.002%
97	12.925	3741	3743	3745	rBV	677	436	0.02%	0.003%
98	13.131	3803	3807	3809	rBV2	612	473	0.02%	0.003%
99	13.549	3934	3937	3939	rBV2	1154	721	0.04%	0.004%
100	14.417	4203	4207	4211	rBV5	855	997	0.05%	0.006%


Sum of corrected areas: 16034315

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090518\
Data File : VV007388.D
Acq On : 05 Sep 2018 17:28
Operator : SY/MD
Sample : J4719-01 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

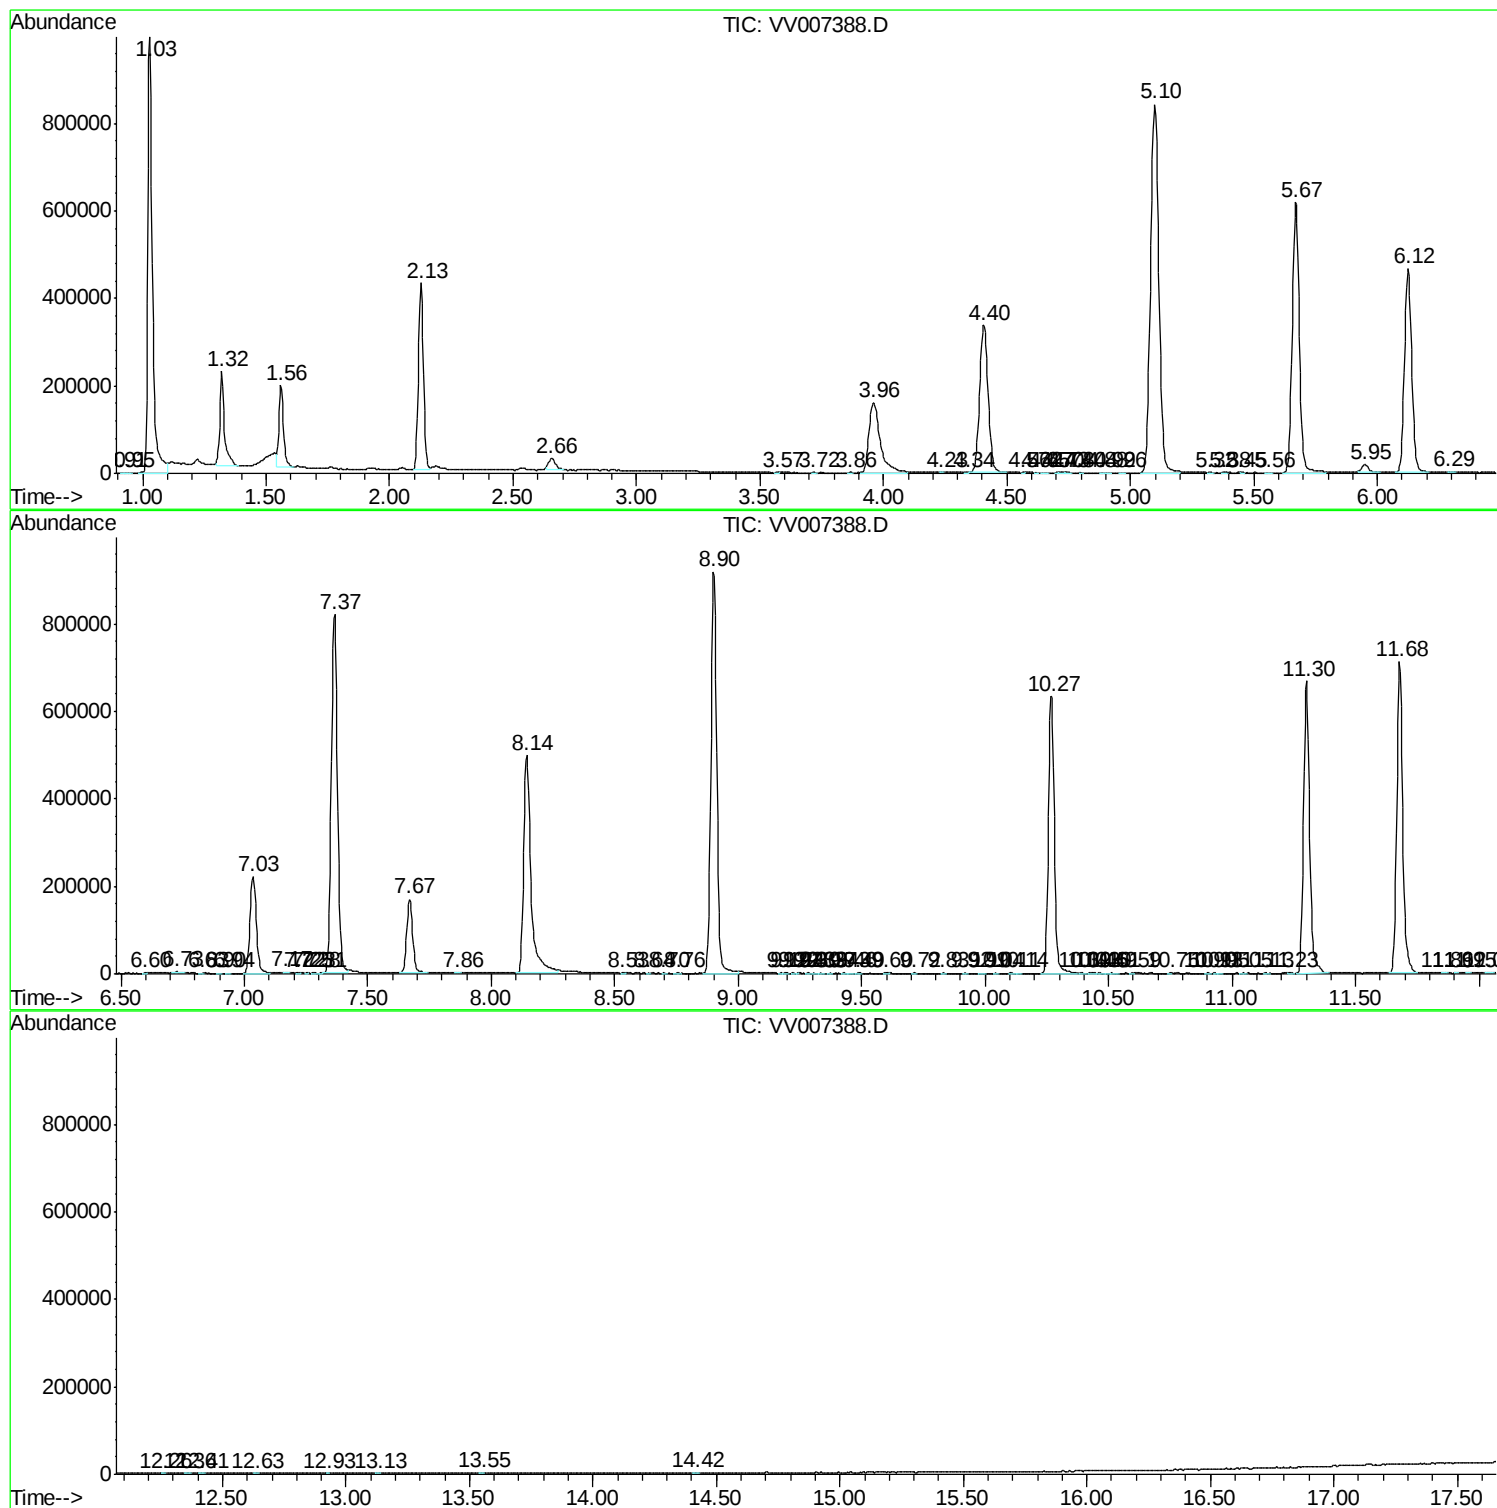

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007388.D
Acq On : 05 Sep 2018 17:28
Operator : SY/MD
Sample : J4719-01 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGD7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007388.D
Acq On : 05 Sep 2018 17:28
Operator : SY/MD
Sample : J4719-01 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc