

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007391.D
 Acq On : 05 Sep 2018 18:43
 Operator : SY/MD
 Sample : J4719-04 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.028	24	43	66	rBV	1218487	1536675	80.09%	9.706%
2	1.321	126	134	153	rVB	198190	253307	13.20%	1.600%
3	1.556	202	207	225	rVB	180592	229752	11.97%	1.451%
4	2.125	374	384	395	rBV	414647	581281	30.29%	3.672%
5	2.655	540	549	570	rVB2	21396	48833	2.55%	0.308%
6	3.376	771	773	777	rVV3	807	437	0.02%	0.003%
7	3.392	777	778	781	rVB3	616	296	0.02%	0.002%
8	3.559	828	830	834	rVB4	515	310	0.02%	0.002%
9	3.591	834	840	843	rBV3	765	764	0.04%	0.005%
10	3.710	873	877	883	rBV2	281	407	0.02%	0.003%
11	3.739	883	886	888	rVV3	593	408	0.02%	0.003%
12	3.768	892	895	899	rVB2	489	343	0.02%	0.002%
13	3.797	899	904	907	rBV2	409	492	0.03%	0.003%
14	3.961	935	955	999	rBV2	164738	514847	26.83%	3.252%
15	4.405	1076	1093	1119	rBV	325504	776591	40.47%	4.905%
16	4.552	1137	1139	1143	rVB4	677	425	0.02%	0.003%
17	4.617	1156	1159	1162	rBV3	361	344	0.02%	0.002%
18	4.707	1182	1187	1188	rBV3	648	448	0.02%	0.003%
19	4.736	1192	1196	1198	rVV3	874	704	0.04%	0.004%
20	4.765	1202	1205	1209	rVB2	554	406	0.02%	0.003%
21	4.803	1213	1217	1221	rVB3	512	333	0.02%	0.002%
22	4.906	1246	1249	1253	rBV	430	344	0.02%	0.002%
23	4.932	1253	1257	1260	rBV2	333	272	0.01%	0.002%
24	5.019	1280	1284	1290	rBV3	395	412	0.02%	0.003%
25	5.099	1290	1309	1350	rBV2	810098	1918756	100.00%	12.119%
26	5.443	1411	1416	1417	rBV4	382	359	0.02%	0.002%
27	5.459	1417	1421	1424	rVB5	994	671	0.03%	0.004%
28	5.507	1433	1436	1441	rVV4	506	490	0.03%	0.003%
29	5.668	1469	1486	1507	rBV	588777	1162517	60.59%	7.343%
30	5.951	1563	1574	1587	rVB3	14650	29566	1.54%	0.187%
31	6.125	1612	1628	1656	rBV	451621	905208	47.18%	5.718%
32	6.324	1688	1690	1694	rVB2	662	343	0.02%	0.002%
33	6.347	1694	1697	1699	rBV2	545	375	0.02%	0.002%
34	6.392	1707	1711	1714	rBV	479	366	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007391.D
 Acq On : 05 Sep 2018 18:43
 Operator : SY/MD
 Sample : J4719-04 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.427	1719	1722	1725	rVB2	609	394	0.02%	0.002%
36	6.498	1740	1744	1747	rBV4	596	469	0.02%	0.003%
37	6.536	1754	1756	1758	rVB2	635	274	0.01%	0.002%
38	6.646	1787	1790	1792	rBV2	706	547	0.03%	0.003%
39	6.726	1807	1815	1826	rVB4	2829	4782	0.25%	0.030%
40	6.829	1843	1847	1853	rVB6	524	598	0.03%	0.004%
41	6.938	1879	1881	1886	rBV2	570	476	0.02%	0.003%
42	6.967	1886	1890	1894	rVB3	641	522	0.03%	0.003%
43	7.035	1898	1911	1931	rBV	211180	376629	19.63%	2.379%
44	7.170	1951	1953	1957	rVB3	979	609	0.03%	0.004%
45	7.237	1968	1974	1980	rBV6	1068	1675	0.09%	0.011%
46	7.276	1983	1986	1987	rBV2	463	285	0.01%	0.002%
47	7.363	1999	2013	2047	rBV	773780	1362582	71.01%	8.606%
48	7.549	2068	2071	2075	rBV4	814	646	0.03%	0.004%
49	7.604	2084	2088	2090	rBV3	788	622	0.03%	0.004%
50	7.668	2096	2108	2128	rBV	156372	267154	13.92%	1.687%
51	8.022	2208	2218	2231	rVB3	30308	52112	2.72%	0.329%
52	8.144	2243	2256	2292	rBV2	505838	1014724	52.88%	6.409%
53	8.510	2366	2370	2373	rBV3	911	870	0.05%	0.005%
54	8.543	2378	2380	2383	rVV2	675	482	0.03%	0.003%
55	8.620	2401	2404	2407	rBV2	670	506	0.03%	0.003%
56	8.642	2407	2411	2415	rVB4	495	487	0.03%	0.003%
57	8.687	2422	2425	2428	rBV4	582	416	0.02%	0.003%
58	8.777	2449	2453	2455	rBV	451	362	0.02%	0.002%
59	8.790	2455	2457	2460	rVV2	508	329	0.02%	0.002%
60	8.806	2460	2462	2467	rVB3	588	390	0.02%	0.002%
61	8.832	2467	2470	2472	rBV2	596	418	0.02%	0.003%
62	8.900	2478	2491	2518	rBV	869828	1423485	74.19%	8.991%
63	9.186	2576	2580	2582	rBV2	1013	914	0.05%	0.006%
64	9.237	2591	2596	2601	rBV2	325	347	0.02%	0.002%
65	9.301	2613	2616	2618	rBV3	521	406	0.02%	0.003%
66	9.340	2625	2628	2631	rBV2	450	324	0.02%	0.002%
67	9.359	2631	2634	2636	rBV2	367	274	0.01%	0.002%
68	9.430	2651	2656	2658	rBV4	717	631	0.03%	0.004%
69	9.755	2754	2757	2763	rBV4	407	349	0.02%	0.002%
70	9.816	2772	2776	2777	rBV2	648	464	0.02%	0.003%
71	9.893	2797	2800	2808	rVB4	456	549	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007391.D
 Acq On : 05 Sep 2018 18:43
 Operator : SY/MD
 Sample : J4719-04 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.018	2835	2839	2843	rVB3	609	478	0.02%	0.003%
73	10.153	2877	2881	2884	rVB2	629	439	0.02%	0.003%
74	10.266	2901	2916	2952	rBV	630593	1020309	53.18%	6.445%
75	10.398	2952	2957	2961	rBV4	311	385	0.02%	0.002%
76	10.424	2961	2965	2970	rVV4	534	459	0.02%	0.003%
77	10.465	2975	2978	2988	rVB5	488	595	0.03%	0.004%
78	10.665	3034	3040	3043	rBV4	482	496	0.03%	0.003%
79	10.768	3068	3072	3074	rBV2	481	397	0.02%	0.003%
80	10.777	3074	3075	3080	rVB2	795	453	0.02%	0.003%
81	10.806	3080	3084	3088	rBV2	543	560	0.03%	0.004%
82	11.179	3198	3200	3204	rVB2	540	384	0.02%	0.002%
83	11.215	3204	3211	3213	rBV	547	533	0.03%	0.003%
84	11.234	3213	3217	3221	rVB3	683	746	0.04%	0.005%
85	11.301	3223	3238	3264	rBV	659267	1104991	57.59%	6.979%
86	11.526	3306	3308	3313	rVB2	463	277	0.01%	0.002%
87	11.678	3342	3355	3382	rBV	715484	1203620	62.73%	7.602%
88	12.012	3456	3459	3463	rVB2	690	435	0.02%	0.003%
89	12.324	3554	3556	3562	rVB3	439	357	0.02%	0.002%
90	12.353	3562	3565	3569	rBV4	396	316	0.02%	0.002%
91	12.385	3570	3575	3578	rBV3	564	562	0.03%	0.004%
92	12.613	3643	3646	3649	rBV3	528	398	0.02%	0.003%
93	12.719	3676	3679	3683	rVB3	679	453	0.02%	0.003%
94	12.867	3723	3725	3728	rBV4	535	302	0.02%	0.002%
95	12.932	3742	3745	3750	rBV5	1018	913	0.05%	0.006%
96	13.800	4013	4015	4019	rBV3	766	387	0.02%	0.002%
97	13.893	4040	4044	4046	rBV3	819	562	0.03%	0.004%
98	14.153	4122	4125	4131	rBV6	1228	1504	0.08%	0.009%
99	14.957	4373	4375	4378	rBV3	1233	636	0.03%	0.004%
100	16.549	4867	4870	4873	rVB	11380	6042	0.31%	0.038%


Sum of corrected areas: 15832174

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090518\
Data File : VV007391.D
Acq On : 05 Sep 2018 18:43
Operator : SY/MD
Sample : J4719-04 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

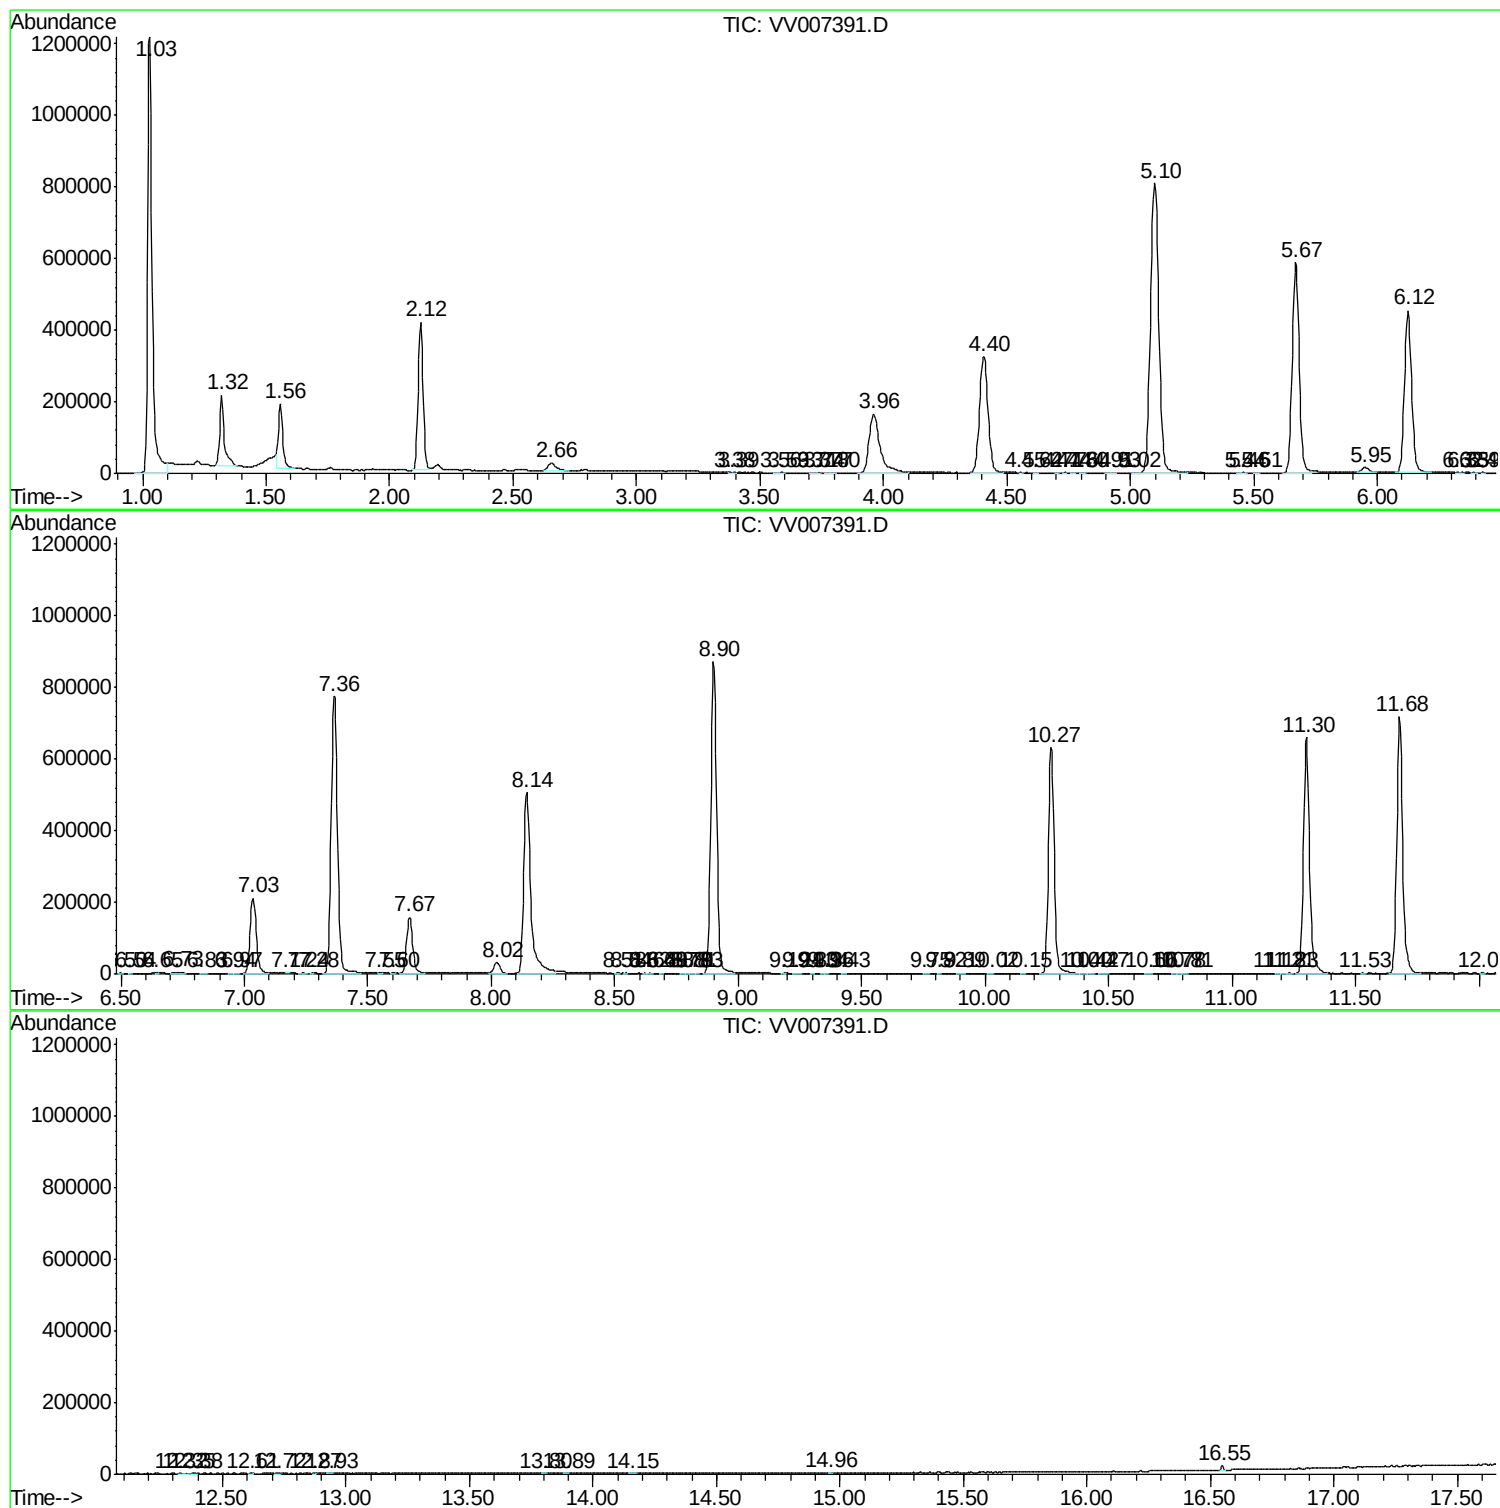

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007391.D
Acq On : 05 Sep 2018 18:43
Operator : SY/MD
Sample : J4719-04 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007391.D
Acq On : 05 Sep 2018 18:43
Operator : SY/MD
Sample : J4719-04 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc