

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007393.D
 Acq On : 05 Sep 2018 19:33
 Operator : SY/MD
 Sample : J4719-06 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.026	28	42	64	rBV	1101576	1383620	74.90%	9.045%
2	1.321	126	134	161	rVB	194639	273175	14.79%	1.786%
3	1.559	203	208	225	rVB	174919	211709	11.46%	1.384%
4	2.125	375	384	396	rBV	396370	555164	30.05%	3.629%
5	2.656	538	549	564	rBV	24442	54007	2.92%	0.353%
6	3.279	741	743	749	rVB5	1545	1111	0.06%	0.007%
7	3.308	750	752	754	rBV3	518	289	0.02%	0.002%
8	3.521	814	818	822	rBV2	497	478	0.03%	0.003%
9	3.630	848	852	853	rBV	588	405	0.02%	0.003%
10	3.877	925	929	933	rBV2	303	287	0.02%	0.002%
11	3.958	937	954	998	rBV2	165094	501494	27.15%	3.278%
12	4.340	1071	1073	1075	rBV2	531	290	0.02%	0.002%
13	4.405	1075	1093	1121	rVV	309384	752677	40.74%	4.920%
14	4.562	1140	1142	1149	rVB3	953	817	0.04%	0.005%
15	4.604	1153	1155	1159	rVB2	692	455	0.02%	0.003%
16	4.656	1167	1171	1174	rBV2	697	677	0.04%	0.004%
17	4.720	1189	1191	1193	rBV2	708	402	0.02%	0.003%
18	4.807	1212	1218	1221	rVB2	429	460	0.02%	0.003%
19	4.849	1228	1231	1234	rBV2	429	354	0.02%	0.002%
20	4.913	1249	1251	1256	rVB2	424	285	0.02%	0.002%
21	4.958	1256	1265	1269	rBV2	434	536	0.03%	0.004%
22	5.099	1287	1309	1343	rBV2	782657	1847410	100.00%	12.077%
23	5.276	1362	1364	1370	rVB4	570	523	0.03%	0.003%
24	5.385	1395	1398	1401	rBV2	365	337	0.02%	0.002%
25	5.443	1414	1416	1419	rBV2	482	330	0.02%	0.002%
26	5.601	1461	1465	1470	rVB3	428	346	0.02%	0.002%
27	5.668	1470	1486	1516	rBV	560031	1115397	60.38%	7.291%
28	5.951	1562	1574	1586	rVB2	12985	24161	1.31%	0.158%
29	6.038	1598	1601	1605	rBV4	879	786	0.04%	0.005%
30	6.125	1612	1628	1653	rBV	434399	883363	47.82%	5.775%
31	6.369	1702	1704	1706	rBV3	520	324	0.02%	0.002%
32	6.395	1709	1712	1714	rBV2	562	333	0.02%	0.002%
33	6.572	1764	1767	1774	rBV3	456	535	0.03%	0.003%
34	6.649	1780	1791	1800	rBV7	1684	3861	0.21%	0.025%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007393.D
 Acq On : 05 Sep 2018 19:33
 Operator : SY/MD
 Sample : J4719-06 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.723	1805	1814	1828	rVB4	2816	6167	0.33%	0.040%
36	6.945	1876	1883	1885	rBV3	432	418	0.02%	0.003%
37	6.971	1888	1891	1897	rVB4	534	497	0.03%	0.003%
38	7.035	1897	1911	1935	rBV	199740	363137	19.66%	2.374%
39	7.363	1998	2013	2042	rBV	736791	1296307	70.17%	8.474%
40	7.575	2077	2079	2085	rVB5	880	705	0.04%	0.005%
41	7.668	2095	2108	2131	rBV	151616	259564	14.05%	1.697%
42	7.974	2201	2203	2205	rBV	539	340	0.02%	0.002%
43	7.993	2205	2209	2211	rVV3	1155	905	0.05%	0.006%
44	8.022	2214	2218	2226	rVB6	1405	1844	0.10%	0.012%
45	8.141	2241	2255	2295	rBV2	524204	1039584	56.27%	6.796%
46	8.501	2364	2367	2369	rVB3	648	355	0.02%	0.002%
47	8.607	2397	2400	2403	rBV2	359	271	0.01%	0.002%
48	8.745	2437	2443	2444	rBV5	565	469	0.03%	0.003%
49	8.768	2446	2450	2453	rVB3	370	366	0.02%	0.002%
50	8.900	2477	2491	2515	rBV	837782	1373406	74.34%	8.978%
51	9.099	2551	2553	2555	rBV2	699	286	0.02%	0.002%
52	9.331	2620	2625	2627	rBV2	437	418	0.02%	0.003%
53	9.356	2630	2633	2636	rVB3	422	268	0.01%	0.002%
54	9.414	2647	2651	2655	rBV2	581	382	0.02%	0.002%
55	9.466	2663	2667	2673	rVB3	479	419	0.02%	0.003%
56	9.543	2688	2691	2697	rBV3	456	282	0.02%	0.002%
57	9.601	2707	2709	2714	rVB2	616	363	0.02%	0.002%
58	9.697	2736	2739	2741	rBV2	473	354	0.02%	0.002%
59	9.736	2746	2751	2755	rBV4	446	403	0.02%	0.003%
60	9.813	2772	2775	2781	rVB2	442	411	0.02%	0.003%
61	9.861	2786	2790	2792	rBV2	444	270	0.01%	0.002%
62	10.032	2840	2843	2845	rBV	410	311	0.02%	0.002%
63	10.131	2870	2874	2879	rBV3	545	558	0.03%	0.004%
64	10.160	2879	2883	2885	rVV2	402	304	0.02%	0.002%
65	10.176	2885	2888	2891	rBV2	429	281	0.02%	0.002%
66	10.266	2903	2916	2949	rBV	624852	1025575	55.51%	6.704%
67	10.430	2959	2967	2972	rBV3	855	1485	0.08%	0.010%
68	10.552	3003	3005	3009	rVV2	358	283	0.02%	0.002%
69	10.630	3026	3029	3032	rBV2	693	362	0.02%	0.002%
70	10.758	3064	3069	3072	rVV2	506	402	0.02%	0.003%
71	10.835	3087	3093	3095	rBV2	400	404	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007393.D
 Acq On : 05 Sep 2018 19:33
 Operator : SY/MD
 Sample : J4719-06 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.848	3095	3097	3099	rVV2	510	330	0.02%	0.002%
73	10.877	3102	3106	3111	rVV3	436	425	0.02%	0.003%
74	10.903	3111	3114	3118	rVV4	627	575	0.03%	0.004%
75	10.958	3126	3131	3135	rVB3	423	500	0.03%	0.003%
76	11.077	3165	3168	3172	rBV3	532	519	0.03%	0.003%
77	11.154	3187	3192	3195	rBV3	597	562	0.03%	0.004%
78	11.234	3214	3217	3220	rVB2	453	345	0.02%	0.002%
79	11.302	3224	3238	3265	rBV	658682	1088152	58.90%	7.113%
80	11.433	3274	3279	3281	rVB4	426	348	0.02%	0.002%
81	11.543	3309	3313	3319	rBV3	611	608	0.03%	0.004%
82	11.614	3332	3335	3340	rVB4	636	447	0.02%	0.003%
83	11.678	3341	3355	3379	rBV	708038	1201062	65.01%	7.851%
84	11.826	3398	3401	3403	rBV3	539	330	0.02%	0.002%
85	12.102	3483	3487	3491	rBV5	457	443	0.02%	0.003%
86	12.257	3533	3535	3540	rVB2	764	559	0.03%	0.004%
87	12.295	3540	3547	3549	rBV2	1091	967	0.05%	0.006%
88	12.520	3614	3617	3620	rVB3	550	297	0.02%	0.002%
89	12.543	3622	3624	3627	rBV3	680	488	0.03%	0.003%
90	12.617	3644	3647	3649	rBV3	458	323	0.02%	0.002%
91	12.655	3656	3659	3665	rVB4	564	610	0.03%	0.004%
92	12.932	3741	3745	3749	rBV7	703	843	0.05%	0.006%
93	13.109	3795	3800	3806	rBV5	620	787	0.04%	0.005%
94	13.147	3809	3812	3815	rBV2	622	519	0.03%	0.003%
95	13.353	3873	3876	3877	rBV2	571	320	0.02%	0.002%
96	13.678	3975	3977	3979	rBV	545	330	0.02%	0.002%
97	13.752	3998	4000	4004	rVB3	824	404	0.02%	0.003%
98	13.970	4063	4068	4070	rBV3	657	594	0.03%	0.004%
99	14.411	4203	4205	4208	rBV2	953	741	0.04%	0.005%
100	14.523	4238	4240	4242	rBV3	720	333	0.02%	0.002%


Sum of corrected areas: 15297315

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090518\
Data File : VV007393.D
Acq On : 05 Sep 2018 19:33
Operator : SY/MD
Sample : J4719-06 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

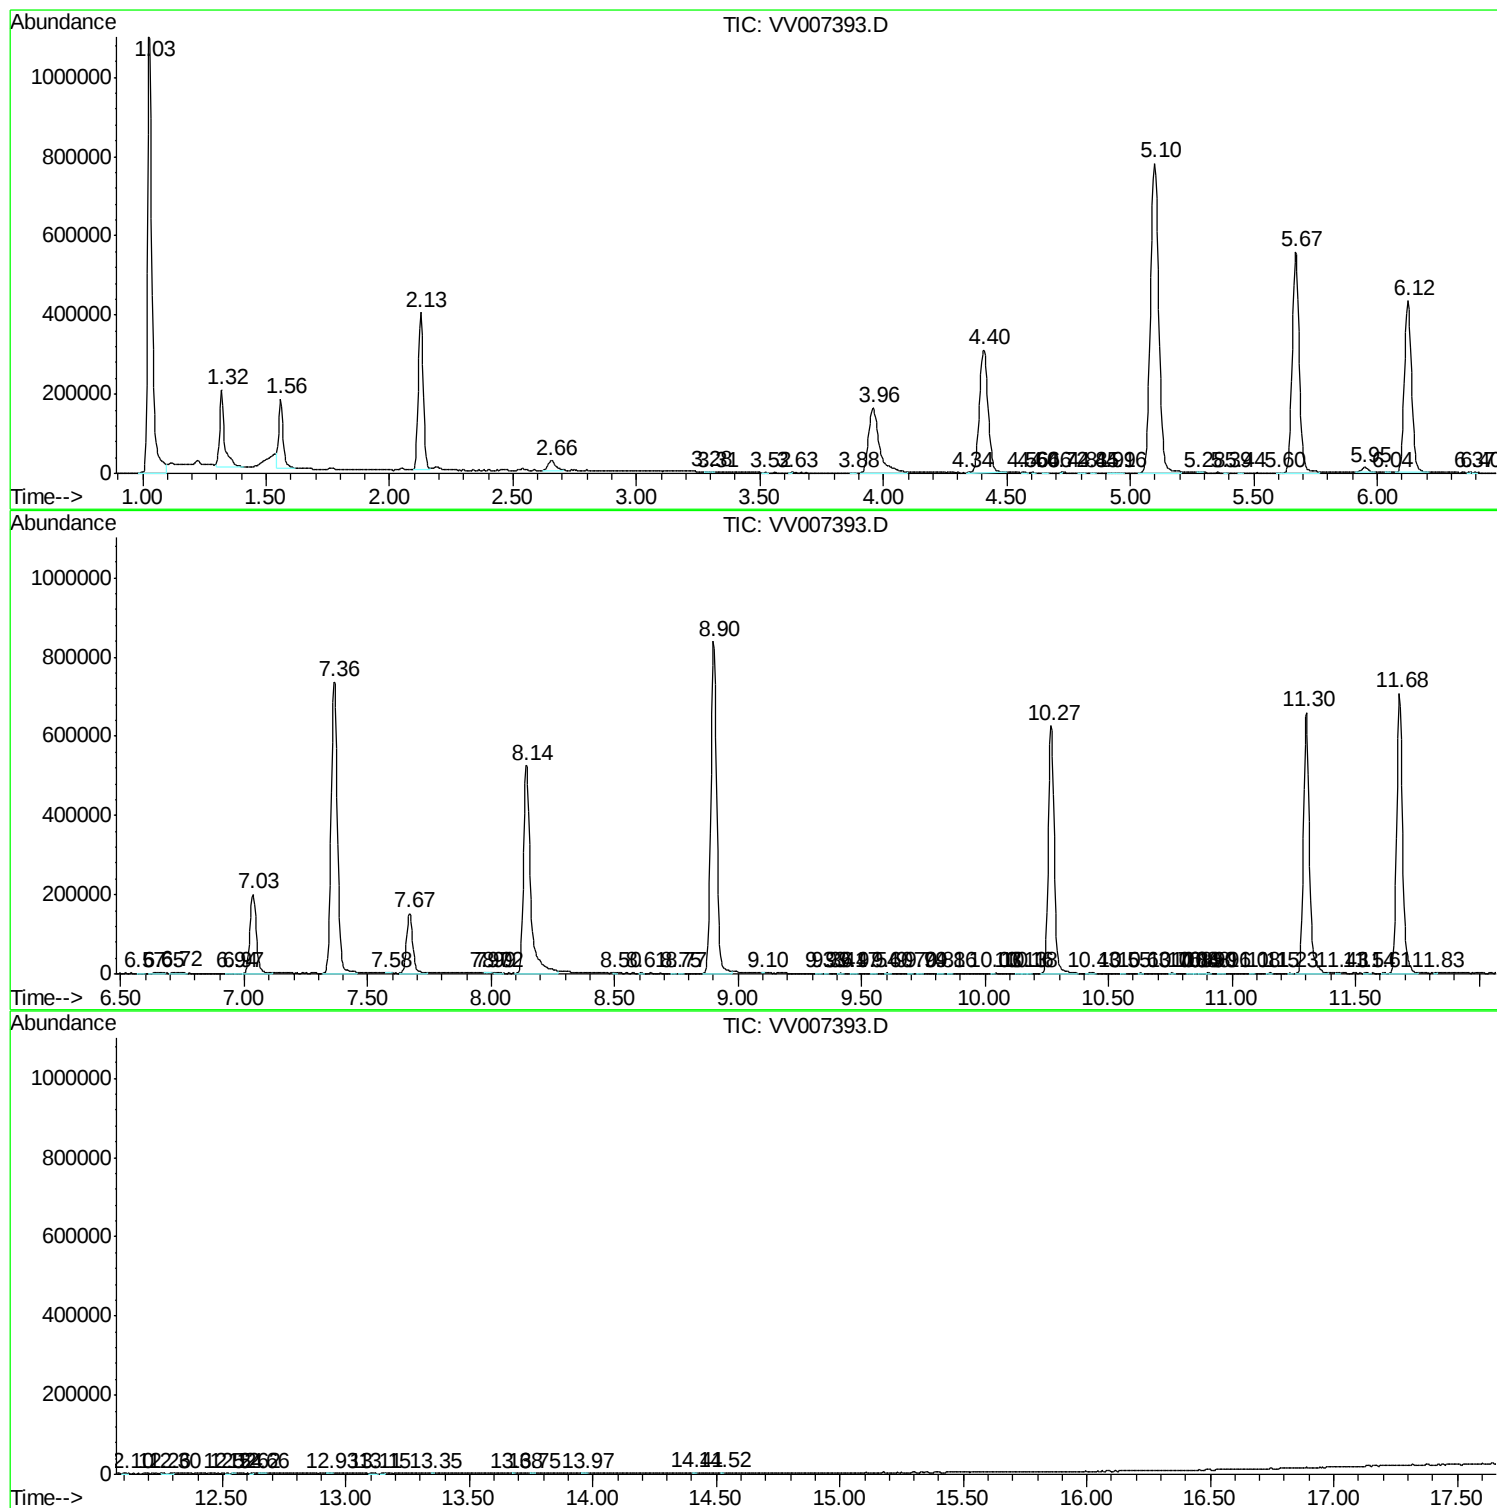

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007393.D
Acq On : 05 Sep 2018 19:33
Operator : SY/MD
Sample : J4719-06 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV090518\
Data File : VV007393.D
Acq On : 05 Sep 2018 19:33
Operator : SY/MD
Sample : J4719-06 50X
Misc : 5.0 mL/MSV0A_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
BEGE2

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc