

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007397.D
 Acq On : 05 Sep 2018 21:13
 Operator : SY/MD
 Sample : J4719-10 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.939	10	15	17	rBV	372	340	0.002%	0.0002%
2	1.029	27	43	65	rBV	1034816	1333357	70.13%	8.702%
3	1.321	126	134	153	rVB	201063	257063	13.52%	1.678%
4	1.556	202	207	223	rVB	185611	235099	12.36%	1.534%
5	2.125	374	384	396	rBV	412182	575151	30.25%	3.754%
6	3.460	796	799	800	rBV	502	263	0.01%	0.0002%
7	3.498	809	811	814	rBV2	463	302	0.02%	0.0002%
8	3.646	854	857	858	rBV2	538	292	0.02%	0.0002%
9	3.669	863	864	867	rVV	515	269	0.01%	0.0002%
10	3.685	867	869	872	rVV2	549	438	0.02%	0.0003%
11	3.759	887	892	895	rBV4	574	563	0.03%	0.0004%
12	3.961	936	955	1005	rVV2	154382	503099	26.46%	3.284%
13	4.405	1075	1093	1122	rBV	326745	778036	40.92%	5.078%
14	4.578	1145	1147	1150	rVB3	682	321	0.02%	0.0002%
15	4.662	1170	1173	1177	rBV4	419	322	0.02%	0.0002%
16	4.697	1182	1184	1186	rBV3	447	285	0.01%	0.0002%
17	4.775	1205	1208	1211	rBV	363	273	0.01%	0.0002%
18	4.855	1230	1233	1237	rVV3	533	393	0.02%	0.0003%
19	4.968	1261	1268	1272	rBV3	538	513	0.03%	0.0003%
20	5.096	1289	1308	1338	rBV2	810839	1901397	100.00%	12.410%
21	5.402	1400	1403	1405	rVV2	380	275	0.01%	0.0002%
22	5.411	1405	1406	1412	rVB2	589	362	0.02%	0.0002%
23	5.447	1412	1417	1424	rVB5	913	1241	0.07%	0.0008%
24	5.572	1451	1456	1461	rBV4	530	525	0.03%	0.0003%
25	5.668	1471	1486	1511	rBV	566009	1125593	59.20%	7.346%
26	5.948	1562	1573	1586	rBV3	12943	27284	1.43%	0.178%
27	6.035	1597	1600	1604	rBV2	470	451	0.02%	0.0003%
28	6.070	1607	1611	1612	rBV2	610	397	0.02%	0.0003%
29	6.125	1612	1628	1647	rBV	448649	907039	47.70%	5.920%
30	6.311	1684	1686	1690	rBV3	417	319	0.02%	0.0002%
31	6.411	1713	1717	1722	rBV3	642	640	0.03%	0.0004%
32	6.569	1763	1766	1770	rBV	323	317	0.02%	0.0002%
33	6.646	1779	1790	1791	rBV3	1428	1708	0.09%	0.011%
34	6.723	1803	1814	1831	rBV5	2798	7348	0.39%	0.048%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007397.D
 Acq On : 05 Sep 2018 21:13
 Operator : SY/MD
 Sample : J4719-10 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.784	1831	1833	1839	rVB3	625	478	0.03%	0.003%
36	6.832	1845	1848	1851	rBV3	534	414	0.02%	0.003%
37	6.890	1863	1866	1869	rBV2	382	299	0.02%	0.002%
38	6.938	1875	1881	1883	rBV2	345	361	0.02%	0.002%
39	6.971	1888	1891	1894	rVB2	497	348	0.02%	0.002%
40	7.035	1898	1911	1935	rBV	208790	371615	19.54%	2.425%
41	7.167	1949	1952	1954	rBV2	669	428	0.02%	0.003%
42	7.276	1984	1986	1989	rBV3	438	297	0.02%	0.002%
43	7.363	1999	2013	2035	rBV	779408	1339683	70.46%	8.744%
44	7.562	2072	2075	2077	rVV2	729	389	0.02%	0.003%
45	7.668	2094	2108	2131	rBV	154552	264298	13.90%	1.725%
46	7.800	2147	2149	2152	rBV3	465	280	0.01%	0.002%
47	8.064	2227	2231	2233	rBV2	452	358	0.02%	0.002%
48	8.144	2240	2256	2300	rBV2	501481	1020844	53.69%	6.663%
49	8.530	2373	2376	2382	rVB4	768	685	0.04%	0.004%
50	8.569	2384	2388	2393	rVB3	521	538	0.03%	0.004%
51	8.636	2407	2409	2412	rBV2	501	299	0.02%	0.002%
52	8.652	2412	2414	2419	rVB3	533	333	0.02%	0.002%
53	8.739	2438	2441	2444	rBV	478	327	0.02%	0.002%
54	8.755	2444	2446	2448	rBV	545	267	0.01%	0.002%
55	8.810	2460	2463	2466	rBV	573	378	0.02%	0.002%
56	8.845	2470	2474	2476	rBV2	663	389	0.02%	0.003%
57	8.900	2478	2491	2516	rBV	844258	1388655	73.03%	9.063%
58	9.061	2539	2541	2546	rVB4	1338	851	0.04%	0.006%
59	9.109	2553	2556	2564	rVB6	1480	1632	0.09%	0.011%
60	9.186	2576	2580	2581	rBV4	456	352	0.02%	0.002%
61	9.196	2581	2583	2586	rVB	831	369	0.02%	0.002%
62	9.360	2630	2634	2639	rBV4	703	665	0.03%	0.004%
63	9.430	2653	2656	2659	rBV2	523	281	0.01%	0.002%
64	9.453	2659	2663	2667	rBV3	332	327	0.02%	0.002%
65	9.491	2671	2675	2680	rBV2	524	529	0.03%	0.003%
66	9.562	2693	2697	2702	rVB4	420	411	0.02%	0.003%
67	9.598	2702	2708	2712	rVB3	751	792	0.04%	0.005%
68	9.797	2768	2770	2773	rVB	451	276	0.01%	0.002%
69	9.819	2773	2777	2780	rBV2	547	493	0.03%	0.003%
70	10.077	2853	2857	2860	rVV	348	284	0.01%	0.002%
71	10.192	2887	2893	2895	rBV2	317	319	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007397.D
 Acq On : 05 Sep 2018 21:13
 Operator : SY/MD
 Sample : J4719-10 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.266	2903	2916	2948	rVV	630126	1030095	54.18%	6.723%
73	10.382	2950	2952	2956	rVB2	760	426	0.02%	0.003%
74	10.530	2996	2998	3004	rVB3	472	480	0.03%	0.003%
75	10.623	3024	3027	3028	rBV	773	471	0.02%	0.003%
76	10.675	3041	3043	3047	rVB2	356	266	0.01%	0.002%
77	10.810	3081	3085	3092	rVB3	610	649	0.03%	0.004%
78	10.874	3099	3105	3109	rBV2	519	594	0.03%	0.004%
79	10.987	3137	3140	3145	rVB2	687	640	0.03%	0.004%
80	11.038	3149	3156	3158	rBV3	416	452	0.02%	0.003%
81	11.067	3160	3165	3168	rBV3	386	315	0.02%	0.002%
82	11.147	3187	3190	3193	rVB2	632	405	0.02%	0.003%
83	11.176	3193	3199	3204	rBV4	486	557	0.03%	0.004%
84	11.215	3208	3211	3215	rBV3	426	282	0.01%	0.002%
85	11.241	3215	3219	3221	rBV3	578	415	0.02%	0.003%
86	11.302	3225	3238	3265	rBV	624789	1048596	55.15%	6.844%
87	11.440	3279	3281	3285	rBV3	424	341	0.02%	0.002%
88	11.549	3312	3315	3317	rBV2	469	286	0.02%	0.002%
89	11.588	3323	3327	3331	rBV2	471	431	0.02%	0.003%
90	11.678	3341	3355	3376	rBV	678661	1170972	61.58%	7.642%
91	11.916	3427	3429	3433	rVB2	485	313	0.02%	0.002%
92	11.938	3433	3436	3438	rBV3	512	294	0.02%	0.002%
93	12.501	3609	3611	3615	rBV2	492	394	0.02%	0.003%
94	12.668	3658	3663	3665	rBV3	909	704	0.04%	0.005%
95	12.797	3700	3703	3706	rVB2	541	381	0.02%	0.002%
96	12.845	3715	3718	3720	rBV	502	286	0.02%	0.002%
97	12.916	3737	3740	3743	rBV2	581	464	0.02%	0.003%
98	12.977	3757	3759	3763	rBV3	557	345	0.02%	0.002%
99	13.552	3935	3938	3941	rBV5	486	448	0.02%	0.003%
100	14.424	4206	4209	4213	rBV4	1017	808	0.04%	0.005%


Sum of corrected areas: 15321929

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090518\
Data File : VV007397.D
Acq On : 05 Sep 2018 21:13
Operator : SY/MD
Sample : J4719-10 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

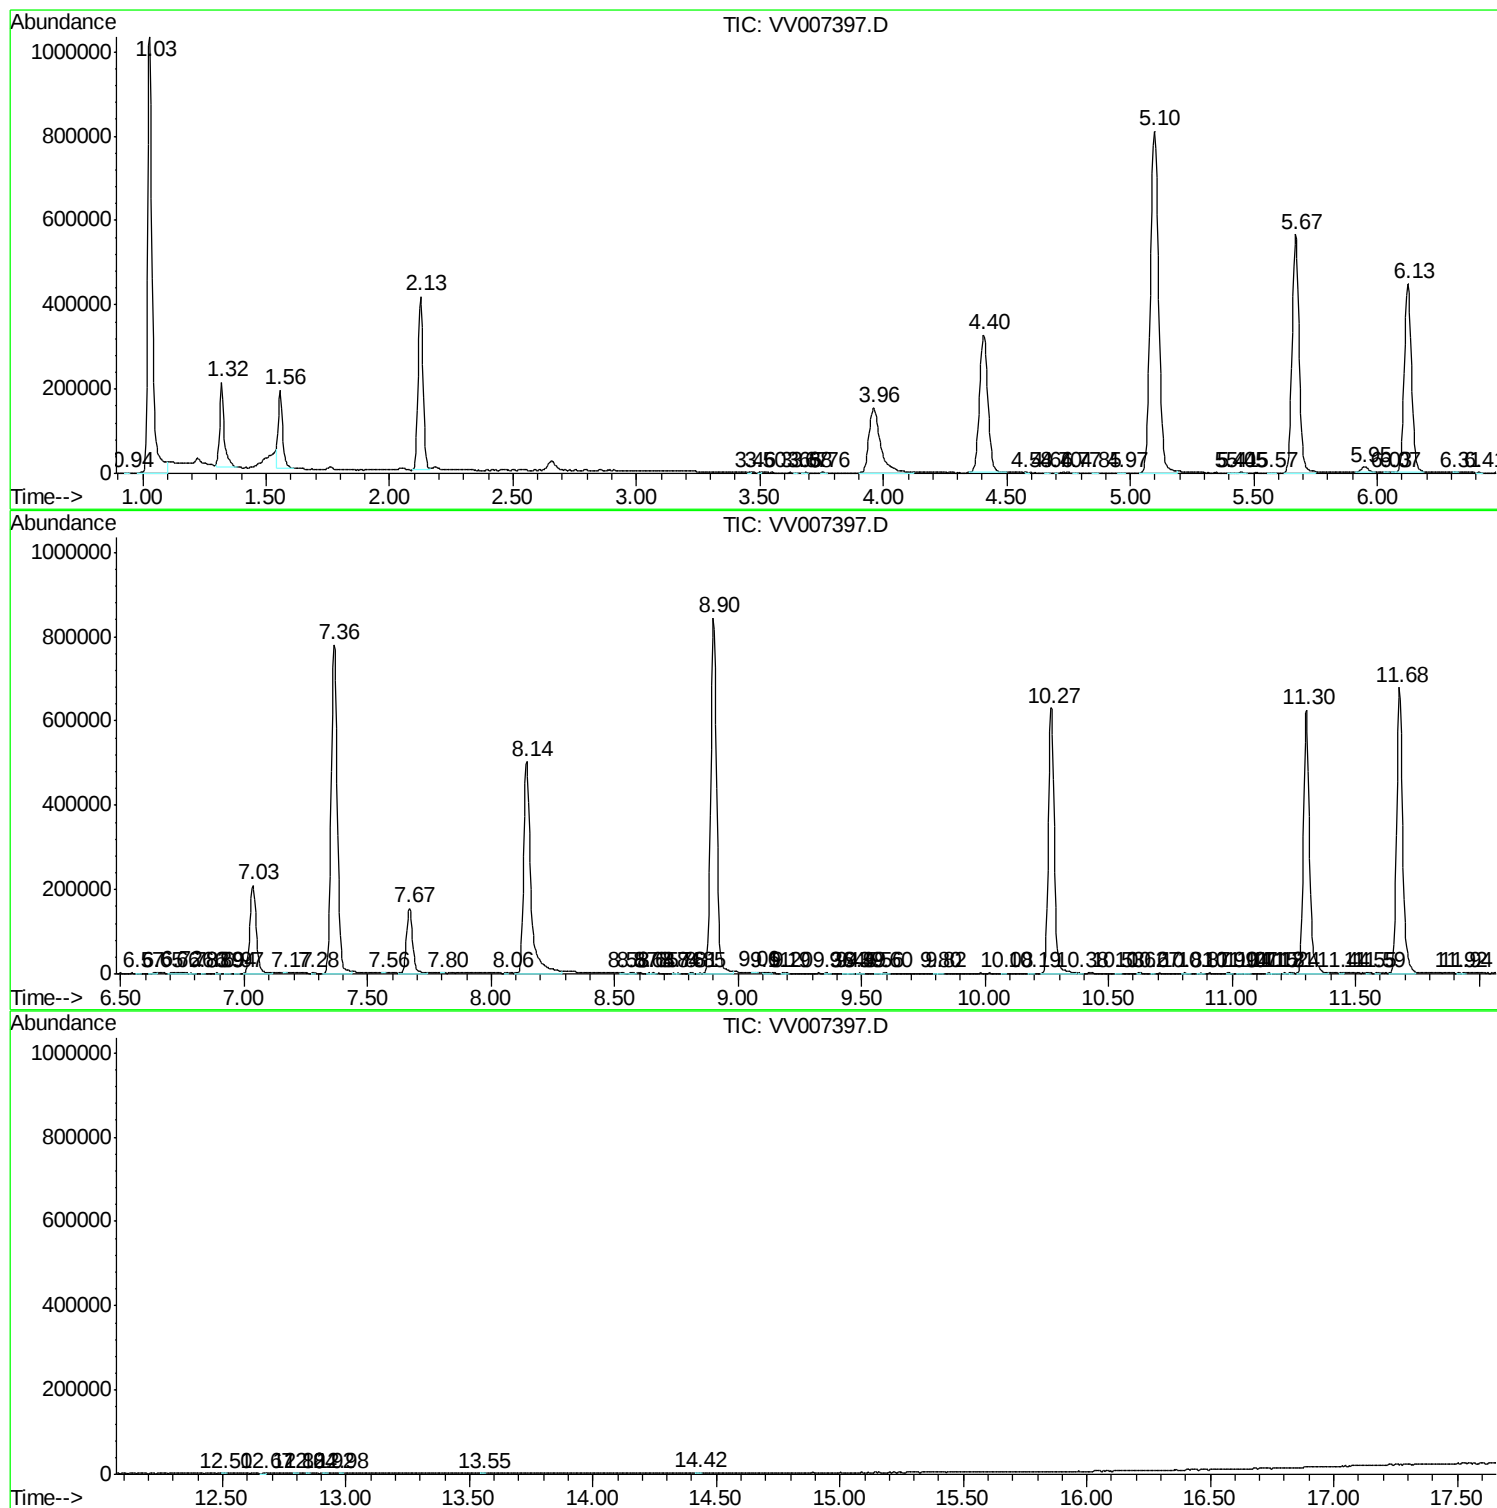

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007397.D
Acq On : 05 Sep 2018 21:13
Operator : SY/MD
Sample : J4719-10 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007397.D
Acq On : 05 Sep 2018 21:13
Operator : SY/MD
Sample : J4719-10 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc