

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007399.D
 Acq On : 05 Sep 2018 22:03
 Operator : SY/MD
 Sample : J4719-12 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.916	3	8	14	rBV4	356	354	0.002%	0.0002%
2	0.948	14	18	22	rBV3	489	399	0.002%	0.0003%
3	1.029	26	43	67	rBV	1136119	1433583	76.03%	9.199%
4	1.321	127	134	154	rVB	201401	258717	13.72%	1.660%
5	1.556	203	207	226	rVB	178581	221314	11.74%	1.420%
6	2.125	374	384	396	rBV	405565	568948	30.18%	3.651%
7	3.508	812	814	819	rVB3	612	343	0.002%	0.0002%
8	3.617	846	848	852	rBV2	381	278	0.001%	0.0002%
9	3.890	926	933	936	rBV3	539	543	0.003%	0.0003%
10	3.961	936	955	999	rBV2	150562	490771	26.03%	3.149%
11	4.263	1047	1049	1052	rVB2	779	466	0.002%	0.0003%
12	4.299	1058	1060	1066	rVV3	441	366	0.002%	0.0002%
13	4.340	1070	1073	1075	rVV3	566	323	0.002%	0.0002%
14	4.405	1075	1093	1129	rVV	318742	769752	40.83%	4.939%
15	4.572	1140	1145	1146	rBV2	531	407	0.002%	0.0003%
16	4.581	1146	1148	1151	rVB3	581	339	0.002%	0.0002%
17	4.601	1151	1154	1158	rBV3	728	645	0.003%	0.0004%
18	4.681	1176	1179	1183	rBV2	669	534	0.003%	0.0003%
19	4.726	1190	1193	1198	rVV5	364	340	0.002%	0.0002%
20	4.864	1230	1236	1238	rBV2	413	307	0.002%	0.0002%
21	4.948	1256	1262	1263	rBV2	547	360	0.002%	0.0002%
22	5.099	1288	1309	1346	rBV2	797389	1885452	100.00%	12.099%
23	5.366	1391	1392	1399	rVB3	654	467	0.002%	0.0003%
24	5.398	1399	1402	1406	rVB	503	368	0.002%	0.0002%
25	5.424	1406	1410	1412	rBV3	446	278	0.001%	0.0002%
26	5.466	1421	1423	1429	rVB3	505	426	0.002%	0.0003%
27	5.581	1456	1459	1462	rBV2	387	259	0.001%	0.0002%
28	5.668	1470	1486	1517	rBV	578223	1149236	60.95%	7.375%
29	5.954	1565	1575	1589	rVB6	17266	37204	1.97%	0.239%
30	6.044	1600	1603	1606	rVB4	656	368	0.002%	0.0002%
31	6.125	1610	1628	1650	rBV	455260	904190	47.96%	5.802%
32	6.343	1694	1696	1701	rVB3	548	387	0.002%	0.0002%
33	6.369	1701	1704	1708	rVV3	516	384	0.002%	0.0002%
34	6.388	1708	1710	1713	rVB2	589	338	0.002%	0.0002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007399.D
 Acq On : 05 Sep 2018 22:03
 Operator : SY/MD
 Sample : J4719-12 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.405	1713	1715	1717	rBV2	431	251	0.01%	0.002%
36	6.585	1768	1771	1776	rBV3	554	481	0.03%	0.003%
37	6.610	1776	1779	1783	rBV3	575	453	0.02%	0.003%
38	6.662	1787	1795	1800	rVV6	942	1602	0.08%	0.010%
39	6.729	1806	1816	1825	rBV2	2348	4391	0.23%	0.028%
40	6.794	1834	1836	1843	rVB4	416	323	0.02%	0.002%
41	6.848	1847	1853	1854	rBV2	392	368	0.02%	0.002%
42	6.871	1857	1860	1865	rBV2	559	327	0.02%	0.002%
43	7.035	1898	1911	1929	rBV	201423	357104	18.94%	2.292%
44	7.176	1948	1955	1959	rBV8	1332	1960	0.10%	0.013%
45	7.286	1985	1989	1995	rBV4	926	1148	0.06%	0.007%
46	7.363	1998	2013	2034	rBV	764792	1328261	70.45%	8.523%
47	7.559	2071	2074	2076	rBV2	578	426	0.02%	0.003%
48	7.668	2097	2108	2127	rBV	154025	255440	13.55%	1.639%
49	7.929	2186	2189	2192	rBV	634	367	0.02%	0.002%
50	8.022	2206	2218	2235	rVB	122291	204055	10.82%	1.309%
51	8.144	2242	2256	2300	rBV2	484090	1000174	53.05%	6.418%
52	8.588	2391	2394	2396	rVB2	486	300	0.02%	0.002%
53	8.720	2430	2435	2436	rBV2	305	257	0.01%	0.002%
54	8.848	2472	2475	2476	rBV	447	253	0.01%	0.002%
55	8.900	2478	2491	2526	rVV	866854	1412019	74.89%	9.061%
56	9.192	2579	2582	2586	rVB3	542	424	0.02%	0.003%
57	9.253	2599	2601	2604	rBV2	404	303	0.02%	0.002%
58	9.539	2681	2690	2693	rVB4	513	804	0.04%	0.005%
59	9.568	2696	2699	2702	rBV2	617	460	0.02%	0.003%
60	9.646	2721	2723	2728	rVB3	522	424	0.02%	0.003%
61	9.700	2737	2740	2744	rVB3	411	333	0.02%	0.002%
62	9.774	2759	2763	2768	rBV2	412	487	0.03%	0.003%
63	9.800	2768	2771	2774	rVB2	384	251	0.01%	0.002%
64	9.819	2774	2777	2780	rBV2	381	306	0.02%	0.002%
65	9.990	2829	2830	2834	rVV	481	280	0.01%	0.002%
66	10.105	2863	2866	2869	rBV2	501	279	0.01%	0.002%
67	10.157	2878	2882	2883	rBV2	384	294	0.02%	0.002%
68	10.163	2883	2884	2888	rVV2	562	299	0.02%	0.002%
69	10.189	2888	2892	2894	rVV3	371	256	0.01%	0.002%
70	10.205	2894	2897	2903	rVV2	708	508	0.03%	0.003%
71	10.266	2903	2916	2949	rVV	624636	1012513	53.70%	6.497%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007399.D
 Acq On : 05 Sep 2018 22:03
 Operator : SY/MD
 Sample : J4719-12 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGE8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.417	2958	2963	2964	rBV3	419	340	0.02%	0.002%
73	10.748	3060	3066	3067	rBV4	487	322	0.02%	0.002%
74	10.758	3067	3069	3072	rBV3	401	318	0.02%	0.002%
75	10.813	3082	3086	3087	rBV	599	355	0.02%	0.002%
76	10.855	3096	3099	3102	rBV2	531	357	0.02%	0.002%
77	10.903	3111	3114	3119	rVB3	617	418	0.02%	0.003%
78	10.929	3119	3122	3125	rBV2	474	341	0.02%	0.002%
79	11.019	3147	3150	3153	rBV3	420	295	0.02%	0.002%
80	11.157	3190	3193	3197	rVB2	353	264	0.01%	0.002%
81	11.189	3197	3203	3207	rBV3	531	679	0.04%	0.004%
82	11.228	3212	3215	3216	rVV2	449	254	0.01%	0.002%
83	11.237	3216	3218	3223	rVB2	561	334	0.02%	0.002%
84	11.301	3223	3238	3265	rBV	635995	1079401	57.25%	6.927%
85	11.395	3265	3267	3272	rVB5	672	444	0.02%	0.003%
86	11.572	3320	3322	3326	rBV	400	286	0.02%	0.002%
87	11.678	3341	3355	3381	rBV	688744	1175333	62.34%	7.542%
88	11.809	3393	3396	3401	rBV5	483	522	0.03%	0.003%
89	11.890	3415	3421	3423	rBV3	442	466	0.02%	0.003%
90	12.070	3474	3477	3481	rVB2	427	280	0.01%	0.002%
91	12.276	3533	3541	3543	rBV3	808	1147	0.06%	0.007%
92	12.655	3656	3659	3660	rBV	582	335	0.02%	0.002%
93	12.684	3666	3668	3672	rVB2	776	381	0.02%	0.002%
94	12.707	3672	3675	3678	rBV3	673	388	0.02%	0.002%
95	12.941	3743	3748	3754	rVB4	1394	1245	0.07%	0.008%
96	13.446	3903	3905	3908	rBV2	464	322	0.02%	0.002%
97	13.481	3913	3916	3919	rBV3	791	520	0.03%	0.003%
98	13.536	3928	3933	3935	rBV2	778	766	0.04%	0.005%
99	13.871	4035	4037	4039	rBV3	512	321	0.02%	0.002%
100	13.887	4039	4042	4045	rVV2	804	576	0.03%	0.004%


Sum of corrected areas: 15583637

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090518\
Data File : VV007399.D
Acq On : 05 Sep 2018 22:03
Operator : SY/MD
Sample : J4719-12 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

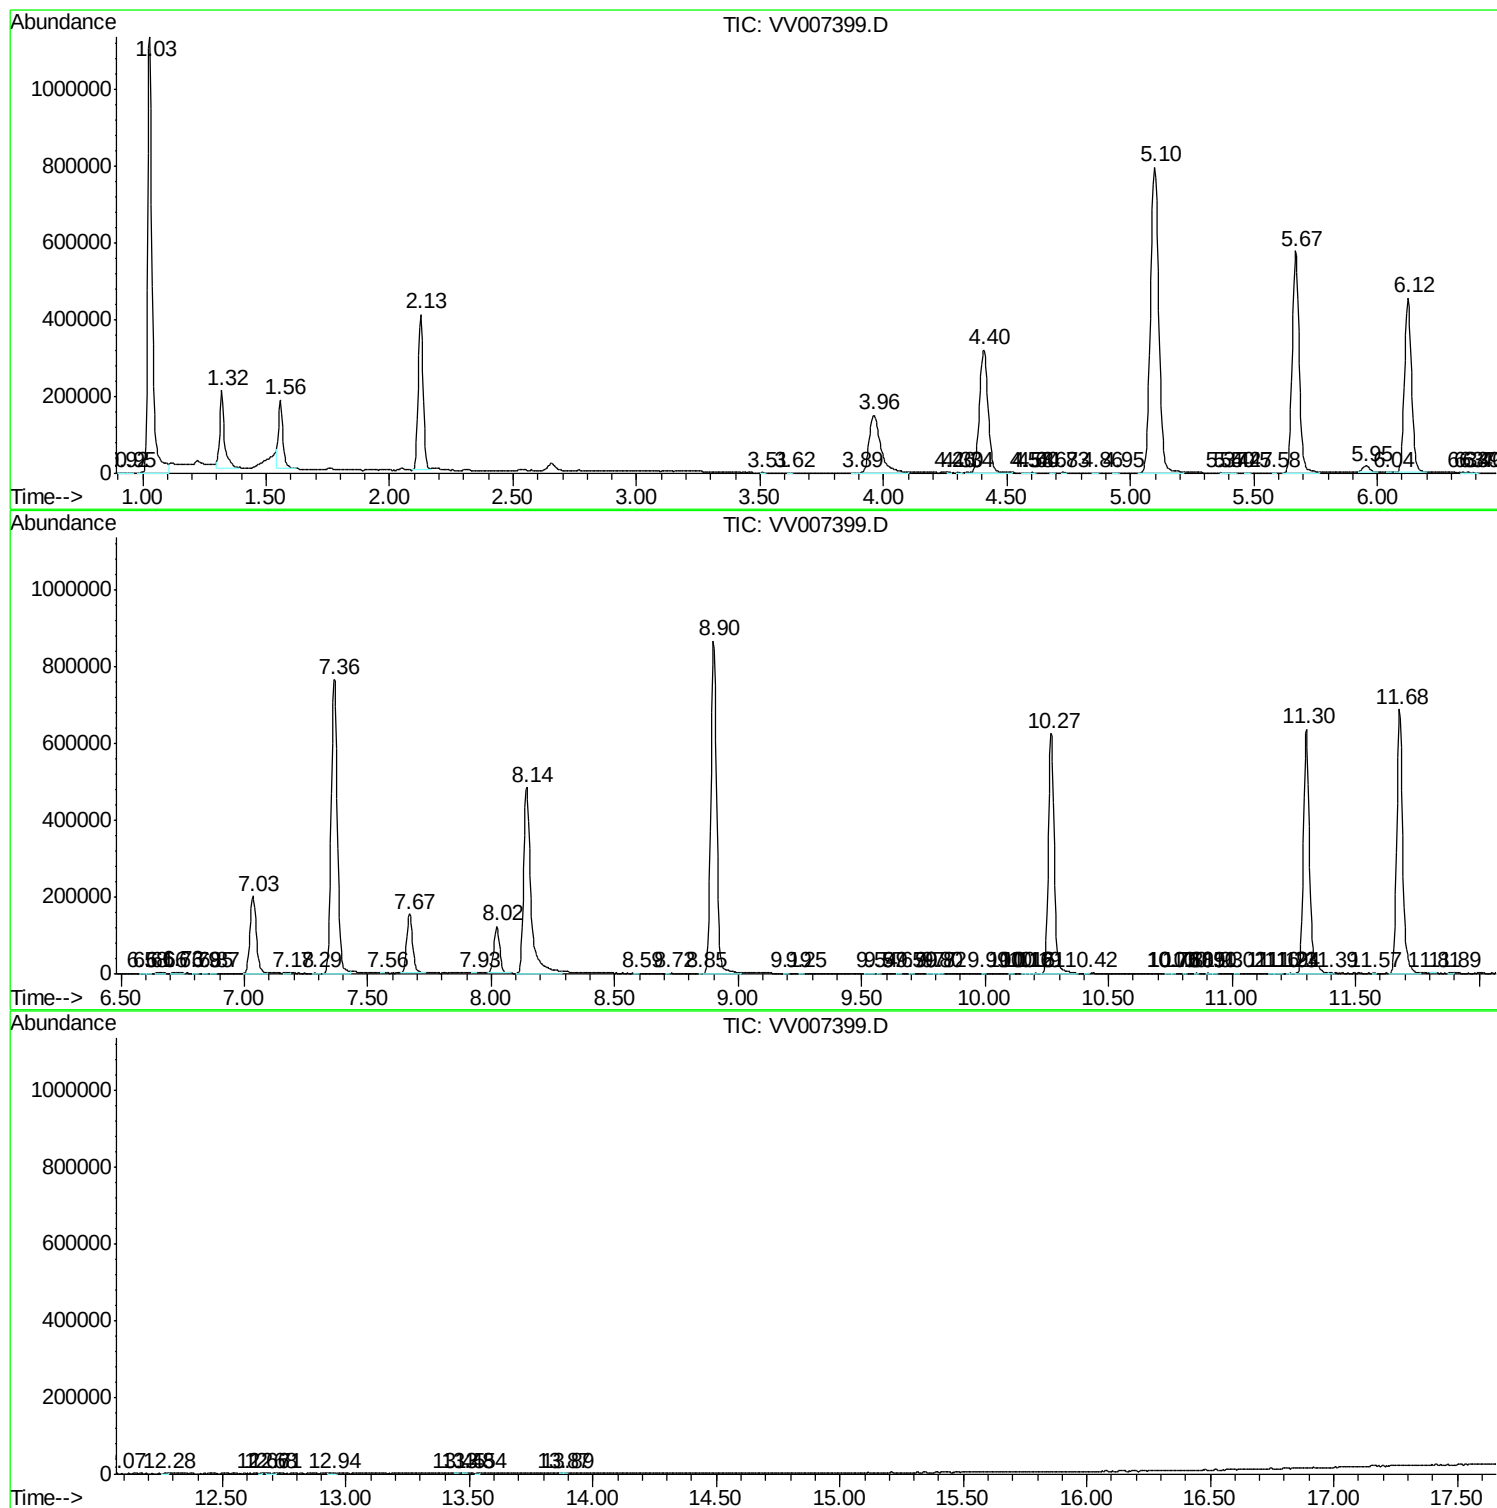

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007399.D
Acq On : 05 Sep 2018 22:03
Operator : SY/MD
Sample : J4719-12 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007399.D
Acq On : 05 Sep 2018 22:03
Operator : SY/MD
Sample : J4719-12 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGE8

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc