

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007403.D
 Acq On : 05 Sep 2018 23:43
 Operator : SY/MD
 Sample : J4719-16 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGF2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.903	3	4	11	rVB2	501	409	0.02%	0.003%
2	0.942	11	16	22	rVB3	490	611	0.03%	0.004%
3	1.029	29	43	65	rBV	1053823	1332243	71.72%	8.520%
4	1.321	126	134	152	rVB	195737	250748	13.50%	1.604%
5	1.556	202	207	226	rVB	185846	236545	12.73%	1.513%
6	2.125	374	384	397	rBV	389564	542826	29.22%	3.472%
7	3.366	768	770	774	rBV2	510	422	0.02%	0.003%
8	3.392	776	778	780	rVB2	531	241	0.01%	0.002%
9	3.411	780	784	790	rBV5	524	641	0.03%	0.004%
10	3.627	848	851	853	rBV	430	331	0.02%	0.002%
11	3.832	910	915	918	rBV3	461	493	0.03%	0.003%
12	3.961	935	955	992	rBV2	166920	521217	28.06%	3.333%
13	4.292	1054	1058	1060	rBV2	343	299	0.02%	0.002%
14	4.405	1075	1093	1118	rBV	323679	766560	41.26%	4.903%
15	4.556	1137	1140	1141	rBV3	413	245	0.01%	0.002%
16	4.729	1185	1194	1202	rVB5	1513	2555	0.14%	0.016%
17	4.765	1202	1205	1206	rBV2	484	267	0.01%	0.002%
18	4.823	1221	1223	1230	rVB2	323	258	0.01%	0.002%
19	4.919	1250	1253	1257	rVB2	503	361	0.02%	0.002%
20	4.945	1257	1261	1265	rBV3	592	550	0.03%	0.004%
21	5.003	1276	1279	1285	rVB3	573	537	0.03%	0.003%
22	5.099	1289	1309	1334	rBV2	791462	1857685	100.00%	11.881%
23	5.244	1352	1354	1357	rVB2	907	531	0.03%	0.003%
24	5.299	1368	1371	1374	rVB2	722	569	0.03%	0.004%
25	5.318	1374	1377	1380	rVB3	404	271	0.01%	0.002%
26	5.440	1412	1415	1419	rBV2	544	366	0.02%	0.002%
27	5.498	1430	1433	1437	rBV2	616	646	0.03%	0.004%
28	5.517	1437	1439	1441	rVV2	555	368	0.02%	0.002%
29	5.575	1451	1457	1461	rBV4	402	434	0.02%	0.003%
30	5.668	1471	1486	1514	rBV	569730	1132342	60.95%	7.242%
31	5.961	1562	1577	1597	rVB5	32147	74031	3.99%	0.473%
32	6.125	1611	1628	1651	rBV	446249	898697	48.38%	5.748%
33	6.305	1680	1684	1692	rVB6	668	743	0.04%	0.005%
34	6.356	1698	1700	1703	rBV2	444	303	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007403.D
 Acq On : 05 Sep 2018 23:43
 Operator : SY/MD
 Sample : J4719-16 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGF2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.405	1713	1715	1719	rVB4	373	240	0.01%	0.002%
36	6.466	1728	1734	1742	rVB3	959	1316	0.07%	0.008%
37	6.501	1742	1745	1747	rBV3	395	314	0.02%	0.002%
38	6.601	1772	1776	1780	rBV2	336	286	0.02%	0.002%
39	6.623	1780	1783	1785	rBV3	595	449	0.02%	0.003%
40	6.646	1786	1790	1797	rVV5	1091	1506	0.08%	0.010%
41	6.723	1808	1814	1826	rBV6	2979	5252	0.28%	0.034%
42	6.774	1826	1830	1835	rBV6	470	527	0.03%	0.003%
43	6.823	1841	1845	1848	rBV2	589	486	0.03%	0.003%
44	6.858	1853	1856	1859	rBV3	571	479	0.03%	0.003%
45	6.916	1871	1874	1876	rBV3	386	272	0.01%	0.002%
46	7.035	1897	1911	1930	rBV	194308	353412	19.02%	2.260%
47	7.147	1941	1946	1948	rBV3	591	546	0.03%	0.003%
48	7.363	2000	2013	2032	rBV	736383	1275269	68.65%	8.156%
49	7.668	2095	2108	2131	rBV	151520	257034	13.84%	1.644%
50	8.022	2205	2218	2242	rVB	330376	551730	29.70%	3.529%
51	8.144	2243	2256	2292	rBV2	484223	995505	53.59%	6.367%
52	8.395	2332	2334	2337	rVB3	905	495	0.03%	0.003%
53	8.511	2367	2370	2376	rBV7	592	541	0.03%	0.003%
54	8.803	2458	2461	2464	rVB3	490	300	0.02%	0.002%
55	8.823	2464	2467	2469	rBV3	553	339	0.02%	0.002%
56	8.900	2478	2491	2517	rBV	833191	1371926	73.85%	8.774%
57	9.183	2573	2579	2581	rBV3	1029	995	0.05%	0.006%
58	9.257	2600	2602	2608	rBV3	366	356	0.02%	0.002%
59	9.334	2622	2626	2628	rBV	436	375	0.02%	0.002%
60	9.482	2670	2672	2677	rVB	357	271	0.01%	0.002%
61	9.565	2693	2698	2700	rBV3	401	458	0.02%	0.003%
62	9.594	2702	2707	2712	rBV5	551	717	0.04%	0.005%
63	9.623	2712	2716	2718	rBV2	550	389	0.02%	0.002%
64	9.636	2718	2720	2723	rVB	589	279	0.02%	0.002%
65	9.684	2729	2735	2738	rBV2	510	646	0.03%	0.004%
66	9.874	2792	2794	2798	rVB2	553	390	0.02%	0.002%
67	9.893	2798	2800	2803	rBV	424	247	0.01%	0.002%
68	9.951	2816	2818	2824	rVB3	432	331	0.02%	0.002%
69	10.028	2839	2842	2847	rBV2	497	503	0.03%	0.003%
70	10.051	2847	2849	2852	rVV	404	280	0.02%	0.002%
71	10.266	2902	2916	2949	rBV	614278	1015125	54.64%	6.492%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007403.D
 Acq On : 05 Sep 2018 23:43
 Operator : SY/MD
 Sample : J4719-16 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGF2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.478	2980	2982	2985	rBV	414	251	0.01%	0.002%
73	10.568	3007	3010	3015	rBV2	420	388	0.02%	0.002%
74	10.623	3023	3027	3033	rVB4	803	798	0.04%	0.005%
75	10.652	3033	3036	3039	rBV	490	397	0.02%	0.003%
76	10.832	3087	3092	3095	rBV2	579	480	0.03%	0.003%
77	10.877	3103	3106	3107	rBV	439	255	0.01%	0.002%
78	10.906	3112	3115	3119	rVV3	394	313	0.02%	0.002%
79	10.958	3128	3131	3134	rBV3	607	456	0.02%	0.003%
80	10.983	3134	3139	3141	rVB2	516	450	0.02%	0.003%
81	11.003	3141	3145	3146	rBV2	391	256	0.01%	0.002%
82	11.044	3155	3158	3163	rVB3	587	511	0.03%	0.003%
83	11.167	3191	3196	3197	rBV	341	269	0.01%	0.002%
84	11.228	3213	3215	3219	rVV2	410	343	0.02%	0.002%
85	11.302	3225	3238	3270	rBV	609296	1032198	55.56%	6.601%
86	11.446	3279	3283	3288	rBV4	621	627	0.03%	0.004%
87	11.565	3316	3320	3323	rBV5	488	408	0.02%	0.003%
88	11.604	3329	3332	3335	rVB2	698	441	0.02%	0.003%
89	11.678	3342	3355	3379	rBV	649855	1112863	59.91%	7.117%
90	11.797	3390	3392	3395	rVB2	605	270	0.01%	0.002%
91	11.980	3447	3449	3452	rVB3	526	314	0.02%	0.002%
92	12.031	3463	3465	3470	rVB4	480	383	0.02%	0.002%
93	12.266	3534	3538	3542	rBV2	413	447	0.02%	0.003%
94	12.523	3614	3618	3621	rBV2	378	348	0.02%	0.002%
95	12.707	3672	3675	3680	rBV4	612	436	0.02%	0.003%
96	12.732	3680	3683	3689	rBV3	494	576	0.03%	0.004%
97	13.755	3999	4001	4003	rBV	599	348	0.02%	0.002%
98	14.096	4104	4107	4108	rBV2	1211	690	0.04%	0.004%
99	14.160	4124	4127	4131	rBV3	834	675	0.04%	0.004%
100	16.269	4780	4783	4788	rVB	27395	14876	0.80%	0.095%


Sum of corrected areas: 15635998

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090518\
Data File : VV007403.D
Acq On : 05 Sep 2018 23:43
Operator : SY/MD
Sample : J4719-16 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGF2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

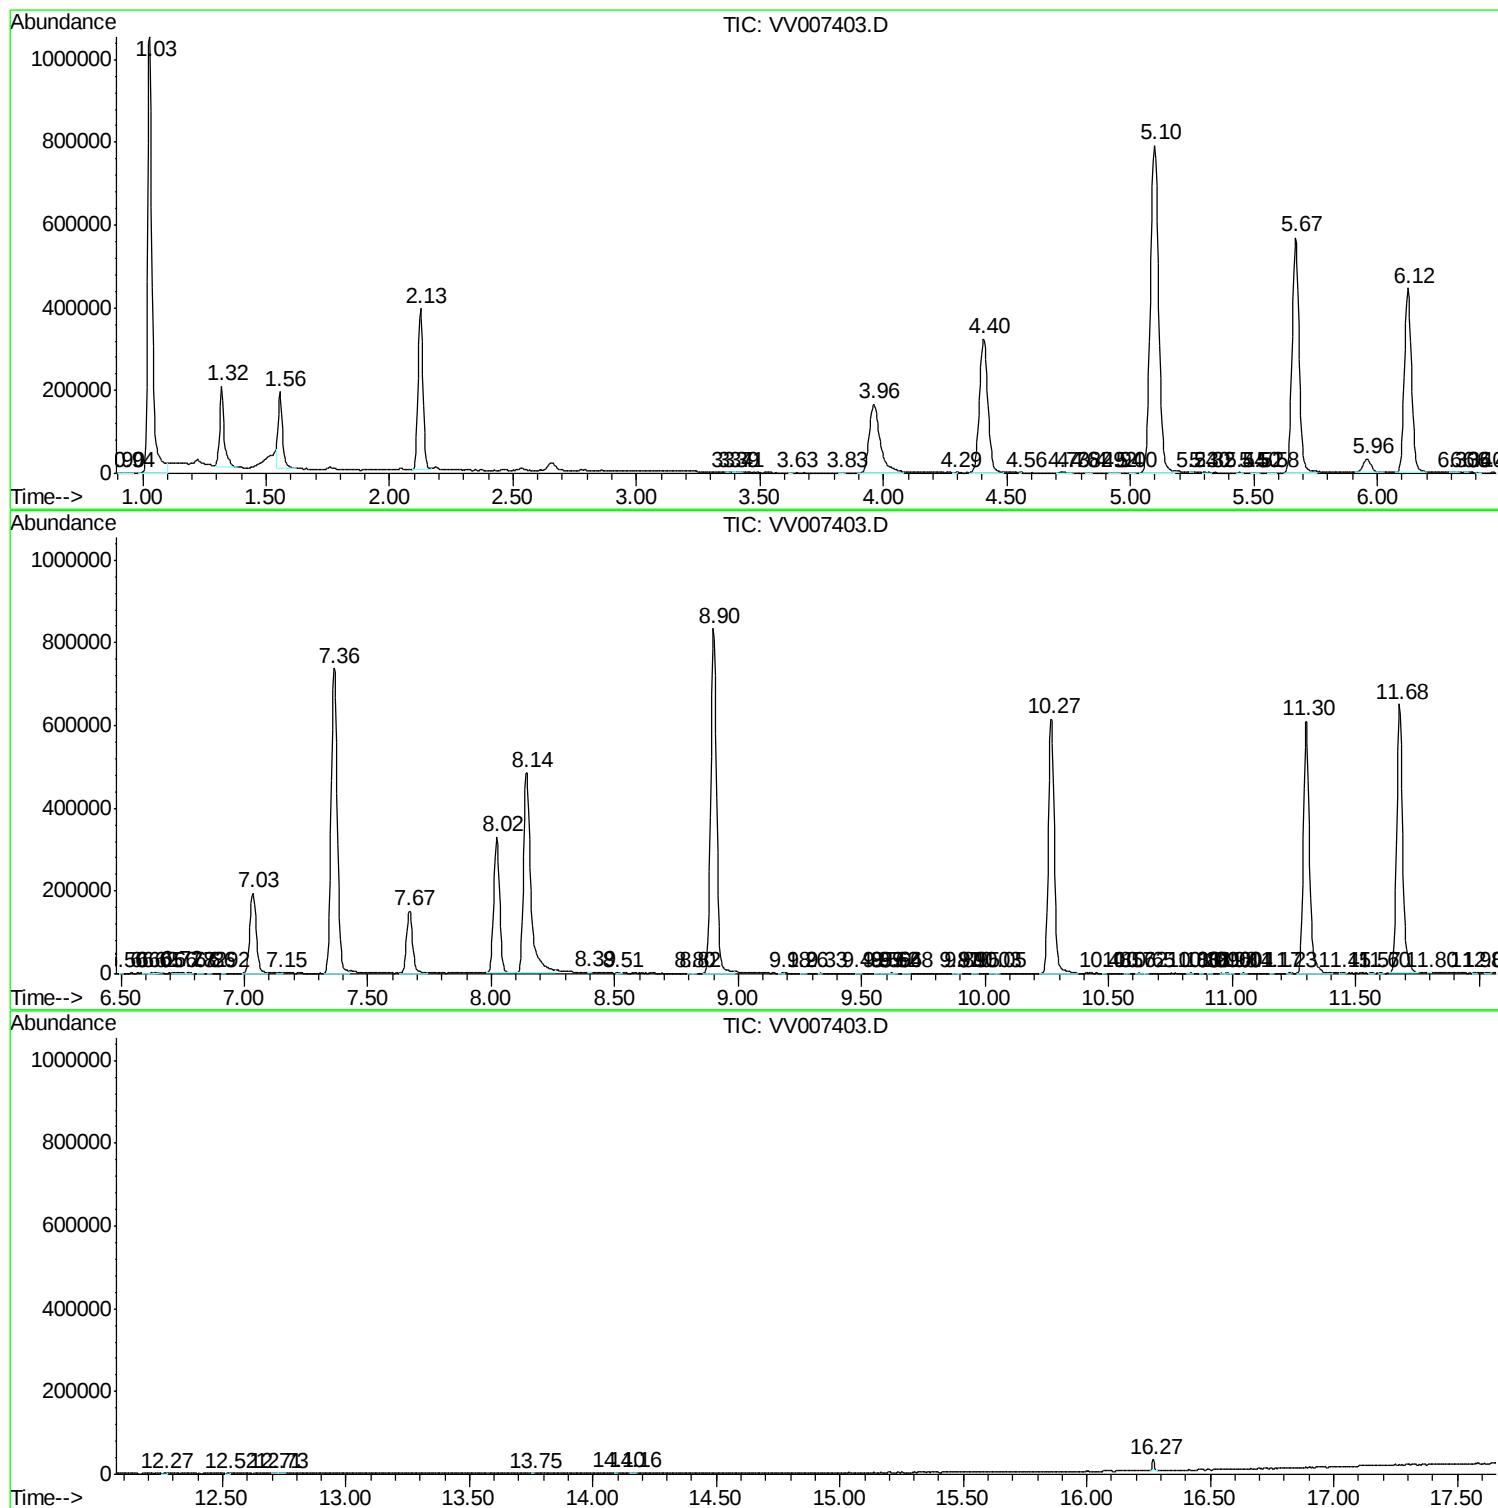

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007403.D
Acq On : 05 Sep 2018 23:43
Operator : SY/MD
Sample : J4719-16 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGF2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007403.D
Acq On : 05 Sep 2018 23:43
Operator : SY/MD
Sample : J4719-16 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGF2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc