

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007409.D
 Acq On : 06 Sep 2018 02:13
 Operator : SY/MD
 Sample : J4751-01 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.932	9	13	14	rBV2	395	235	0.00%	0.001%
2	1.029	29	43	65	rBV	1126495	1422174	7.22%	3.973%
3	1.321	126	134	152	rVB	196795	250616	1.27%	0.700%
4	1.559	202	208	225	rVB	178137	234340	1.19%	0.655%
5	2.125	374	384	396	rBV	403250	573334	2.91%	1.602%
6	2.655	541	549	567	rVB	26541	56560	0.29%	0.158%
7	3.382	772	775	776	rBV2	628	301	0.00%	0.001%
8	3.469	799	802	804	rBV4	505	267	0.00%	0.001%
9	3.530	818	821	824	rVB3	482	262	0.00%	0.001%
10	3.556	827	829	831	rVB	586	211	0.00%	0.001%
11	3.861	919	924	925	rBV	677	440	0.00%	0.001%
12	3.890	930	933	936	rVB2	648	460	0.00%	0.001%
13	3.958	936	954	1007	rBV2	167348	533474	2.71%	1.490%
14	4.302	1059	1061	1063	rBV3	433	279	0.00%	0.001%
15	4.327	1067	1069	1072	rBV2	503	295	0.00%	0.001%
16	4.405	1075	1093	1117	rBV	324950	780784	3.97%	2.181%
17	4.601	1151	1154	1159	rVB4	677	520	0.00%	0.001%
18	4.662	1171	1173	1175	rBV	442	232	0.00%	0.001%
19	4.700	1181	1185	1186	rBV2	474	249	0.00%	0.001%
20	4.816	1218	1221	1224	rBV	338	265	0.00%	0.001%
21	4.877	1238	1240	1243	rVB3	429	289	0.00%	0.001%
22	4.913	1248	1251	1253	rBV2	327	179	0.00%	0.001%
23	4.948	1258	1262	1265	rVB	636	486	0.00%	0.001%
24	4.980	1265	1272	1278	rBV4	597	690	0.00%	0.002%
25	5.009	1278	1281	1284	rVB3	579	335	0.00%	0.001%
26	5.099	1290	1309	1335	rBV2	816174	1912173	9.71%	5.341%
27	5.318	1375	1377	1378	rBV	398	189	0.00%	0.001%
28	5.372	1391	1394	1395	rBV	361	236	0.00%	0.001%
29	5.446	1409	1417	1420	rBV4	848	1201	0.01%	0.003%
30	5.565	1451	1454	1458	rVB4	342	250	0.00%	0.001%
31	5.668	1470	1486	1504	rBV	602135	1178985	5.99%	3.293%
32	5.964	1564	1578	1597	rVB3	86414	177605	0.90%	0.496%
33	6.032	1597	1599	1600	rBV	516	199	0.00%	0.001%
34	6.125	1612	1628	1654	rBV	455926	917245	4.66%	2.562%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007409.D
 Acq On : 06 Sep 2018 02:13
 Operator : SY/MD
 Sample : J4751-01 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.363	1700	1702	1703	rBV2	470	199	0.00%	0.001%
36	6.408	1714	1716	1718	rVB2	542	191	0.00%	0.001%
37	6.533	1753	1755	1758	rVB2	526	215	0.00%	0.001%
38	6.652	1784	1792	1796	rBV5	1789	2648	0.01%	0.007%
39	6.700	1803	1807	1808	rBV2	524	381	0.00%	0.001%
40	6.720	1808	1813	1821	rVV5	2053	3604	0.02%	0.010%
41	6.861	1854	1857	1860	rBV3	573	346	0.00%	0.001%
42	6.884	1861	1864	1867	rBV2	345	226	0.00%	0.001%
43	6.916	1871	1874	1877	rBV3	446	331	0.00%	0.001%
44	6.932	1877	1879	1882	rVB2	438	194	0.00%	0.001%
45	6.948	1882	1884	1888	rBV3	374	284	0.00%	0.001%
46	6.964	1888	1889	1893	rVB2	573	295	0.00%	0.001%
47	7.035	1893	1911	1939	rBV	202415	364194	1.85%	1.017%
48	7.257	1978	1980	1982	rBV3	526	317	0.00%	0.001%
49	7.289	1987	1990	1996	rVB3	644	573	0.00%	0.002%
50	7.363	1999	2013	2032	rBV	783322	1362339	6.92%	3.806%
51	7.568	2075	2077	2082	rVB4	984	728	0.00%	0.002%
52	7.668	2097	2108	2130	rBV	154978	254567	1.29%	0.711%
53	7.945	2191	2194	2196	rBV2	552	325	0.00%	0.001%
54	8.025	2202	2219	2244	rBV	11957426	19685908	100.00%	54.990%
55	8.141	2246	2255	2285	rVB2	560497	1088432	5.53%	3.040%
56	8.691	2424	2426	2432	rVB4	678	491	0.00%	0.001%
57	8.723	2432	2436	2439	rBV2	499	465	0.00%	0.001%
58	8.851	2474	2476	2478	rBV3	477	251	0.00%	0.001%
59	8.900	2478	2491	2517	rBV	929372	1505061	7.65%	4.204%
60	9.179	2574	2578	2579	rBV3	1081	753	0.00%	0.002%
61	9.237	2590	2596	2600	rBV3	532	647	0.00%	0.002%
62	9.260	2600	2603	2605	rBV2	452	248	0.00%	0.001%
63	9.292	2609	2613	2616	rVV3	384	305	0.00%	0.001%
64	9.334	2622	2626	2630	rVB3	484	408	0.00%	0.001%
65	9.398	2641	2646	2649	rBV2	568	492	0.00%	0.001%
66	9.462	2664	2666	2670	rBV4	291	229	0.00%	0.001%
67	9.601	2706	2709	2712	rBV3	403	380	0.00%	0.001%
68	9.761	2756	2759	2761	rBV2	428	282	0.00%	0.001%
69	9.877	2792	2795	2798	rVB2	515	350	0.00%	0.001%
70	9.912	2804	2806	2808	rVB	412	183	0.00%	0.001%
71	9.928	2808	2811	2813	rBV2	404	235	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007409.D
 Acq On : 06 Sep 2018 02:13
 Operator : SY/MD
 Sample : J4751-01 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	9.980	2821	2827	2834	rBV5	427	650	0.00%	0.002%
73	10.179	2886	2889	2893	rBV2	379	325	0.00%	0.001%
74	10.266	2903	2916	2951	rVB	645424	1045167	5.31%	2.920%
75	10.401	2956	2958	2961	rBV3	433	244	0.00%	0.001%
76	10.424	2962	2965	2971	rVB5	775	712	0.00%	0.002%
77	10.520	2987	2995	2999	rBV4	701	828	0.00%	0.002%
78	10.597	3015	3019	3022	rBV2	298	341	0.00%	0.001%
79	10.710	3052	3054	3056	rBV3	488	204	0.00%	0.001%
80	10.874	3102	3105	3109	rBV3	688	648	0.00%	0.002%
81	10.906	3113	3115	3118	rVB2	758	346	0.00%	0.001%
82	10.925	3118	3121	3123	rBV2	397	296	0.00%	0.001%
83	10.996	3141	3143	3145	rBV2	362	190	0.00%	0.001%
84	11.035	3152	3155	3157	rBV2	565	289	0.00%	0.001%
85	11.096	3170	3174	3176	rBV4	611	444	0.00%	0.001%
86	11.231	3211	3216	3224	rBV6	1442	1952	0.01%	0.005%
87	11.301	3224	3238	3267	rBV	703379	1174517	5.97%	3.281%
88	11.678	3343	3355	3387	rVV	736675	1241544	6.31%	3.468%
89	11.832	3399	3403	3404	rBV2	702	426	0.00%	0.001%
90	11.993	3450	3453	3460	rBV5	603	651	0.00%	0.002%
91	12.073	3476	3478	3482	rBV2	366	280	0.00%	0.001%
92	12.285	3536	3544	3545	rBV5	865	1078	0.01%	0.003%
93	12.674	3662	3665	3668	rBV3	683	492	0.00%	0.001%
94	12.758	3689	3691	3693	rBV2	600	355	0.00%	0.001%
95	12.916	3736	3740	3743	rBV3	674	604	0.00%	0.002%
96	13.073	3786	3789	3797	rVB4	1042	1156	0.01%	0.003%
97	13.108	3797	3800	3804	rBV3	699	669	0.00%	0.002%
98	13.317	3861	3865	3871	rBV5	994	1234	0.01%	0.003%
99	13.443	3901	3904	3906	rBV3	684	475	0.00%	0.001%
100	14.301	4168	4171	4172	rBV2	897	479	0.00%	0.001%


Sum of corrected areas: 35799033

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090518\
Data File : VV007409.D
Acq On : 06 Sep 2018 02:13
Operator : SY/MD
Sample : J4751-01 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

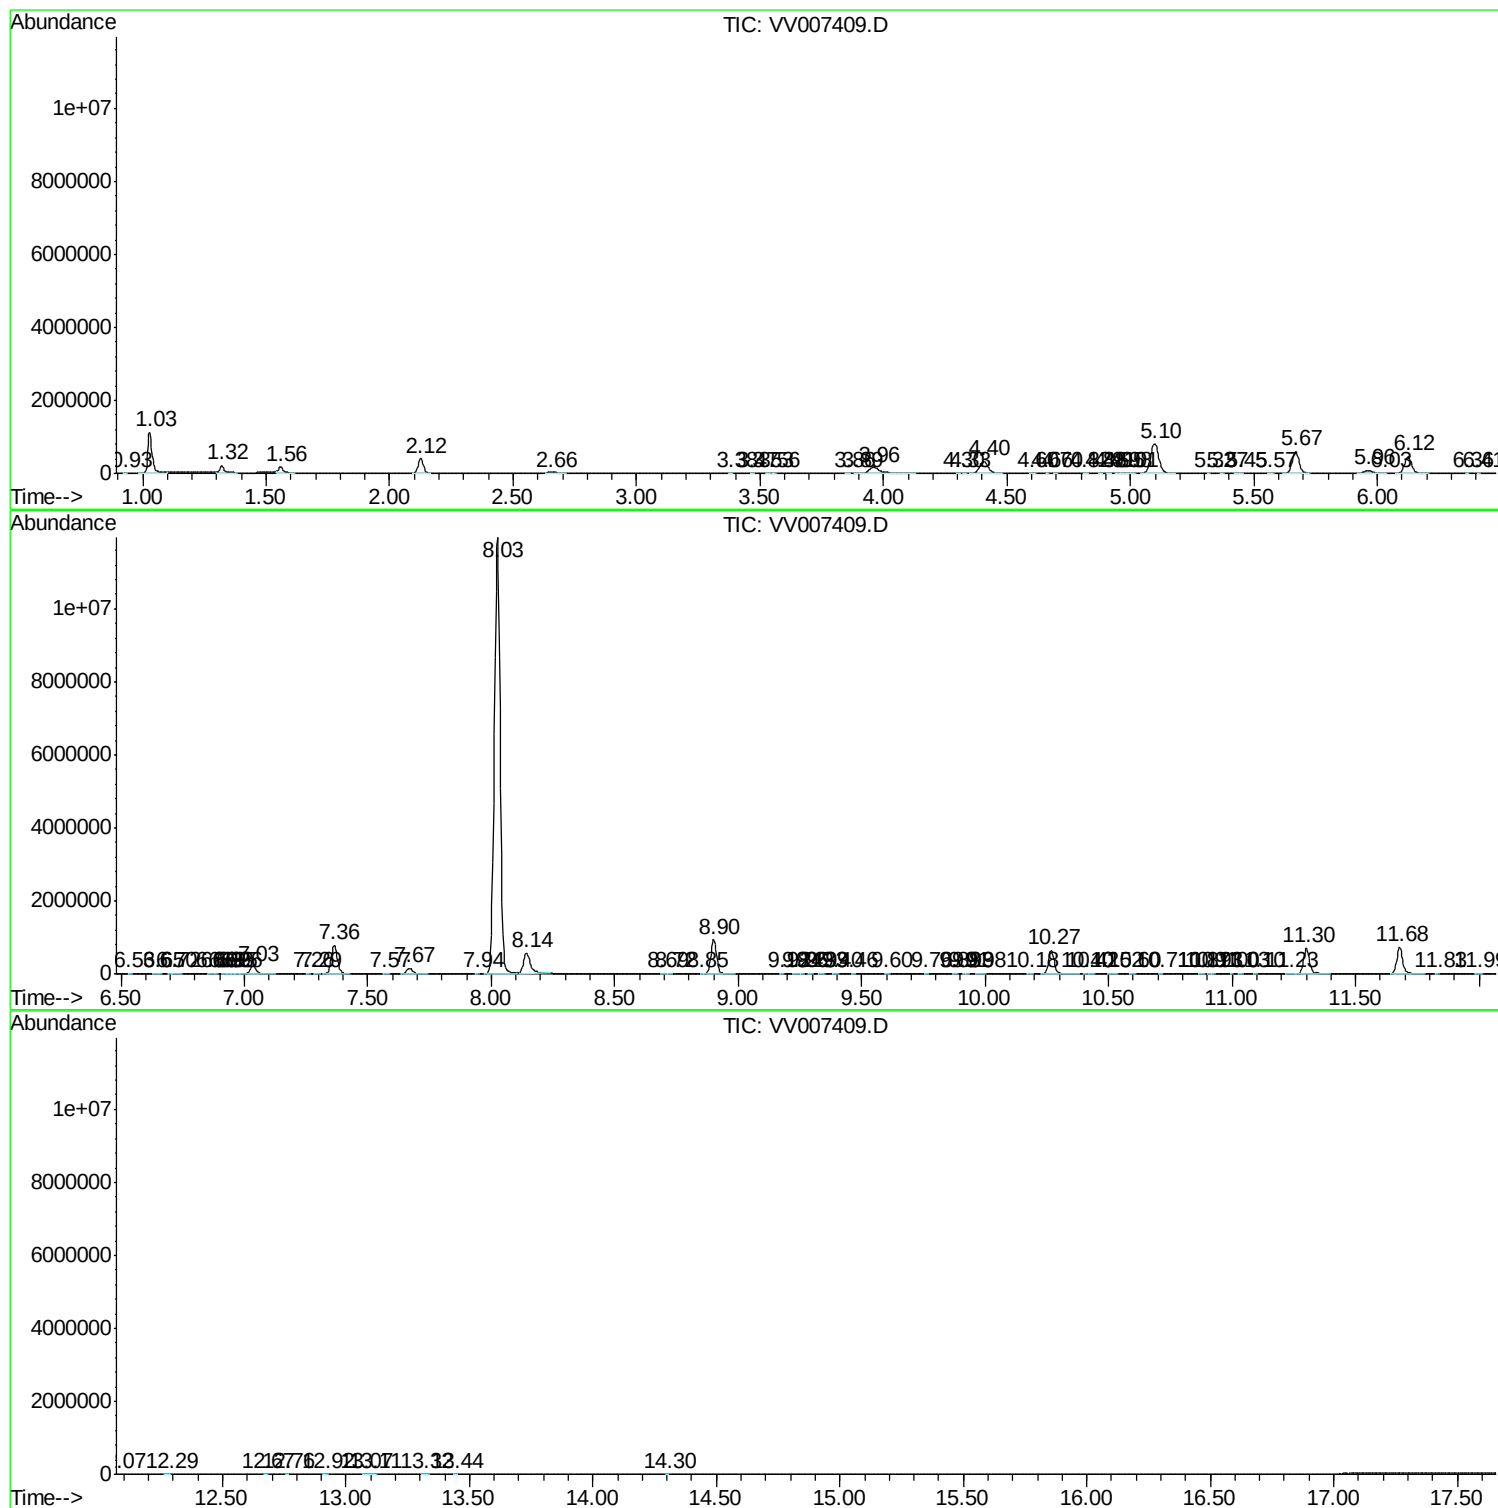

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007409.D
Acq On : 06 Sep 2018 02:13
Operator : SY/MD
Sample : J4751-01 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH2

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007409.D
Acq On : 06 Sep 2018 02:13
Operator : SY/MD
Sample : J4751-01 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH2

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
