

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007410.D
 Acq On : 06 Sep 2018 02:38
 Operator : SY/MD
 Sample : J4751-02 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.935	11	14	16	rBV2	465	351	0.02%	0.002%
2	1.025	29	42	66	rBV	1056101	1323488	71.86%	8.586%
3	1.321	126	134	149	rVB	197142	240265	13.04%	1.559%
4	1.553	201	206	226	rVB	184301	234353	12.72%	1.520%
5	2.125	374	384	396	rBV	366814	519069	28.18%	3.367%
6	2.652	540	548	567	rVB2	27860	61874	3.36%	0.401%
7	3.440	790	793	798	rBV4	554	465	0.03%	0.003%
8	3.640	852	855	857	rBV2	422	302	0.02%	0.002%
9	3.865	922	925	930	rVB2	447	387	0.02%	0.003%
10	3.890	930	933	936	rBV2	307	299	0.02%	0.002%
11	3.961	938	955	997	rBV2	154538	491643	26.69%	3.190%
12	4.405	1073	1093	1120	rBV	315788	761755	41.36%	4.942%
13	4.572	1143	1145	1148	rBV	660	476	0.03%	0.003%
14	4.643	1165	1167	1174	rVB3	650	720	0.04%	0.005%
15	4.726	1191	1193	1196	rVB2	664	360	0.02%	0.002%
16	4.910	1245	1250	1253	rBV2	440	435	0.02%	0.003%
17	4.939	1256	1259	1262	rBV2	612	324	0.02%	0.002%
18	4.990	1271	1275	1278	rBV2	365	352	0.02%	0.002%
19	5.016	1280	1283	1289	rVB	412	453	0.02%	0.003%
20	5.096	1289	1308	1342	rBV2	783474	1841829	100.00%	11.949%
21	5.292	1365	1369	1372	rBV4	567	438	0.02%	0.003%
22	5.334	1378	1382	1385	rBV3	536	433	0.02%	0.003%
23	5.392	1398	1400	1406	rVB3	365	315	0.02%	0.002%
24	5.418	1406	1408	1414	rVB3	535	580	0.03%	0.004%
25	5.447	1414	1417	1418	rBV	587	304	0.02%	0.002%
26	5.472	1423	1425	1428	rBV3	407	337	0.02%	0.002%
27	5.508	1430	1436	1442	rBV4	651	810	0.04%	0.005%
28	5.559	1450	1452	1460	rVB3	649	670	0.04%	0.004%
29	5.668	1469	1486	1511	rBV	561380	1106425	60.07%	7.178%
30	5.955	1563	1575	1591	rVB5	19218	43317	2.35%	0.281%
31	6.122	1612	1627	1646	rBV	444473	887236	48.17%	5.756%
32	6.295	1679	1681	1689	rVB4	1038	780	0.04%	0.005%
33	6.430	1721	1723	1729	rVV3	321	300	0.02%	0.002%
34	6.591	1770	1773	1775	rBV3	477	303	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007410.D
 Acq On : 06 Sep 2018 02:38
 Operator : SY/MD
 Sample : J4751-02 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.649	1784	1791	1795	rBV4	1327	1841	0.10%	0.012%
36	6.723	1806	1814	1822	rBV4	3227	5276	0.29%	0.034%
37	6.784	1830	1833	1836	rBV3	472	328	0.02%	0.002%
38	6.836	1844	1849	1855	rBV3	656	695	0.04%	0.005%
39	6.868	1855	1859	1861	rVV3	577	373	0.02%	0.002%
40	6.900	1865	1869	1871	rBV3	549	375	0.02%	0.002%
41	6.938	1878	1881	1883	rVV3	516	328	0.02%	0.002%
42	6.951	1883	1885	1888	rVB3	525	299	0.02%	0.002%
43	7.035	1897	1911	1929	rBV	189787	342150	18.58%	2.220%
44	7.173	1946	1954	1958	rBV6	945	1281	0.07%	0.008%
45	7.363	1999	2013	2033	rBV	713202	1235936	67.10%	8.018%
46	7.598	2083	2086	2087	rBV3	601	387	0.02%	0.003%
47	7.668	2094	2108	2130	rBV	148237	247406	13.43%	1.605%
48	7.887	2174	2176	2181	rVB	778	479	0.03%	0.003%
49	8.022	2204	2218	2232	rBV	368367	609702	33.10%	3.955%
50	8.144	2243	2256	2298	rBV2	493102	1005106	54.57%	6.521%
51	8.389	2330	2332	2334	rBV	870	561	0.03%	0.004%
52	8.649	2411	2413	2417	rVB2	497	350	0.02%	0.002%
53	8.713	2430	2433	2435	rBV3	598	341	0.02%	0.002%
54	8.729	2435	2438	2443	rVB3	624	587	0.03%	0.004%
55	8.781	2450	2454	2462	rBV3	462	630	0.03%	0.004%
56	8.900	2478	2491	2517	rBV	838242	1345883	73.07%	8.731%
57	9.183	2574	2579	2585	rBV5	876	1036	0.06%	0.007%
58	9.221	2589	2591	2596	rBV4	399	340	0.02%	0.002%
59	9.295	2609	2614	2617	rVB4	462	417	0.02%	0.003%
60	9.324	2617	2623	2628	rBB5	574	585	0.03%	0.004%
61	9.498	2673	2677	2680	rVB3	371	374	0.02%	0.002%
62	9.569	2694	2699	2700	rBV3	389	317	0.02%	0.002%
63	9.896	2796	2801	2804	rBV2	356	479	0.03%	0.003%
64	9.980	2823	2827	2831	rBV4	565	478	0.03%	0.003%
65	10.025	2838	2841	2845	rVB2	527	391	0.02%	0.003%
66	10.083	2856	2859	2864	rBV2	368	412	0.02%	0.003%
67	10.150	2878	2880	2885	rVB	584	441	0.02%	0.003%
68	10.189	2885	2892	2896	rBV5	614	1026	0.06%	0.007%
69	10.215	2896	2900	2903	rVB2	330	299	0.02%	0.002%
70	10.266	2903	2916	2950	rBV	620743	1011274	54.91%	6.561%
71	10.424	2958	2965	2969	rBV3	771	895	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007410.D
 Acq On : 06 Sep 2018 02:38
 Operator : SY/MD
 Sample : J4751-02 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.443	2969	2971	2976	rVB3	524	315	0.02%	0.002%
73	10.633	3026	3030	3033	rBV3	339	317	0.02%	0.002%
74	10.803	3076	3083	3085	rBV3	534	608	0.03%	0.004%
75	10.900	3111	3113	3118	rVB3	755	538	0.03%	0.003%
76	11.035	3151	3155	3160	rBV2	509	403	0.02%	0.003%
77	11.157	3190	3193	3199	rVB3	887	773	0.04%	0.005%
78	11.189	3199	3203	3206	rBV2	713	506	0.03%	0.003%
79	11.221	3211	3213	3217	rBV3	447	330	0.02%	0.002%
80	11.302	3222	3238	3263	rBV	581475	989470	53.72%	6.419%
81	11.678	3343	3355	3377	rVV	632525	1071092	58.15%	6.949%
82	11.797	3389	3392	3394	rBV2	466	323	0.02%	0.002%
83	11.887	3417	3420	3424	rBV2	617	478	0.03%	0.003%
84	12.134	3493	3497	3502	rVB2	749	600	0.03%	0.004%
85	12.157	3502	3504	3508	rBV2	438	374	0.02%	0.002%
86	12.231	3522	3527	3530	rBV3	531	568	0.03%	0.004%
87	12.295	3544	3547	3549	rBV3	482	335	0.02%	0.002%
88	12.350	3559	3564	3567	rBV5	571	508	0.03%	0.003%
89	12.697	3668	3672	3674	rBV3	1097	733	0.04%	0.005%
90	12.723	3678	3680	3684	rBV3	502	292	0.02%	0.002%
91	12.745	3685	3687	3690	rBV2	447	299	0.02%	0.002%
92	12.800	3700	3704	3708	rBV2	637	491	0.03%	0.003%
93	12.935	3743	3746	3749	rBV5	675	448	0.02%	0.003%
94	12.980	3756	3760	3763	rBV4	738	680	0.04%	0.004%
95	13.080	3787	3791	3794	rBV	717	610	0.03%	0.004%
96	13.636	3961	3964	3967	rBV3	993	507	0.03%	0.003%
97	13.703	3983	3985	3988	rVB2	696	335	0.02%	0.002%
98	14.244	4149	4153	4155	rBV4	995	953	0.05%	0.006%
99	14.327	4177	4179	4184	rBV3	797	620	0.03%	0.004%
100	14.443	4213	4215	4216	rBV	913	344	0.02%	0.002%


Sum of corrected areas: 15414376

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090518\
Data File : VV007410.D
Acq On : 06 Sep 2018 02:38
Operator : SY/MD
Sample : J4751-02 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

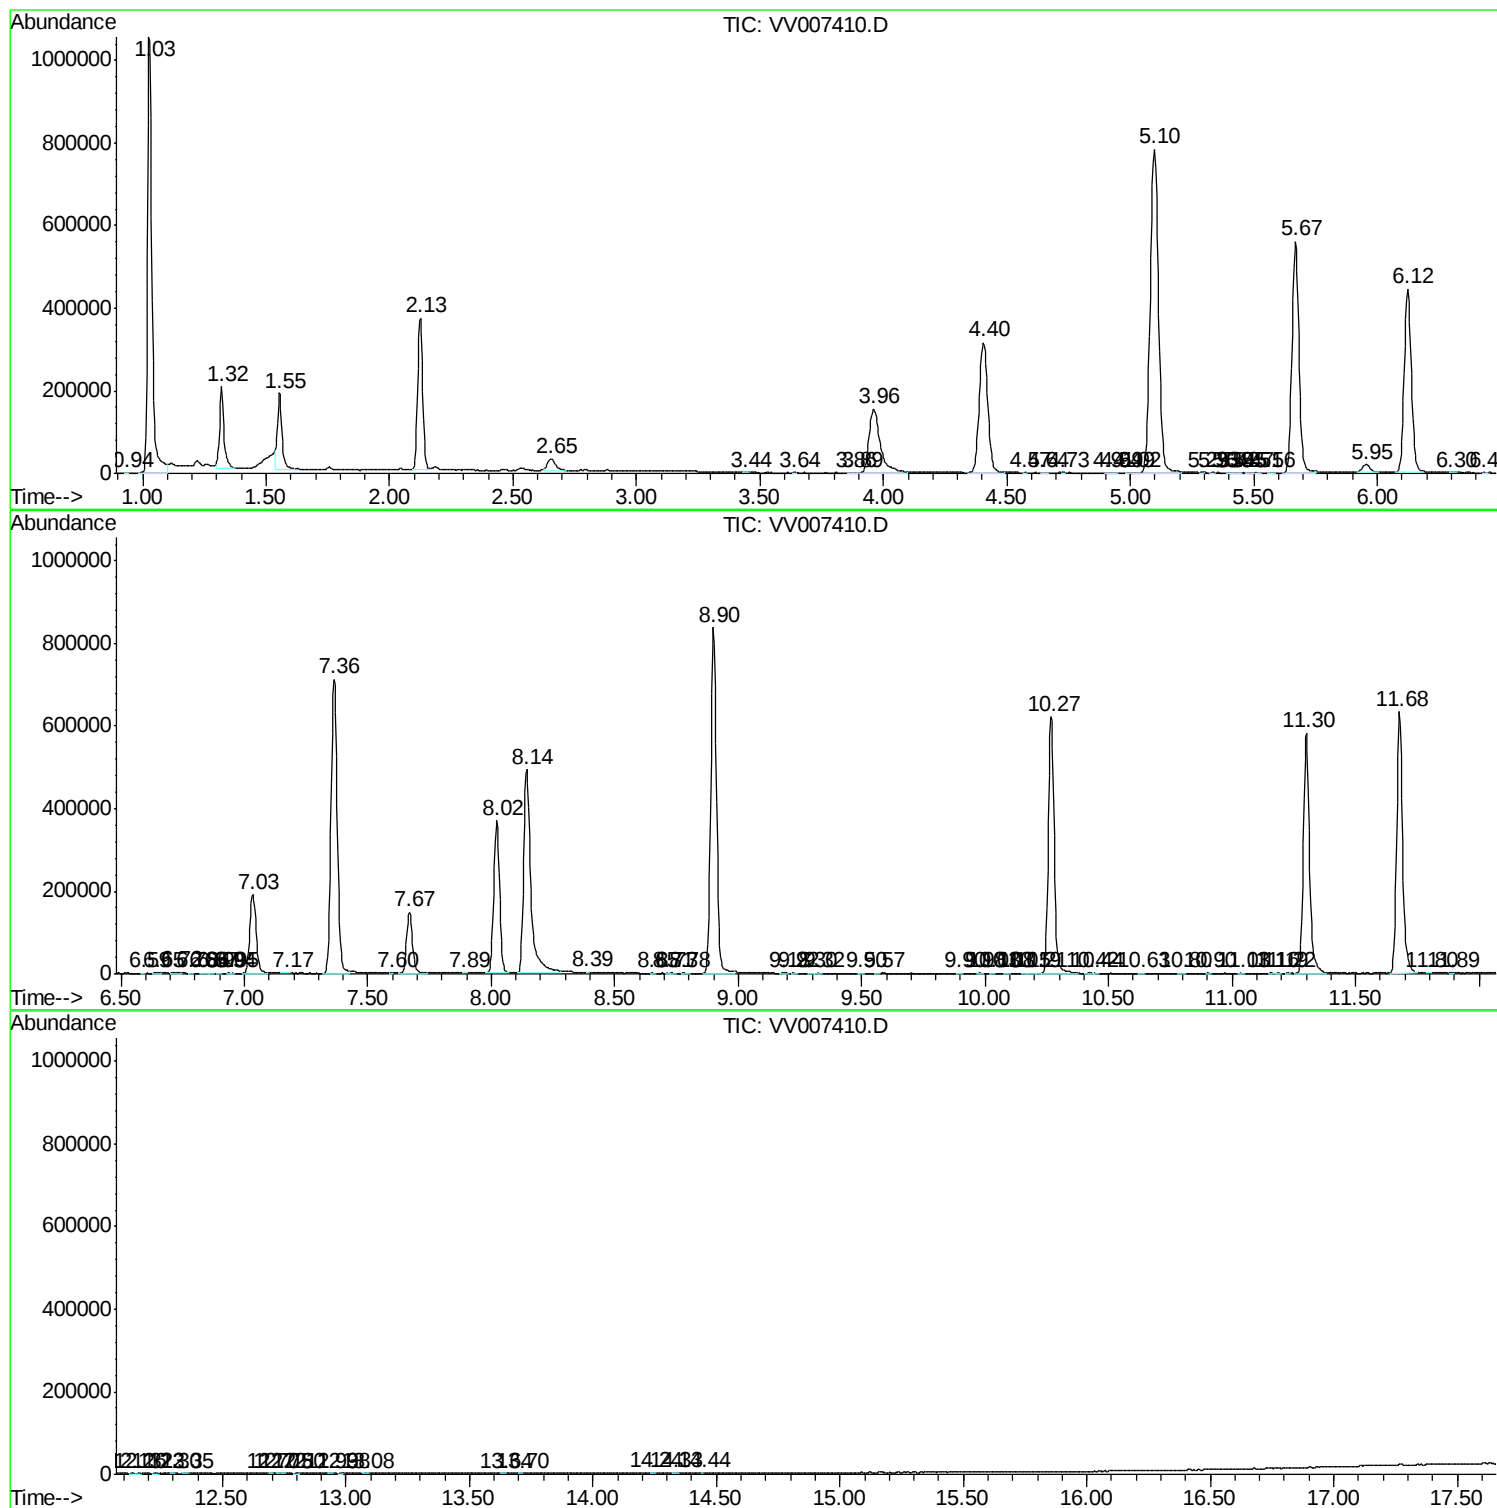

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007410.D
Acq On : 06 Sep 2018 02:38
Operator : SY/MD
Sample : J4751-02 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007410.D
Acq On : 06 Sep 2018 02:38
Operator : SY/MD
Sample : J4751-02 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc