

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007412.D
 Acq On : 06 Sep 2018 03:28
 Operator : SY/MD
 Sample : J4751-04 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	0.942	10	16	20	rBV3	537	733	0.00%	0.002%
2	1.029	27	43	66	rBV	973455	1243513	8.28%	4.154%
3	1.321	126	134	153	rVB	184505	232141	1.55%	0.775%
4	1.556	202	207	225	rVB	181632	222199	1.48%	0.742%
5	2.125	374	384	396	rBV	375116	526578	3.51%	1.759%
6	2.656	540	549	570	rVB2	41086	94510	0.63%	0.316%
7	3.533	819	822	824	rBV2	394	233	0.00%	0.001%
8	3.697	870	873	876	rBV2	296	221	0.00%	0.001%
9	3.768	891	895	899	rVV4	487	490	0.00%	0.002%
10	3.794	899	903	907	rVB2	517	496	0.00%	0.002%
11	3.823	907	912	917	rBV	656	515	0.00%	0.002%
12	3.884	927	931	935	rVB2	445	296	0.00%	0.001%
13	3.958	937	954	1003	rBV2	157103	510115	3.40%	1.704%
14	4.405	1076	1093	1125	rVB	314720	751312	5.00%	2.510%
15	4.906	1246	1249	1252	rBV	263	229	0.00%	0.001%
16	4.926	1252	1255	1260	rVV3	376	381	0.00%	0.001%
17	5.019	1281	1284	1287	rVB2	506	262	0.00%	0.001%
18	5.038	1287	1290	1291	rBV	465	235	0.00%	0.001%
19	5.096	1291	1308	1346	rVV2	778087	1832196	12.20%	6.120%
20	5.315	1374	1376	1379	rBV2	450	290	0.00%	0.001%
21	5.360	1387	1390	1394	rBV2	515	372	0.00%	0.001%
22	5.382	1394	1397	1400	rBV3	429	282	0.00%	0.001%
23	5.498	1431	1433	1436	rBV2	351	245	0.00%	0.001%
24	5.668	1470	1486	1508	rBV	550440	1096327	7.30%	3.662%
25	5.958	1562	1576	1589	rVB6	20173	46787	0.31%	0.156%
26	6.125	1612	1628	1651	rBV	438766	883862	5.89%	2.952%
27	6.347	1694	1697	1701	rBV4	650	539	0.00%	0.002%
28	6.366	1701	1703	1706	rVB2	514	291	0.00%	0.001%
29	6.652	1783	1792	1804	rVB9	1822	3727	0.02%	0.012%
30	6.726	1805	1815	1821	rBV4	2818	5072	0.03%	0.017%
31	6.803	1836	1839	1841	rBV3	306	231	0.00%	0.001%
32	6.871	1855	1860	1864	rVB3	707	814	0.01%	0.003%
33	6.900	1864	1869	1872	rBV3	519	538	0.00%	0.002%
34	6.958	1885	1887	1890	rVB	390	237	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007412.D
 Acq On : 06 Sep 2018 03:28
 Operator : SY/MD
 Sample : J4751-04 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

35	6.987	1892	1896	1898	rBV2	299	215	0.00%	0.001%
36	7.035	1898	1911	1933	rBV	188178	339872	2.26%	1.135%
37	7.221	1967	1969	1974	rBV4	439	340	0.00%	0.001%
38	7.241	1974	1975	1979	rVB3	679	301	0.00%	0.001%
39	7.270	1982	1984	1986	rBV3	410	197	0.00%	0.001%
40	7.286	1986	1989	1995	rVB4	767	735	0.00%	0.002%
41	7.363	1999	2013	2034	rBV	723023	1251157	8.33%	4.179%
42	7.543	2067	2069	2072	rBV3	495	340	0.00%	0.001%
43	7.668	2094	2108	2133	rBV	143000	244805	1.63%	0.818%
44	7.829	2155	2158	2164	rBV5	473	524	0.00%	0.002%
45	7.971	2200	2202	2203	rBV2	654	295	0.00%	0.001%
46	8.022	2203	2218	2244	rVV	9026774	15016388	100.00%	50.160%
47	8.141	2245	2255	2292	rVB2	523920	1068557	7.12%	3.569%
48	8.488	2361	2363	2370	rBV7	607	650	0.00%	0.002%
49	8.742	2440	2442	2444	rBV	604	286	0.00%	0.001%
50	8.768	2448	2450	2453	rBV2	377	272	0.00%	0.001%
51	8.835	2468	2471	2474	rBV4	536	405	0.00%	0.001%
52	8.900	2478	2491	2525	rVV	843172	1376056	9.16%	4.597%
53	9.218	2584	2590	2593	rBV4	451	455	0.00%	0.002%
54	9.385	2640	2642	2645	rBV2	408	197	0.00%	0.001%
55	9.453	2660	2663	2666	rBV2	420	248	0.00%	0.001%
56	9.491	2672	2675	2678	rVB4	691	426	0.00%	0.001%
57	9.514	2678	2682	2684	rVB2	572	329	0.00%	0.001%
58	9.533	2684	2688	2689	rBV2	642	365	0.00%	0.001%
59	9.581	2700	2703	2705	rBV2	582	401	0.00%	0.001%
60	9.620	2712	2715	2721	rVB4	585	553	0.00%	0.002%
61	9.652	2721	2725	2729	rBV	708	679	0.00%	0.002%
62	9.713	2741	2744	2745	rBV2	313	214	0.00%	0.001%
63	9.758	2756	2758	2763	rBV3	388	408	0.00%	0.001%
64	9.813	2772	2775	2781	rBV3	317	274	0.00%	0.001%
65	9.851	2785	2787	2790	rBV2	396	282	0.00%	0.001%
66	10.038	2843	2845	2852	rVB4	376	334	0.00%	0.001%
67	10.115	2867	2869	2872	rBV2	344	212	0.00%	0.001%
68	10.173	2883	2887	2889	rBV2	292	262	0.00%	0.001%
69	10.186	2889	2891	2898	rVB4	712	681	0.00%	0.002%
70	10.218	2898	2901	2904	rBV2	517	419	0.00%	0.001%
71	10.266	2904	2916	2952	rVB	619316	1009572	6.72%	3.372%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV090518\
 Data File : VV007412.D
 Acq On : 06 Sep 2018 03:28
 Operator : SY/MD
 Sample : J4751-04 50X
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BEGH5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
 Title : VOC Analysis

72	10.398	2954	2957	2960	rBV2	386	234	0.00%	0.001%
73	10.671	3039	3042	3045	rBV3	424	240	0.00%	0.001%
74	10.694	3045	3049	3051	rVV2	468	339	0.00%	0.001%
75	10.707	3051	3053	3059	rVV4	474	535	0.00%	0.002%
76	10.732	3059	3061	3065	rVB3	651	419	0.00%	0.001%
77	10.909	3112	3116	3120	rBV3	891	837	0.01%	0.003%
78	11.173	3195	3198	3200	rBV2	422	245	0.00%	0.001%
79	11.257	3221	3224	3225	rBV2	551	290	0.00%	0.001%
80	11.302	3225	3238	3264	rVV	610914	1034948	6.89%	3.457%
81	11.421	3271	3275	3277	rBV3	722	554	0.00%	0.002%
82	11.495	3295	3298	3301	rBV	770	421	0.00%	0.001%
83	11.511	3301	3303	3306	rBV3	536	366	0.00%	0.001%
84	11.597	3328	3330	3335	rBV3	369	283	0.00%	0.001%
85	11.678	3342	3355	3379	rBV	641783	1115199	7.43%	3.725%
86	12.166	3505	3507	3510	rBV3	503	308	0.00%	0.001%
87	12.244	3528	3531	3533	rBV	476	318	0.00%	0.001%
88	12.257	3533	3535	3539	rVV2	790	439	0.00%	0.001%
89	12.469	3599	3601	3603	rVB2	524	235	0.00%	0.001%
90	12.559	3626	3629	3630	rBV2	484	298	0.00%	0.001%
91	12.697	3668	3672	3676	rBV2	664	510	0.00%	0.002%
92	12.716	3676	3678	3682	rBV2	398	293	0.00%	0.001%
93	12.806	3704	3706	3707	rBV2	579	276	0.00%	0.001%
94	12.929	3740	3744	3747	rBV4	778	766	0.01%	0.003%
95	13.064	3784	3786	3789	rBV3	432	233	0.00%	0.001%
96	13.607	3953	3955	3963	rVB3	743	799	0.01%	0.003%
97	13.694	3980	3982	3985	rBV3	622	451	0.00%	0.002%
98	13.867	4034	4036	4039	rVB2	813	440	0.00%	0.001%
99	14.266	4156	4160	4167	rBV5	1355	2024	0.01%	0.007%
100	14.697	4291	4294	4295	rBV2	962	520	0.00%	0.002%


Sum of corrected areas: 29936795

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV090518\
Data File : VV007412.D
Acq On : 06 Sep 2018 03:28
Operator : SY/MD
Sample : J4751-04 50X
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

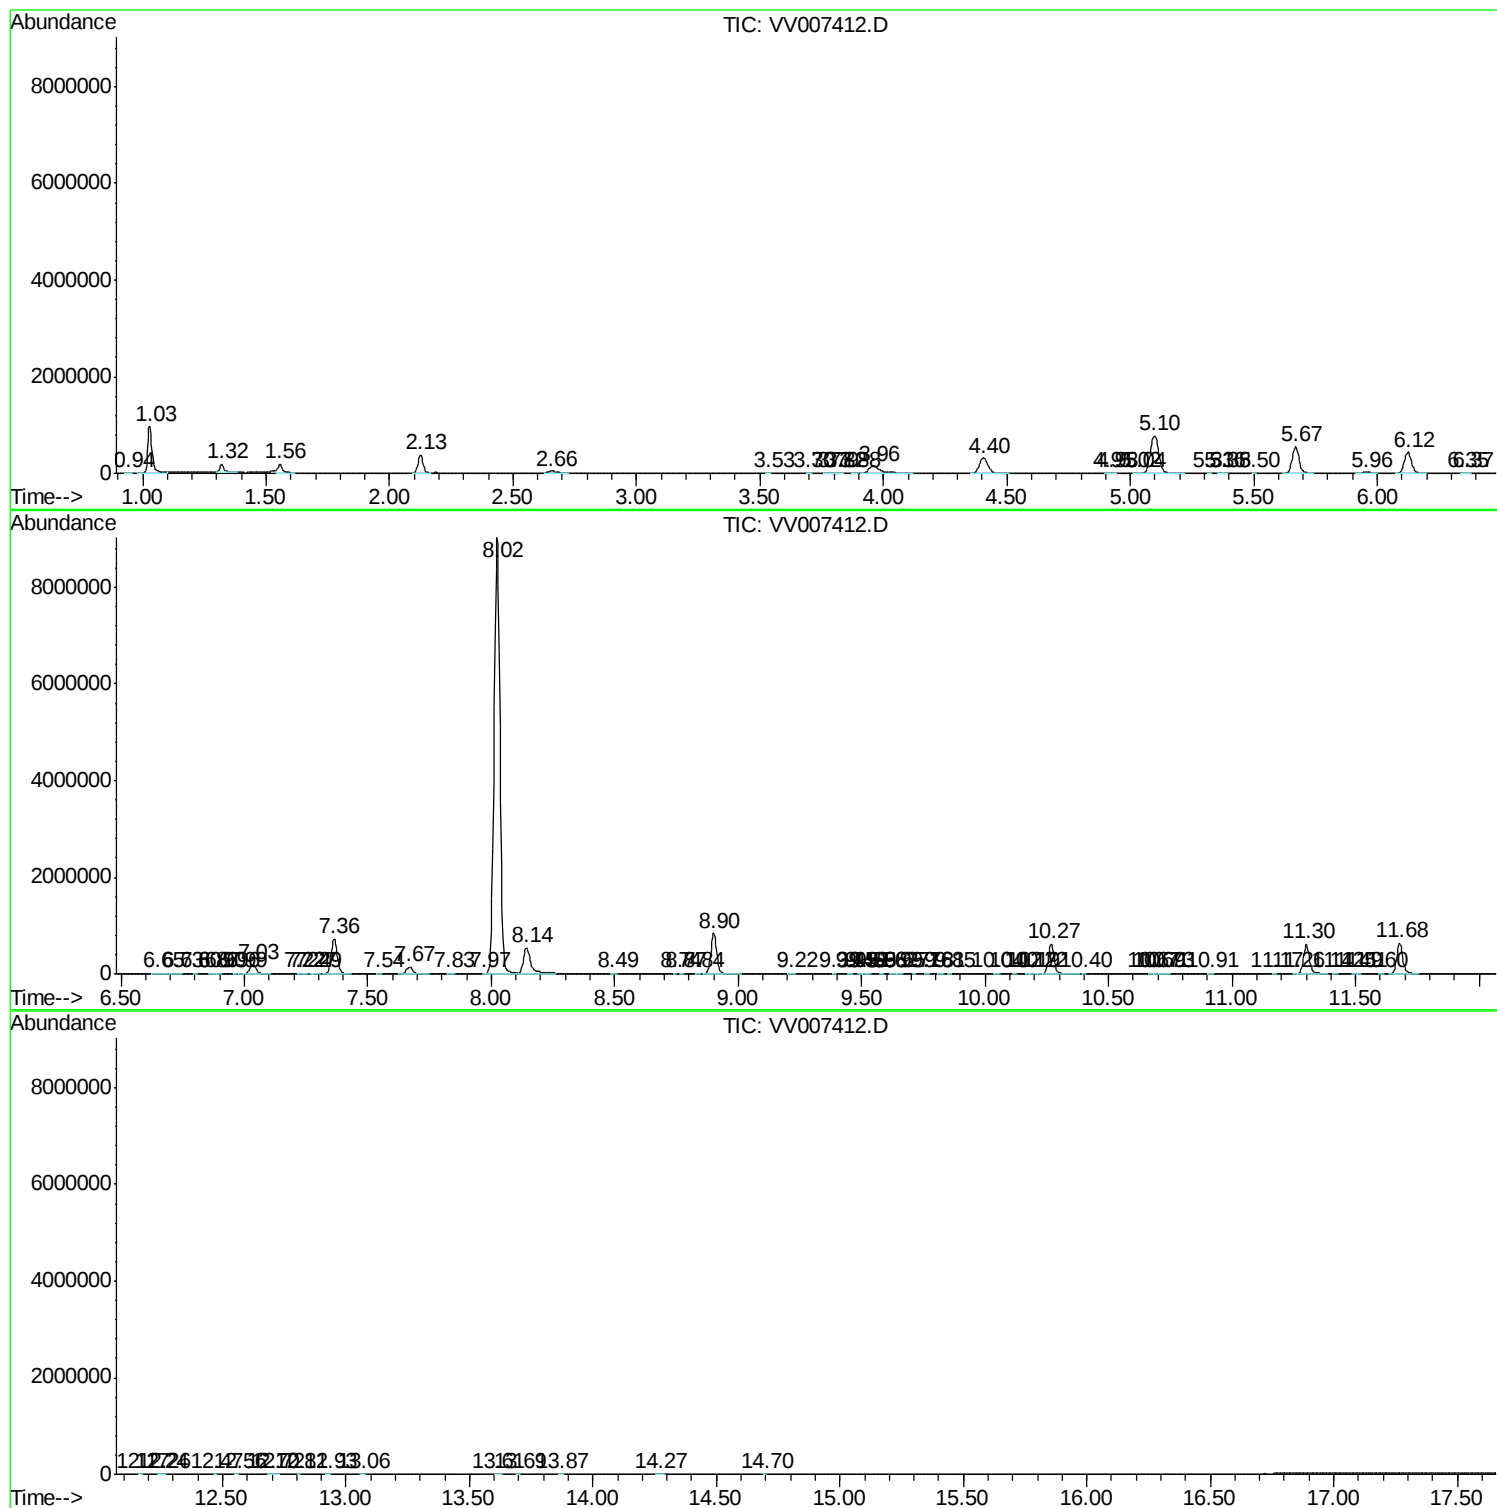

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007412.D
Acq On : 06 Sep 2018 03:28
Operator : SY/MD
Sample : J4751-04 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH5

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV090518\
Data File : VV007412.D
Acq On : 06 Sep 2018 03:28
Operator : SY/MD
Sample : J4751-04 50X
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BEGH5

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM090418WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc